

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101818\
 Data File : P0050212.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Oct 2018 20:26
 Operator : SM/SJ
 Sample : J5518-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 GSTS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 02:12:37 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101818.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 19 02:02:26 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.352	3.359	3249530	2072793	10.890	10.543
2) SA Decachlor...	10.084	8.114	1578506	1541135	7.275	8.063

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101818\
Data File : PO050212.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Oct 2018 20:26
Operator : SM/SJ
Sample : J5518-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
GSTS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 02:12:37 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101818.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 19 02:02:26 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

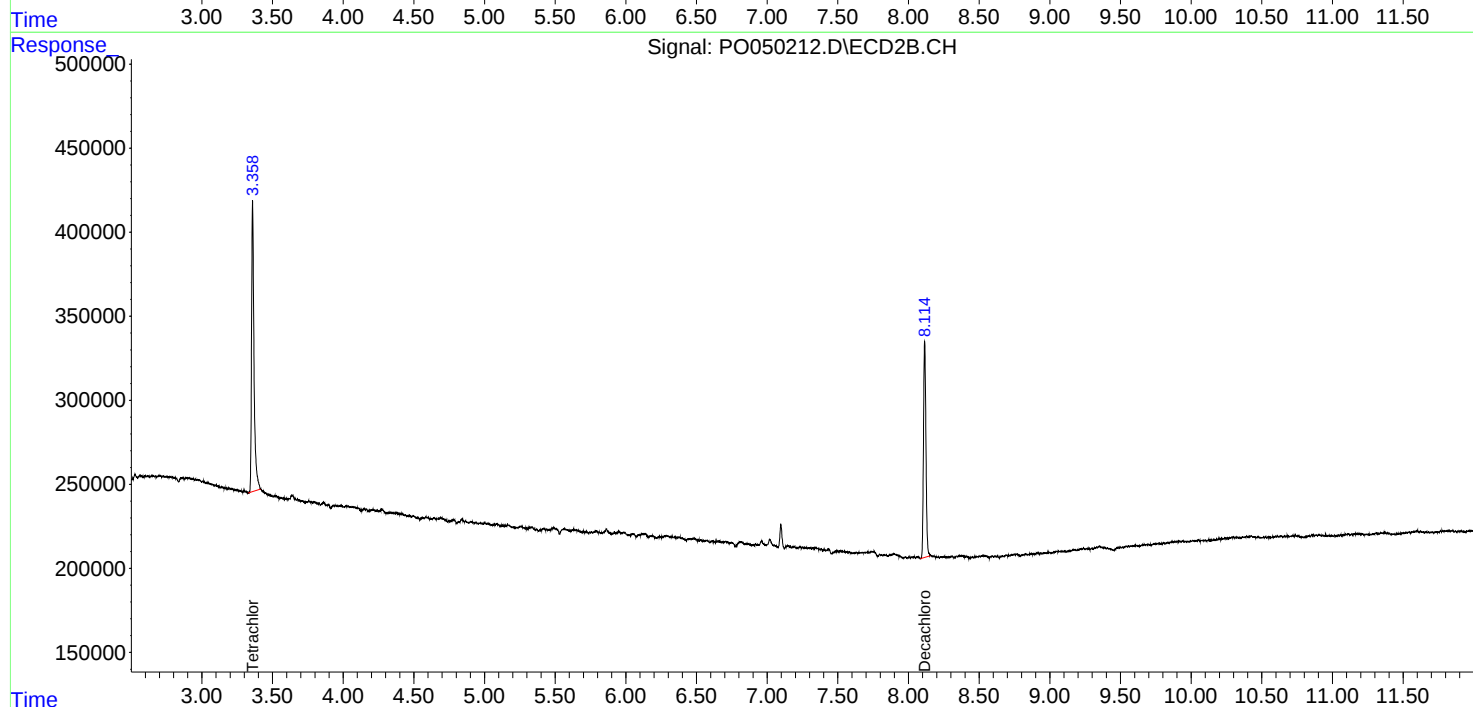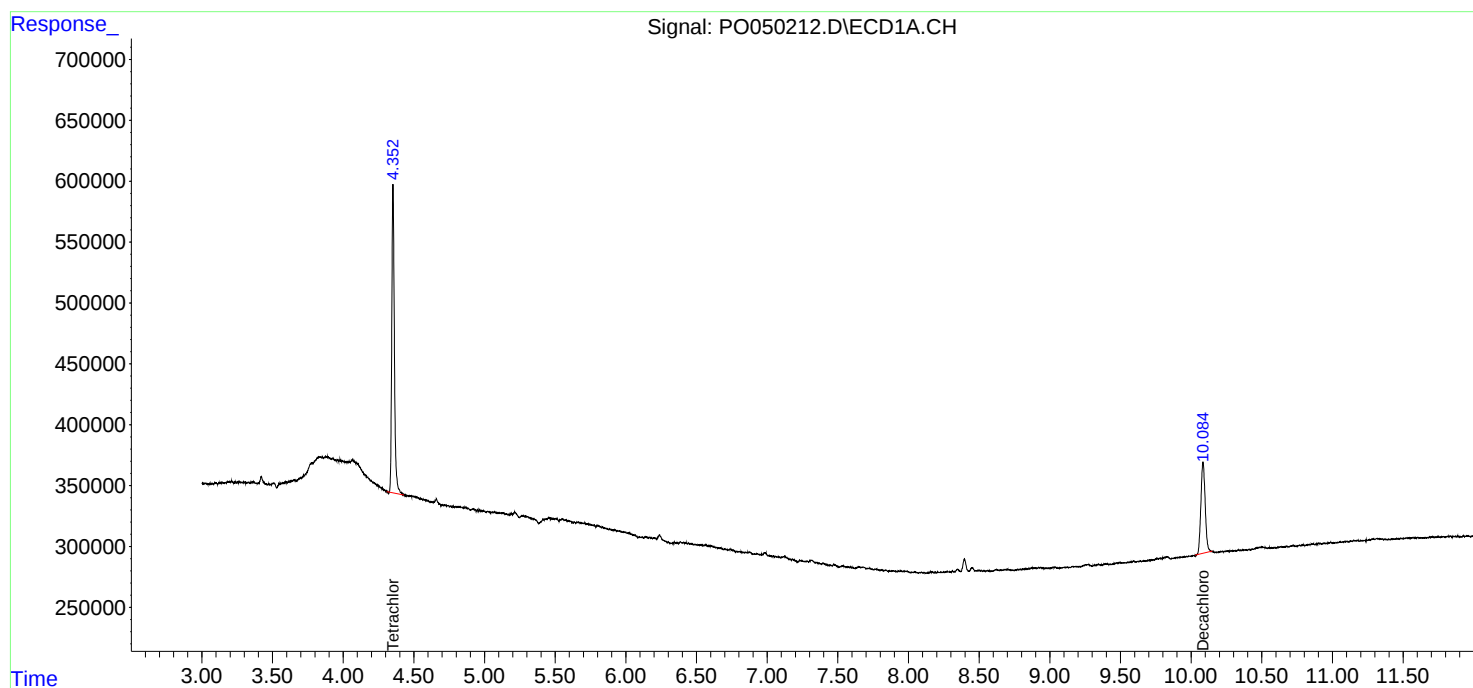


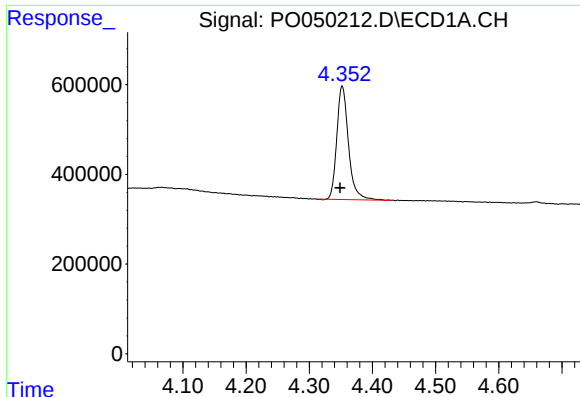

#1 Tetrachloro-m-xylene


R.T.: 4.352 min
Delta R.T.: 0.003 min
Response: 3249530
Conc: 10.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
GSTS

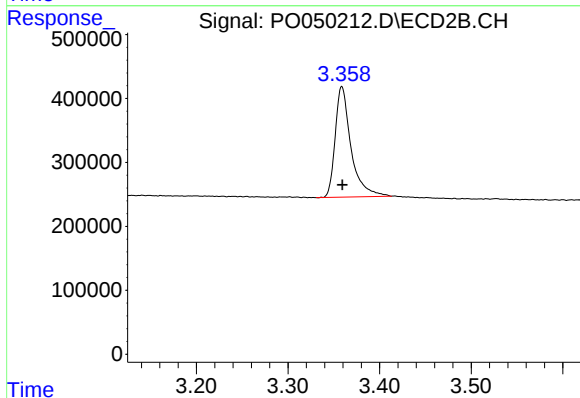


#1 Tetrachloro-m-xylene

R.T.: 3.359 min
Delta R.T.: 0.000 min
Response: 2072793
Conc: 10.54 ng/ml

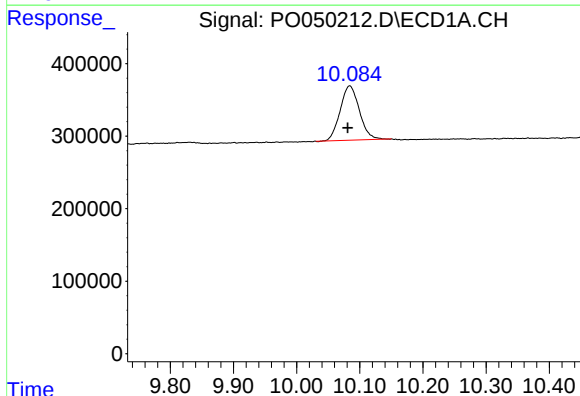

#2 Decachlorobiphenyl

R.T.: 10.084 min
Delta R.T.: 0.003 min
Response: 1578506
Conc: 7.27 ng/ml

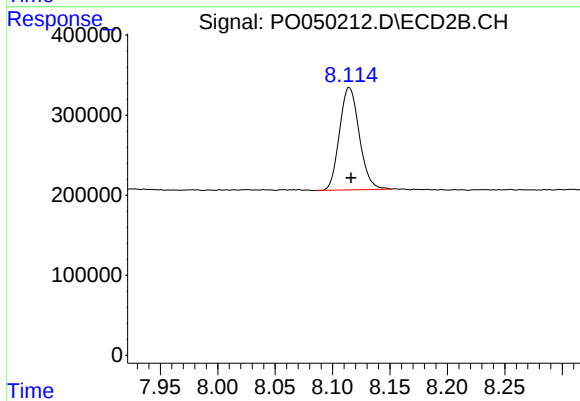

#2 Decachlorobiphenyl

R.T.: 8.114 min
Delta R.T.: -0.002 min
Response: 1541135
Conc: 8.06 ng/ml