

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101818\
 Data File : P0050221.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Oct 2018 23:16
 Operator : SM/SJ
 Sample : J5573-03
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 0692-KM-CA-AMD-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 02:14:54 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101818.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 19 02:02:26 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.354	3.360	6173255	4546543	20.688	23.126
2) SA Decachlor...	10.084	8.115	2574319	2223415	11.864	11.632

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101818\
Data File : PO050221.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Oct 2018 23:16
Operator : SM/SJ
Sample : J5573-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
0692-KM-CA-AMD-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 02:14:54 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101818.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 19 02:02:26 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

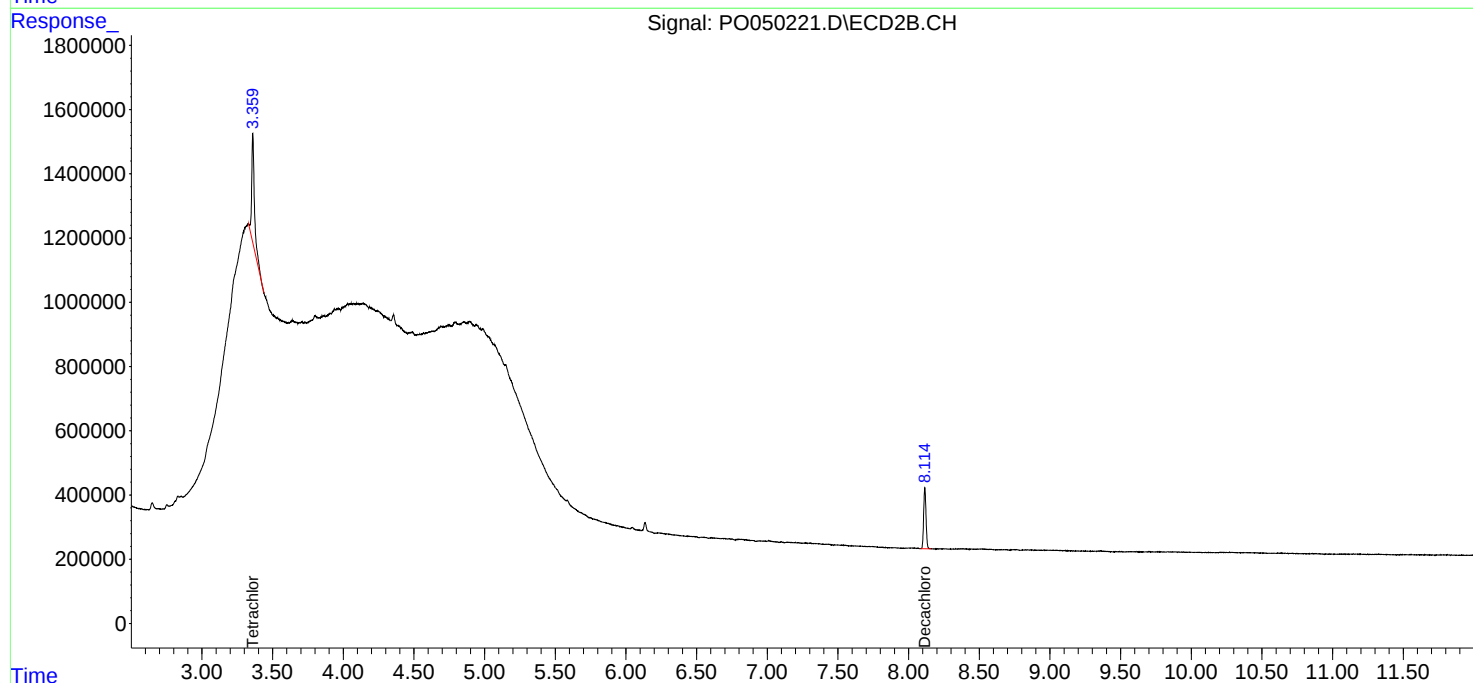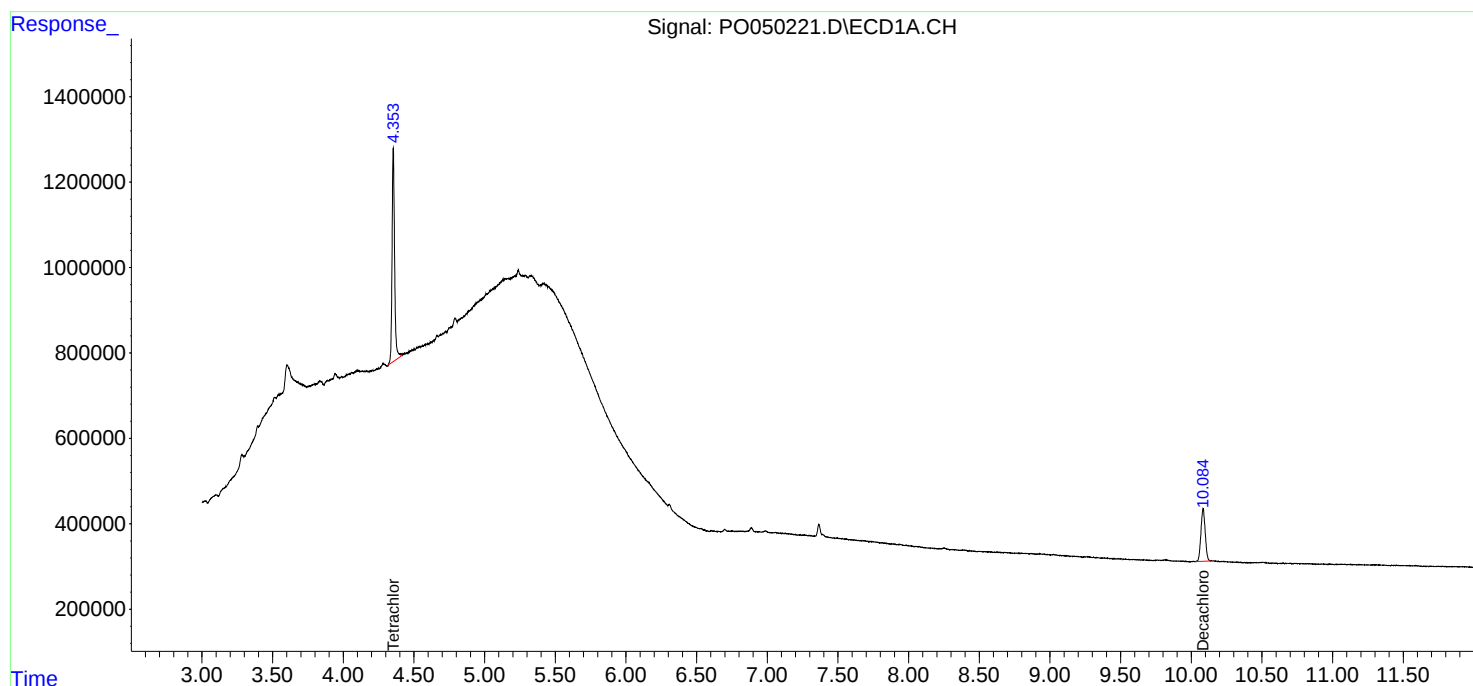


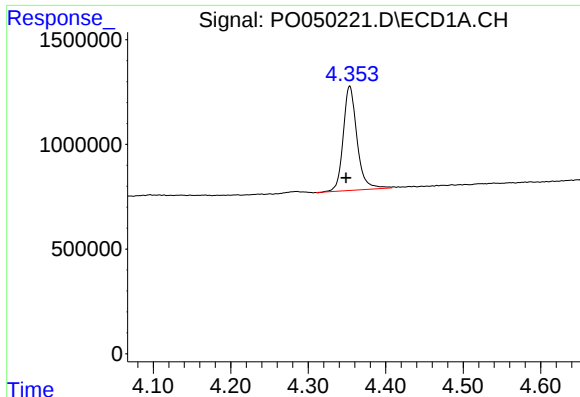

#1 Tetrachloro-m-xylene


R.T.: 4.354 min
Delta R.T.: 0.005 min
Response: 6173255
Conc: 20.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
0692-KM-CA-AMD-COMP

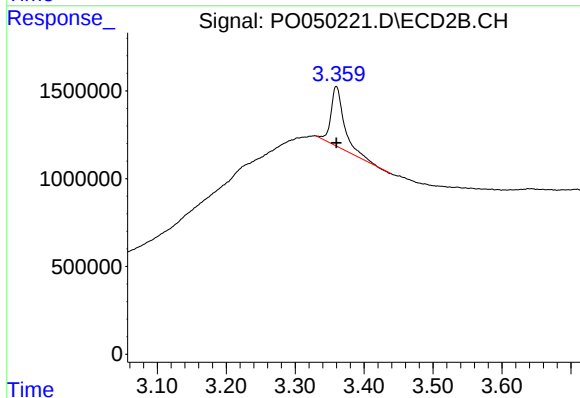


#1 Tetrachloro-m-xylene

R.T.: 3.360 min
Delta R.T.: 0.000 min
Response: 4546543
Conc: 23.13 ng/ml

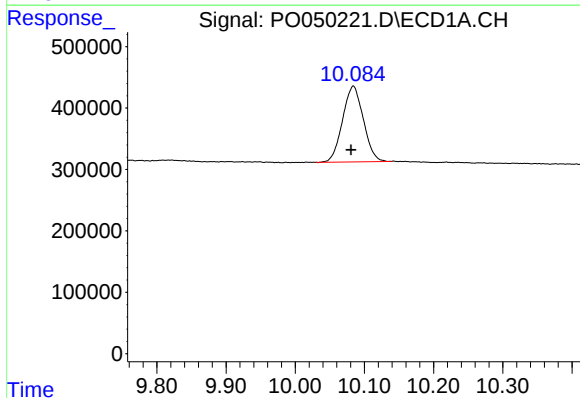

#2 Decachlorobiphenyl

R.T.: 10.084 min
Delta R.T.: 0.003 min
Response: 2574319
Conc: 11.86 ng/ml

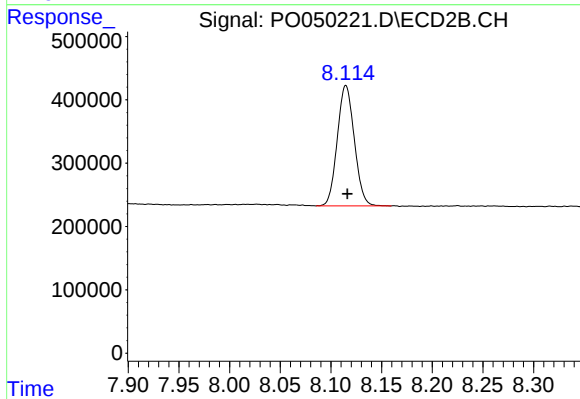

#2 Decachlorobiphenyl

R.T.: 8.115 min
Delta R.T.: -0.001 min
Response: 2223415
Conc: 11.63 ng/ml