

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101819\
 Data File : P0062139.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Oct 2019 12:48
 Operator : HP/AJ
 Sample : K5111-07
 Misc : AR1232 LOD 40 PPB
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2019

Manual Integrations
 APPROVED

Ankita
 10/21/2019 5:01:43 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 02:45:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.323	3.482	878794	641089	14.209	14.950
2)	SA Decachlor...	9.955	8.335	897872	479456	16.047	16.341
Target Compounds							
11)	L3 AR-1232-1	4.694	3.844	74067	55486	33.912	35.808
12)	L3 AR-1232-2	5.219	4.544	36414	60186	30.520m	34.861
13)	L3 AR-1232-3	5.507	4.713	80402	29860	31.429	32.668m
14)	L3 AR-1232-4	5.667	4.795	40907	22709	31.822m	27.914m
15)	L3 AR-1232-5	5.754	4.961	30885	42109	31.205m	47.680m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101819\
Data File : PO062139.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Oct 2019 12:48
Operator : HP/AJ
Sample : K5111-07
Misc : AR1232 LOD 40 PPB
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2019


Manual Integrations
APPROVED

Ankita
10/21/2019 5:01:43 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 02:45:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

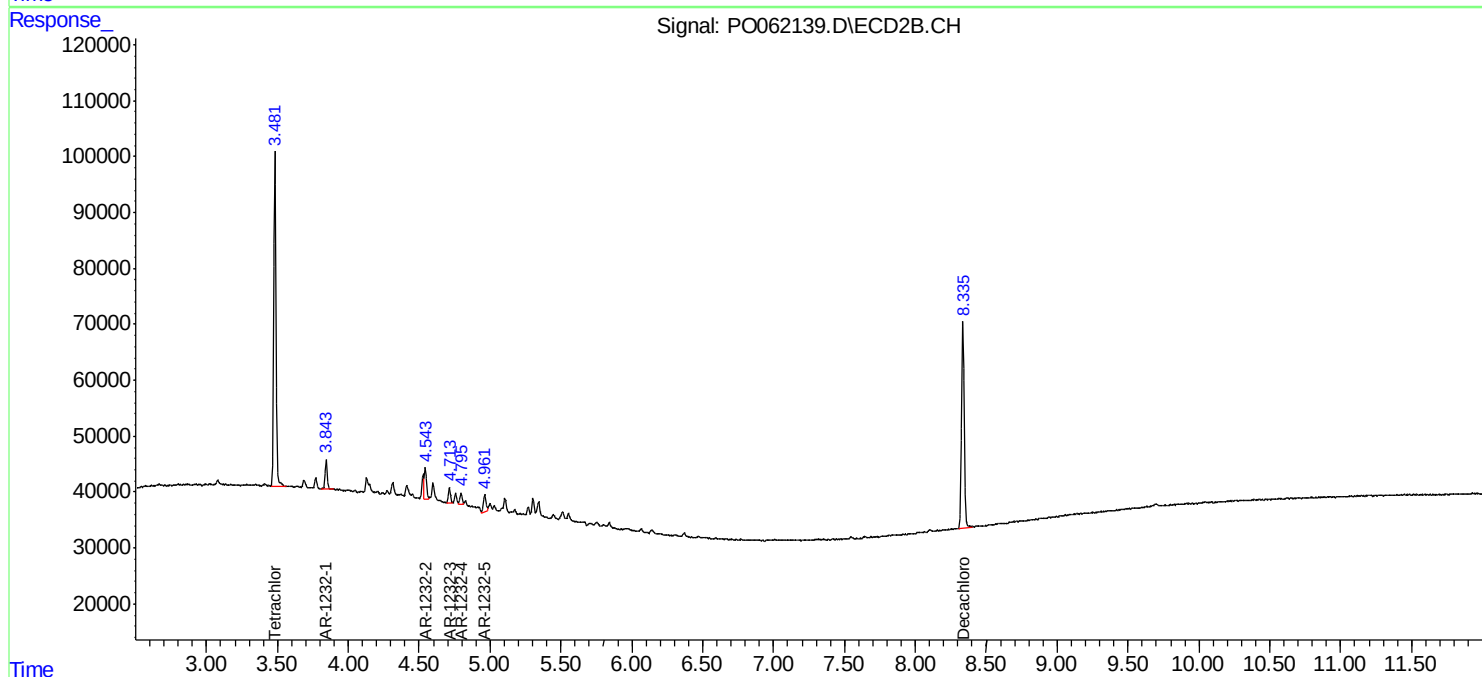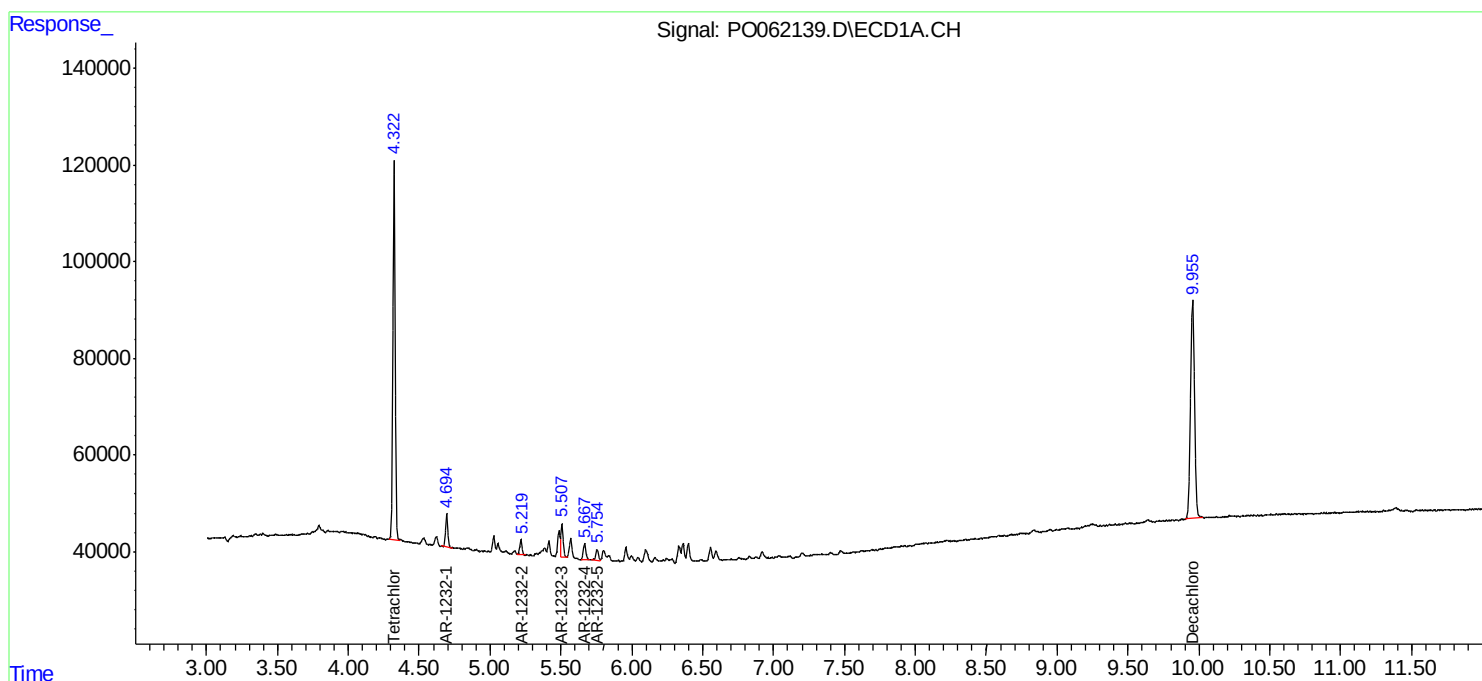

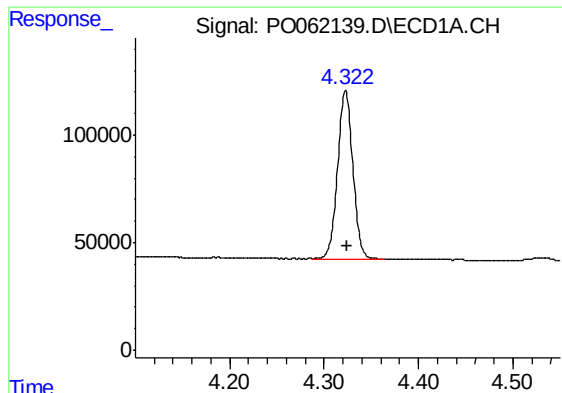


#1 Tetrachloro-m-xylene

R.T.: 4.323 min
Delta R.T.: -0.002 min
Response: 878794
Conc: 14.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2019


Manual Integrations
APPROVED

Ankita
10/21/2019 5:01:43 PM

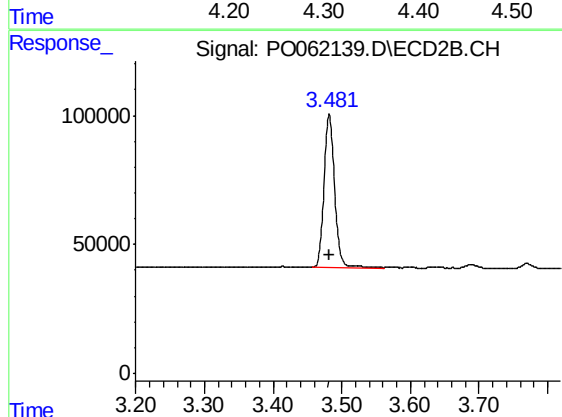


#1 Tetrachloro-m-xylene

R.T.: 3.482 min
Delta R.T.: 0.000 min
Response: 641089
Conc: 14.95 ng/ml

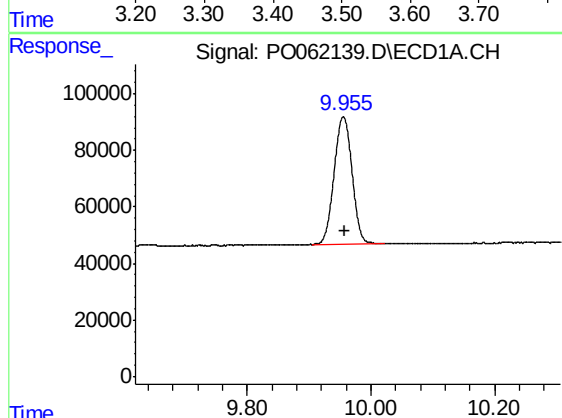


#2 Decachlorobiphenyl

R.T.: 9.955 min
Delta R.T.: -0.001 min
Response: 897872
Conc: 16.05 ng/ml

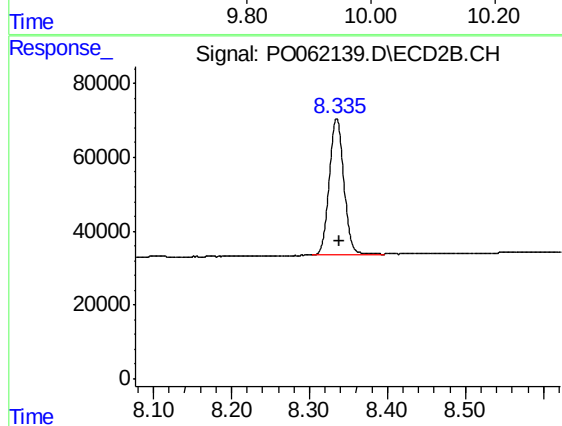

#2 Decachlorobiphenyl

R.T.: 8.335 min
Delta R.T.: -0.003 min
Response: 479456
Conc: 16.34 ng/ml

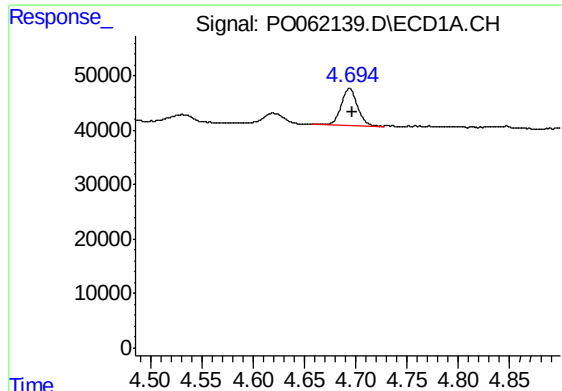


#11 AR-1232-1

R.T.: 4.694 min
Delta R.T.: -0.002 min
Response: 74067
Conc: 33.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2019


Manual Integrations
APPROVED

Ankita
10/21/2019 5:01:43 PM

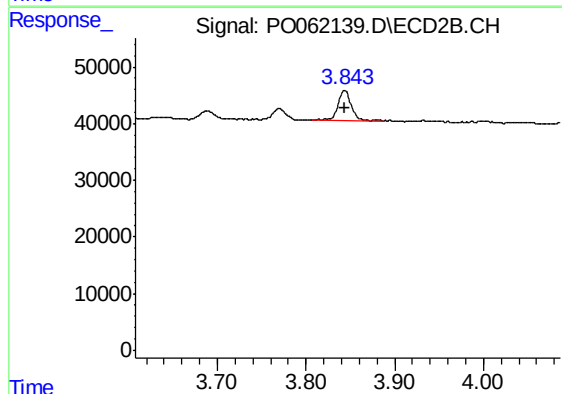


#11 AR-1232-1

R.T.: 3.844 min
Delta R.T.: 0.000 min
Response: 55486
Conc: 35.81 ng/ml

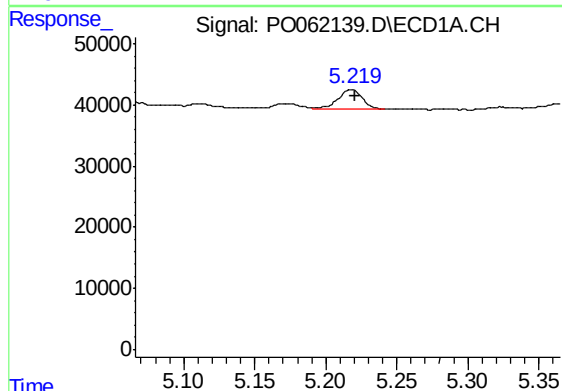


#12 AR-1232-2

R.T.: 5.219 min
Delta R.T.: -0.002 min
Response: 36414
Conc: 30.52 ng/ml m

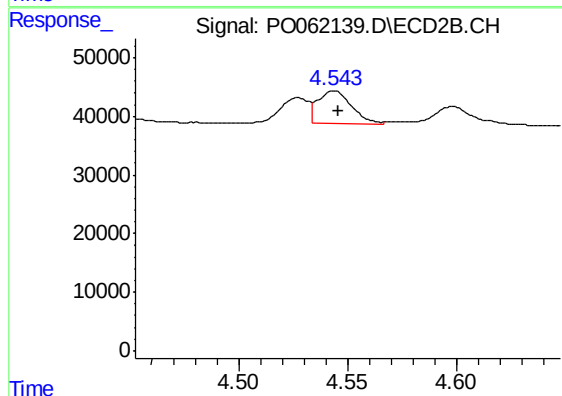

#12 AR-1232-2

R.T.: 4.544 min
Delta R.T.: -0.002 min
Response: 60186
Conc: 34.86 ng/ml

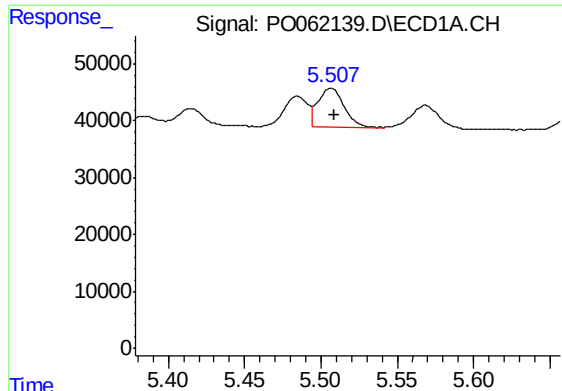


#13 AR-1232-3

R.T.: 5.507 min
Delta R.T.: -0.002 min
Response: 80402
Conc: 31.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2019


Manual Integrations
APPROVED

Ankita
10/21/2019 5:01:43 PM

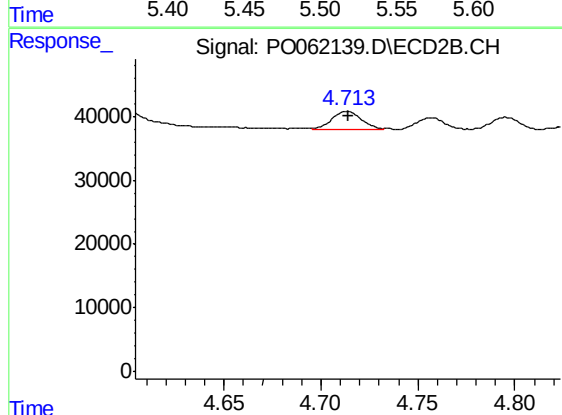


#13 AR-1232-3

R.T.: 4.713 min
Delta R.T.: -0.002 min
Response: 29860
Conc: 32.67 ng/ml m

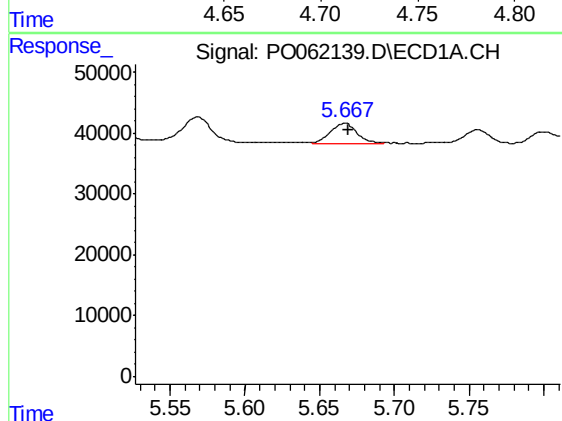


#14 AR-1232-4

R.T.: 5.667 min
Delta R.T.: -0.002 min
Response: 40907
Conc: 31.82 ng/ml m

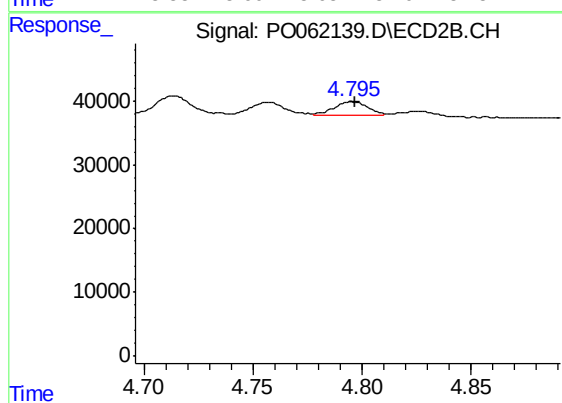

#14 AR-1232-4

R.T.: 4.795 min
Delta R.T.: -0.002 min
Response: 22709
Conc: 27.91 ng/ml m

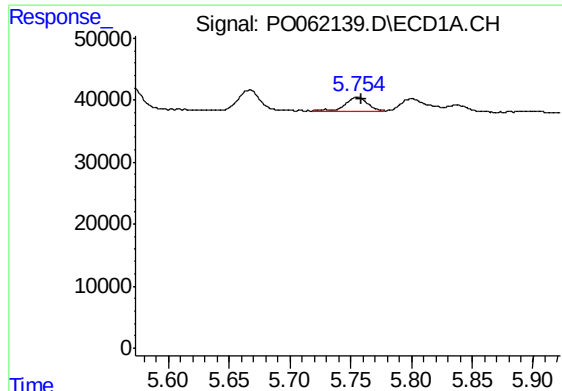


#15 AR-1232-5

R.T.: 5.754 min
Delta R.T.: -0.004 min
Response: 30885
Conc: 31.21 ng/ml m

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2019

Manual Integrations
APPROVED

Ankita
10/21/2019 5:01:43 PM

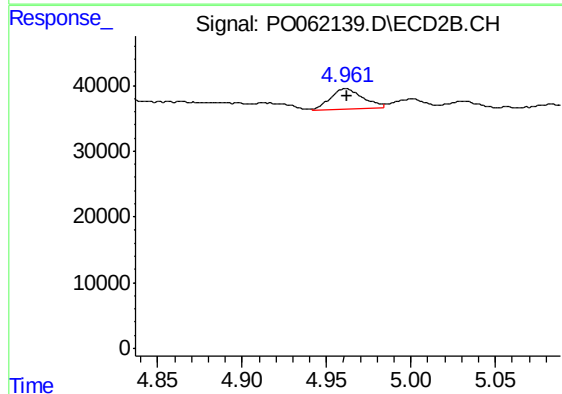

#15 AR-1232-5

R.T.: 4.961 min
Delta R.T.: -0.002 min
Response: 42109
Conc: 47.68 ng/ml m