

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101819\
 Data File : P0062141.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Oct 2019 13:21
 Operator : HP/AJ
 Sample : K5111-07
 Misc : AR1248 LOD 40 PPB
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2019

Manual Integrations
 APPROVED

Ankita
 10/21/2019 5:01:46 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 02:46:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.323	3.482	925070	671012	14.957	15.648
2)	SA Decachlor...	9.953	8.334	920471	491202	16.451	16.741
Target Compounds							
21)	L5 AR-1248-1	5.485	4.527	52946	38115	36.941	38.824m
22)	L5 AR-1248-2	5.755	4.755	69333	48719	34.630	38.455m
23)	L5 AR-1248-3	5.956	4.794	79036	46440	35.786m	34.984m
24)	L5 AR-1248-4	6.360	4.961	108809	69444	42.592	43.886
25)	L5 AR-1248-5	6.398	5.342	97458	53889	39.858	35.015

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101819\
Data File : PO062141.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Oct 2019 13:21
Operator : HP/AJ
Sample : K5111-07
Misc : AR1248 LOD 40 PPB
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2019


Manual Integrations
APPROVED

Ankita
10/21/2019 5:01:46 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 02:46:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

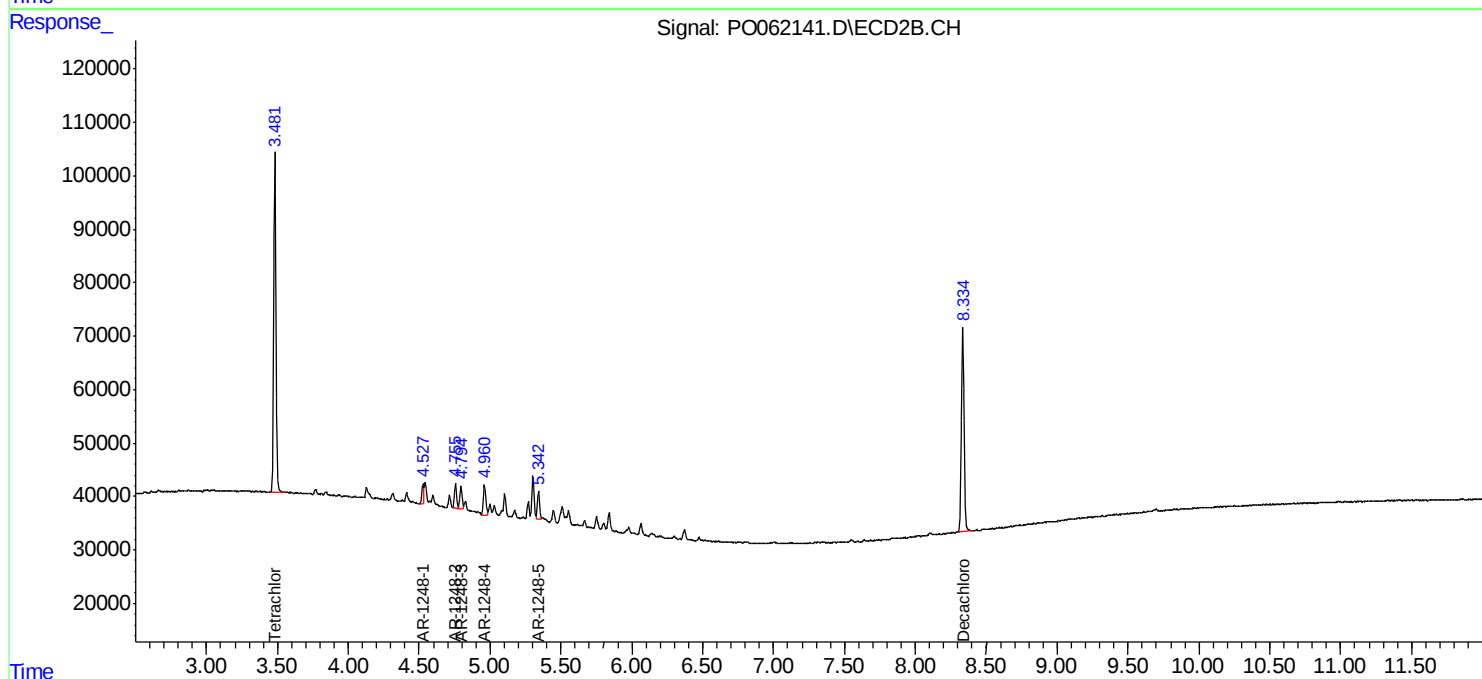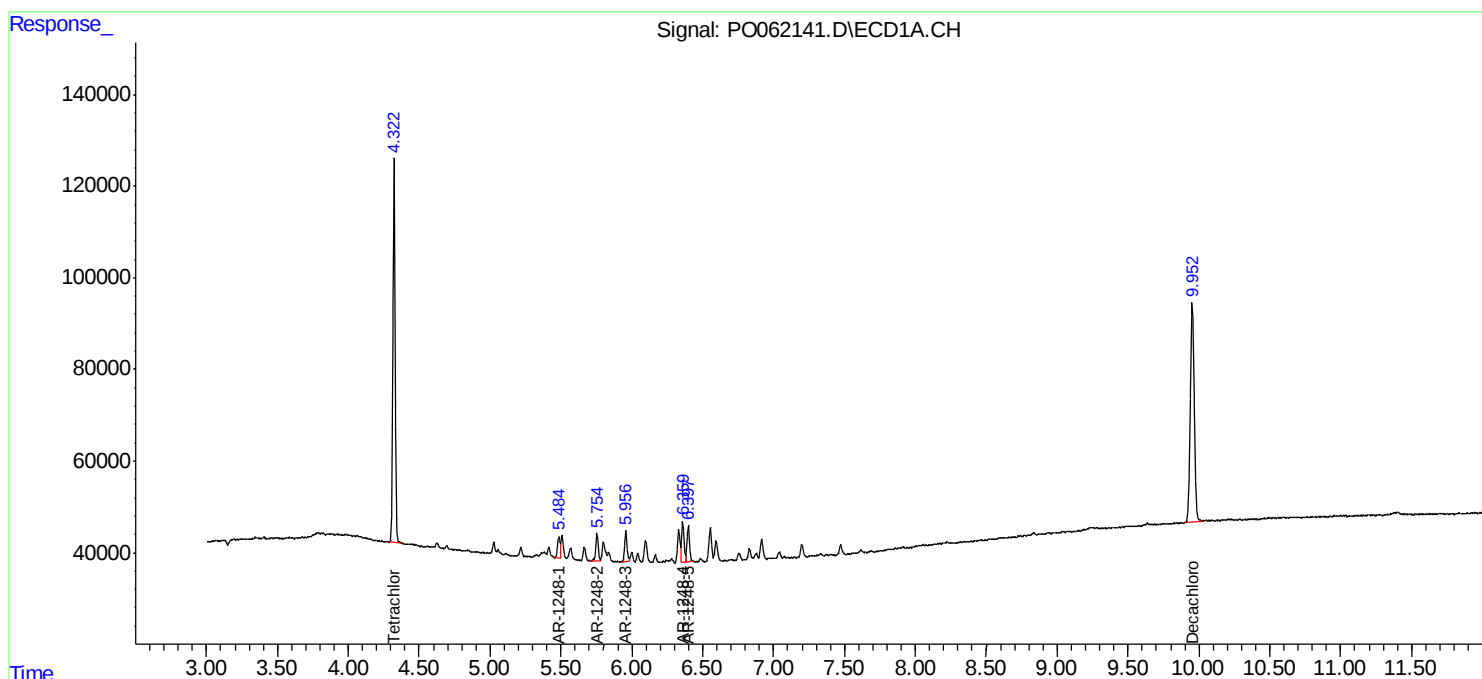

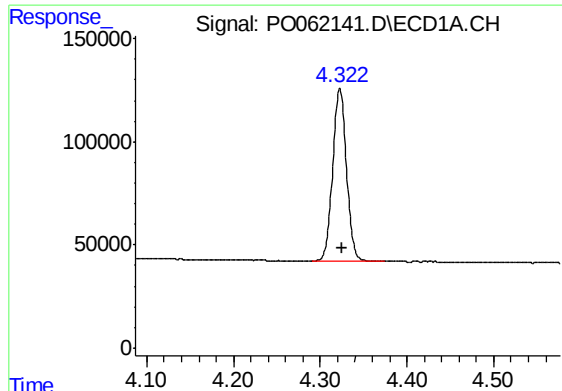


#1 Tetrachloro-m-xylene

R.T.: 4.323 min
Delta R.T.: -0.002 min
Response: 925070
Conc: 14.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2019


Manual Integrations
APPROVED

Ankita
10/21/2019 5:01:46 PM

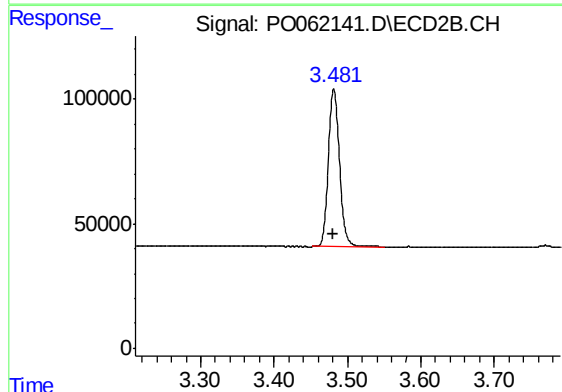


#1 Tetrachloro-m-xylene

R.T.: 3.482 min
Delta R.T.: 0.000 min
Response: 671012
Conc: 15.65 ng/ml

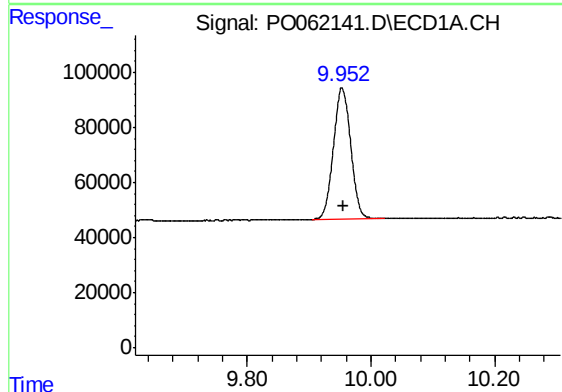


#2 Decachlorobiphenyl

R.T.: 9.953 min
Delta R.T.: -0.003 min
Response: 920471
Conc: 16.45 ng/ml

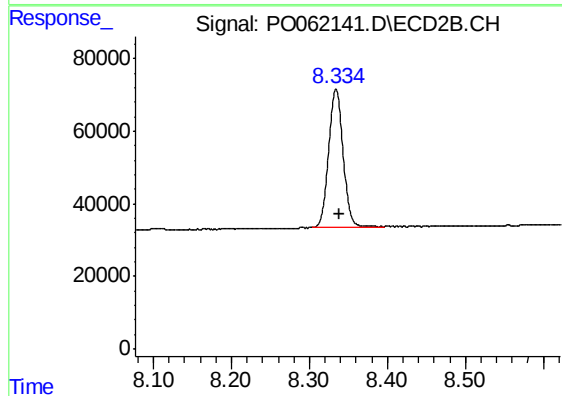

#2 Decachlorobiphenyl

R.T.: 8.334 min
Delta R.T.: -0.004 min
Response: 491202
Conc: 16.74 ng/ml

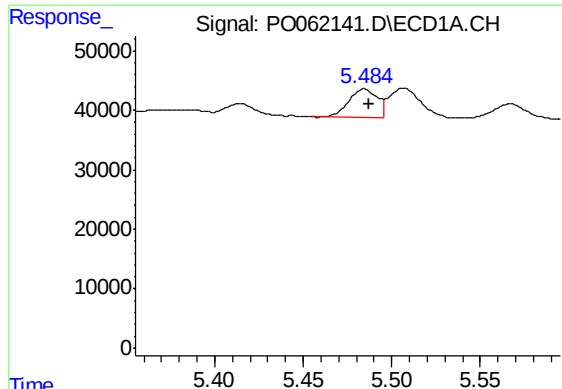


#21 AR-1248-1

R.T.: 5.485 min
Delta R.T.: -0.002 min
Response: 52946
Conc: 36.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2019


Manual Integrations
APPROVED

Ankita
10/21/2019 5:01:46 PM

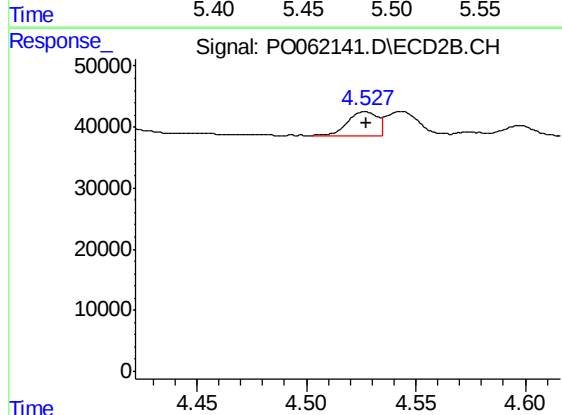


#21 AR-1248-1

R.T.: 4.527 min
Delta R.T.: 0.000 min
Response: 38115
Conc: 38.82 ng/ml m

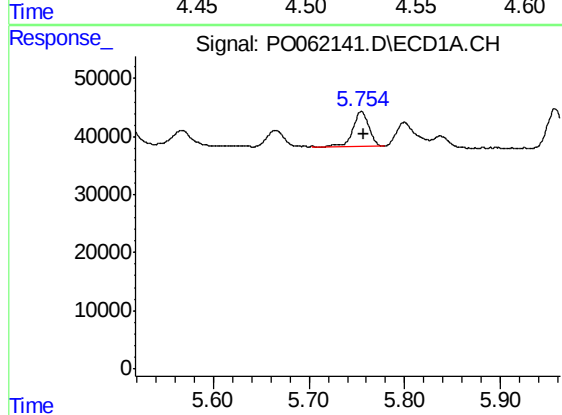


#22 AR-1248-2

R.T.: 5.755 min
Delta R.T.: -0.003 min
Response: 69333
Conc: 34.63 ng/ml

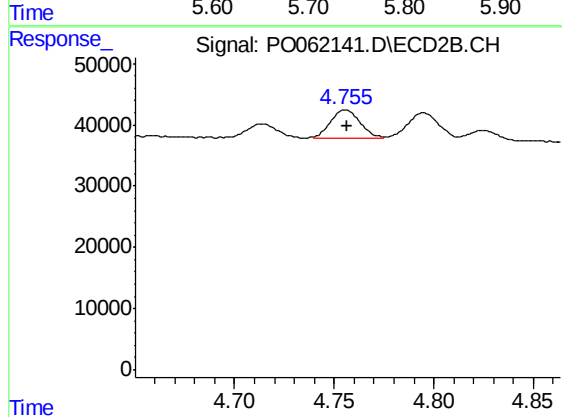

#22 AR-1248-2

R.T.: 4.755 min
Delta R.T.: -0.002 min
Response: 48719
Conc: 38.46 ng/ml m

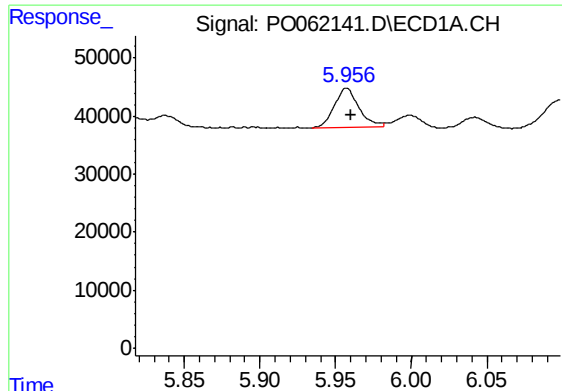


#23 AR-1248-3

R.T.: 5.956 min
Delta R.T.: -0.004 min
Response: 79036
Conc: 35.79 ng/ml m

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2019


Manual Integrations
APPROVED

Ankita
10/21/2019 5:01:46 PM

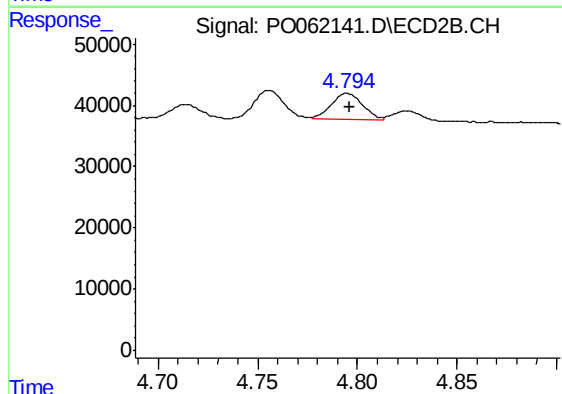


#23 AR-1248-3

R.T.: 4.794 min
Delta R.T.: -0.002 min
Response: 46440
Conc: 34.98 ng/ml m

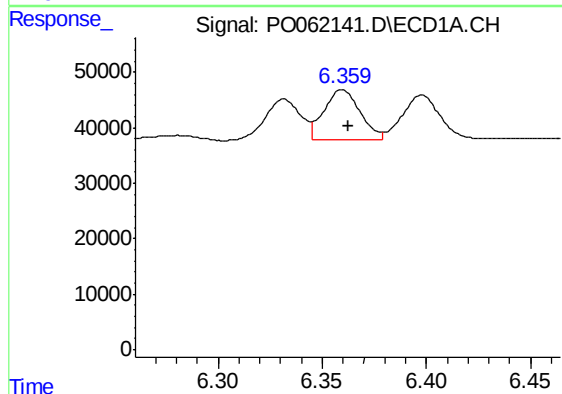


#24 AR-1248-4

R.T.: 6.360 min
Delta R.T.: -0.003 min
Response: 108809
Conc: 42.59 ng/ml

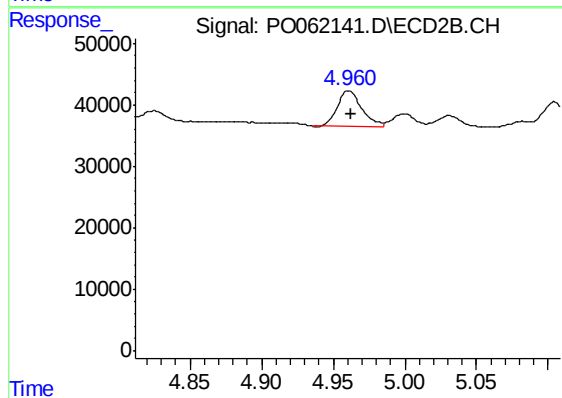

#24 AR-1248-4

R.T.: 4.961 min
Delta R.T.: -0.001 min
Response: 69444
Conc: 43.89 ng/ml

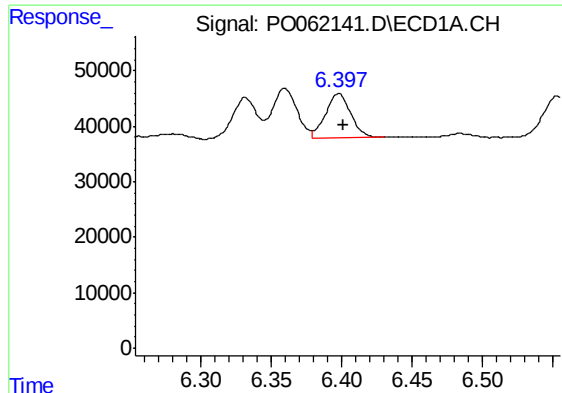


#25 AR-1248-5

R.T.: 6.398 min
Delta R.T.: -0.003 min
Response: 97458
Conc: 39.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2019

Manual Integrations
APPROVED

Ankita
10/21/2019 5:01:46 PM

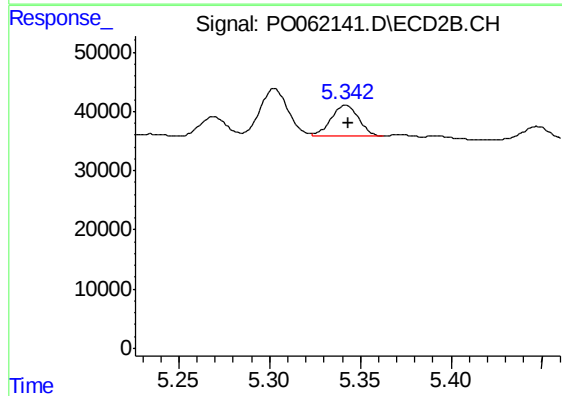

#25 AR-1248-5

R.T.: 5.342 min
Delta R.T.: -0.001 min
Response: 53889
Conc: 35.02 ng/ml