

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101819\
 Data File : P0062142.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Oct 2019 13:38
 Operator : HP/AJ
 Sample : K5111-07
 Misc : AR1254 LOD 40 PPB
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2019

Manual Integrations
 APPROVED

Ankita
 10/21/2019 5:01:48 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 02:46:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.324	3.483	1013149	733245	16.381	17.099
2)	SA Decachlor...	9.954	8.336	985142	528865	17.607	18.025
Target Compounds							
26)	L6 AR-1254-1	6.332	5.303	110168	102369	41.329	41.855
27)	L6 AR-1254-2	6.550	5.448	185008	93230	45.251	44.021
28)	L6 AR-1254-3	6.916	5.840	175591	136556	41.966	41.912
29)	L6 AR-1254-4	7.200	6.065	135875	77186	45.091	39.963
30)	L6 AR-1254-5	7.616	6.473	131142	111563	41.846m	42.239

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101819\
Data File : PO062142.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Oct 2019 13:38
Operator : HP/AJ
Sample : K5111-07
Misc : AR1254 LOD 40 PPB
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2019


Manual Integrations
APPROVED

Ankita
10/21/2019 5:01:48 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 02:46:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

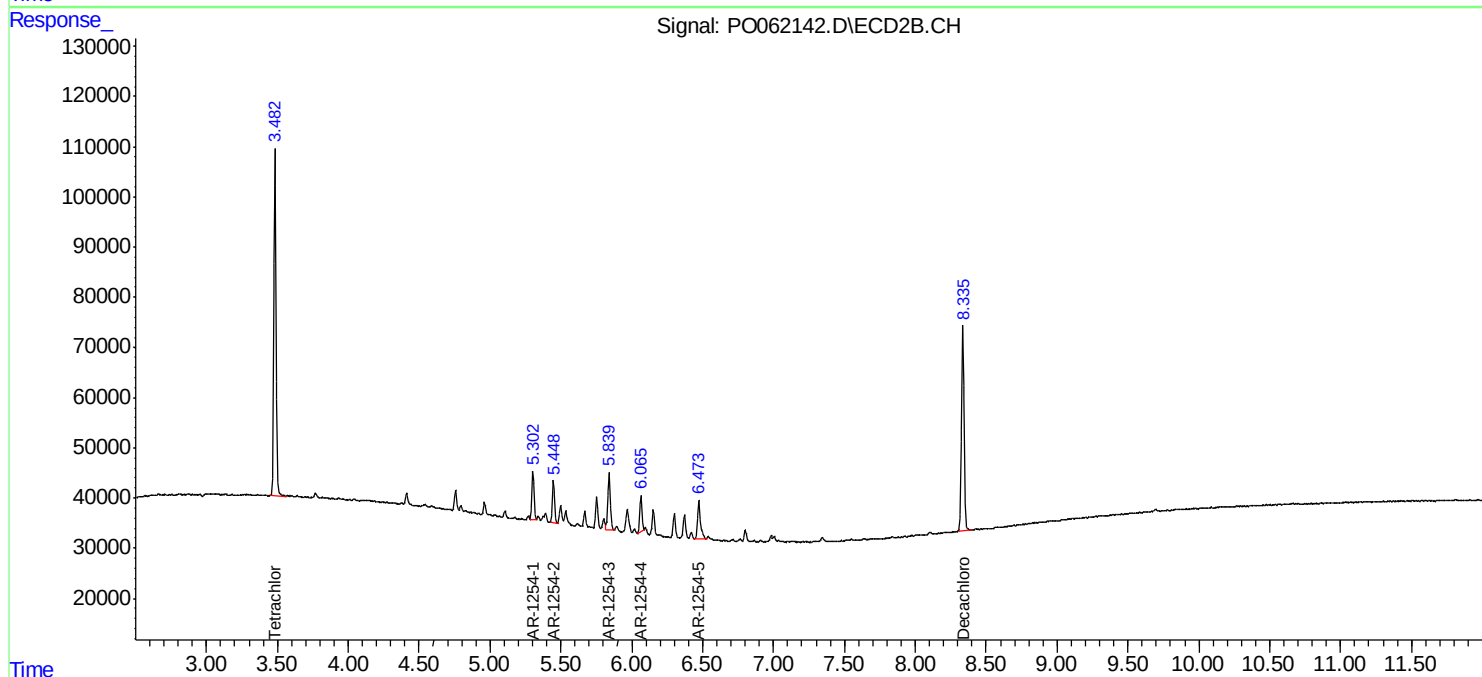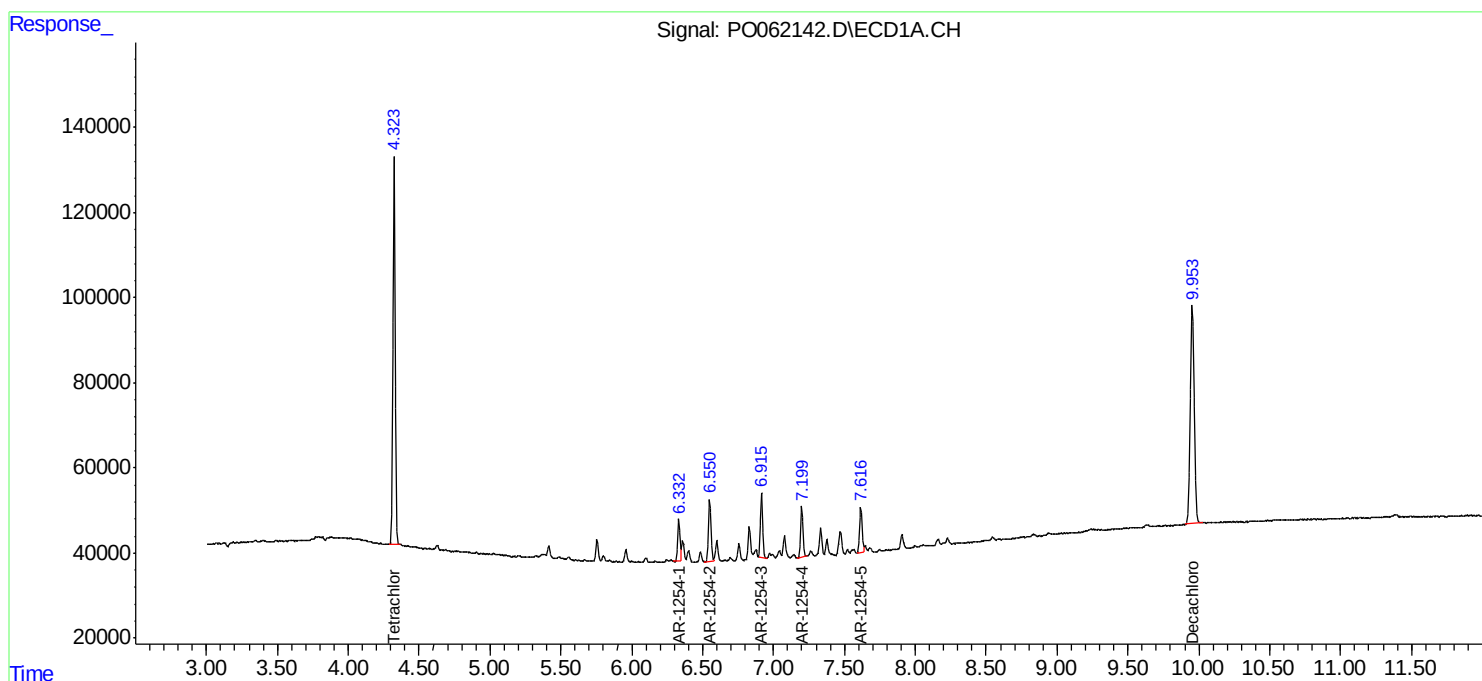

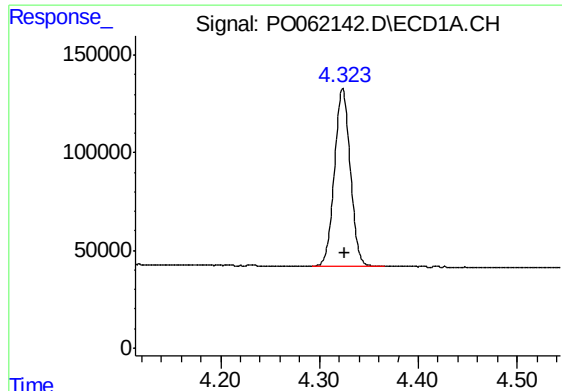


#1 Tetrachloro-m-xylene

R.T.: 4.324 min
Delta R.T.: -0.001 min
Response: 1013149
Conc: 16.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2019


Manual Integrations
APPROVED

Ankita
10/21/2019 5:01:48 PM

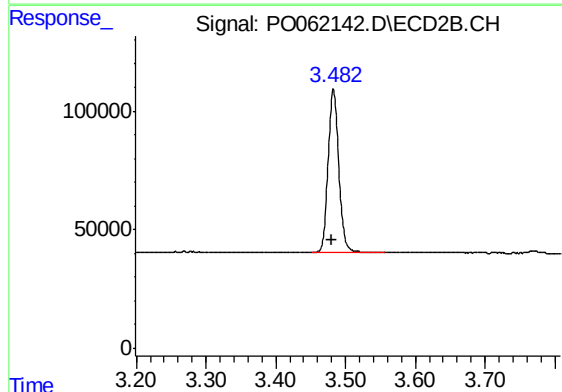


#1 Tetrachloro-m-xylene

R.T.: 3.483 min
Delta R.T.: 0.001 min
Response: 733245
Conc: 17.10 ng/ml

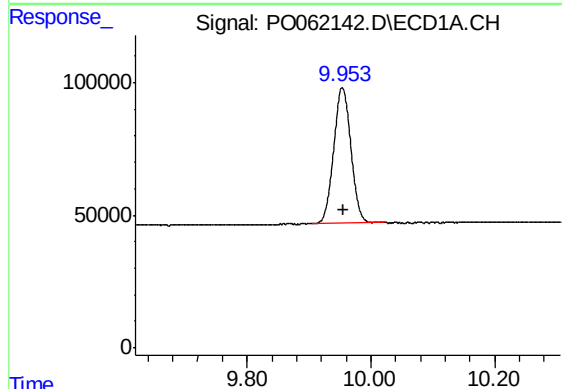


#2 Decachlorobiphenyl

R.T.: 9.954 min
Delta R.T.: -0.003 min
Response: 985142
Conc: 17.61 ng/ml

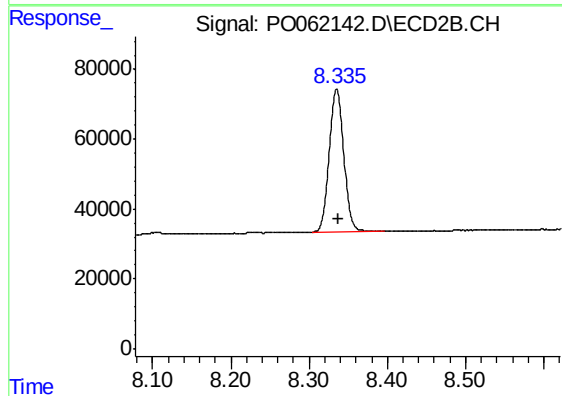

#2 Decachlorobiphenyl

R.T.: 8.336 min
Delta R.T.: -0.002 min
Response: 528865
Conc: 18.02 ng/ml

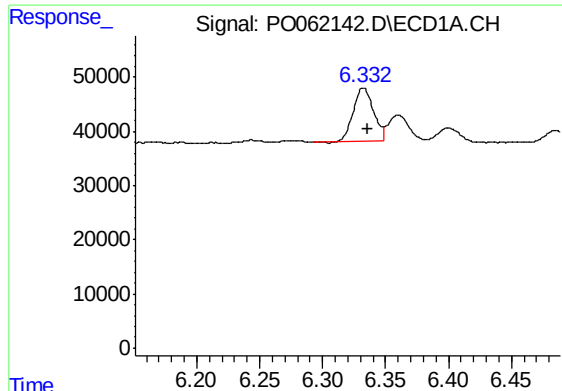


#26 AR-1254-1

R.T.: 6.332 min
Delta R.T.: -0.003 min
Response: 110168
Conc: 41.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2019


Manual Integrations
APPROVED

Ankita
10/21/2019 5:01:48 PM

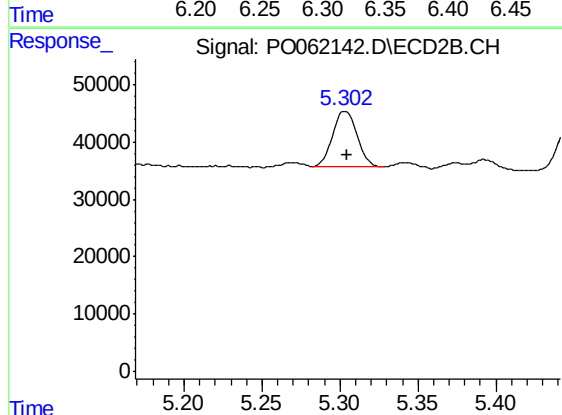


#26 AR-1254-1

R.T.: 5.303 min
Delta R.T.: -0.002 min
Response: 102369
Conc: 41.86 ng/ml

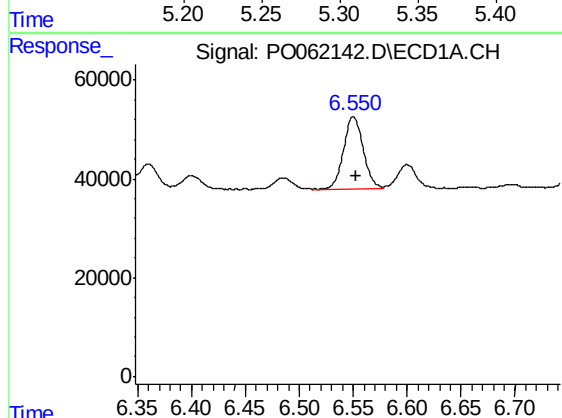


#27 AR-1254-2

R.T.: 6.550 min
Delta R.T.: -0.003 min
Response: 185008
Conc: 45.25 ng/ml

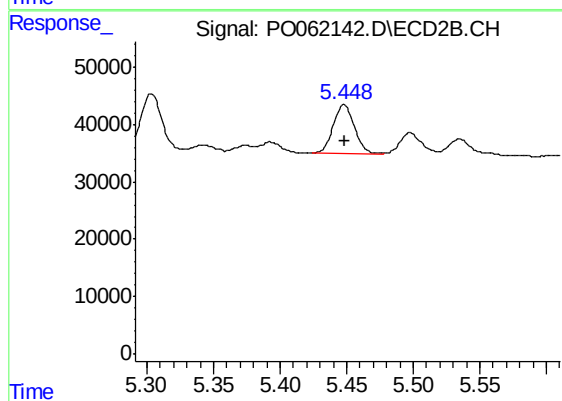

#27 AR-1254-2

R.T.: 5.448 min
Delta R.T.: 0.000 min
Response: 93230
Conc: 44.02 ng/ml

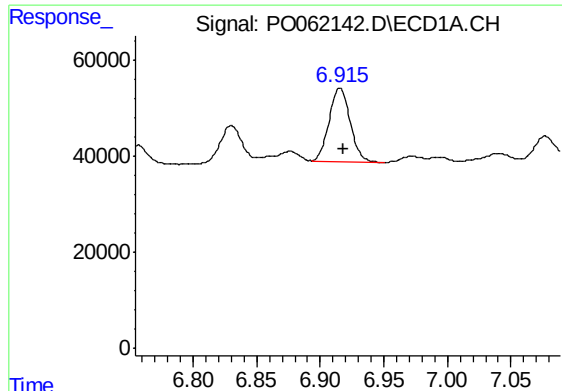


#28 AR-1254-3

R.T.: 6.916 min
Delta R.T.: -0.003 min
Response: 175591
Conc: 41.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2019


Manual Integrations
APPROVED

Ankita
10/21/2019 5:01:48 PM

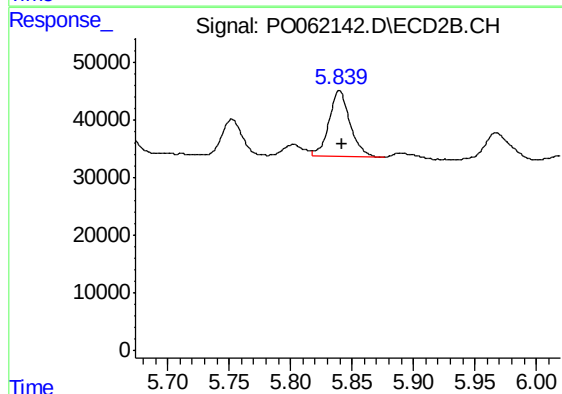


#28 AR-1254-3

R.T.: 5.840 min
Delta R.T.: -0.002 min
Response: 136556
Conc: 41.91 ng/ml

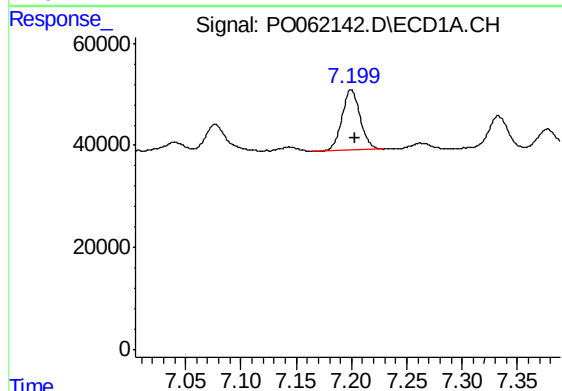


#29 AR-1254-4

R.T.: 7.200 min
Delta R.T.: -0.003 min
Response: 135875
Conc: 45.09 ng/ml

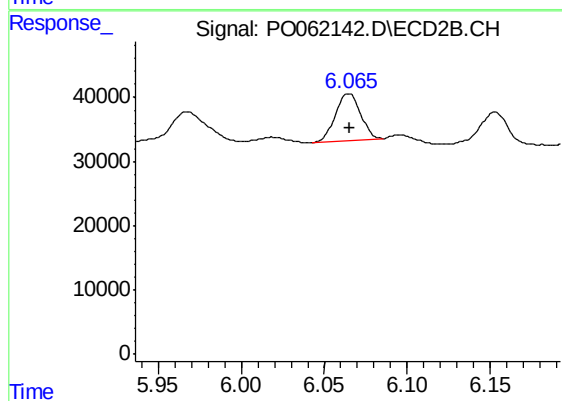

#29 AR-1254-4

R.T.: 6.065 min
Delta R.T.: 0.000 min
Response: 77186
Conc: 39.96 ng/ml

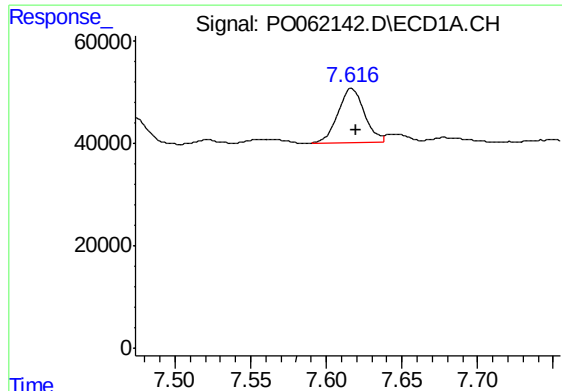


#30 AR-1254-5

R.T.: 7.616 min
Delta R.T.: -0.005 min
Response: 131142
Conc: 41.85 ng/ml m

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2019

Manual Integrations
APPROVED

Ankita
10/21/2019 5:01:48 PM

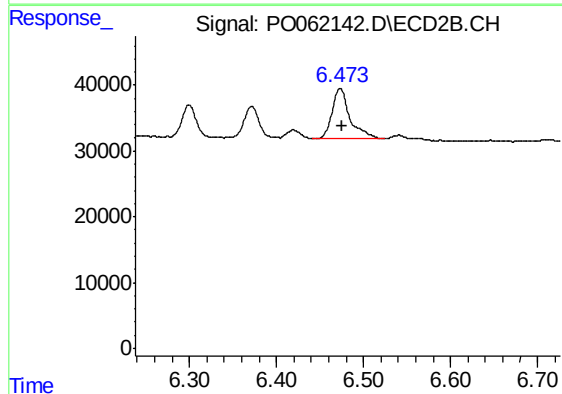

#30 AR-1254-5

R.T.: 6.473 min
Delta R.T.: -0.002 min
Response: 111563
Conc: 42.24 ng/ml