

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101819\
 Data File : P0062143.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Oct 2019 13:54
 Operator : HP/AJ
 Sample : K5111-07
 Misc : AR1262 LOD 40 PPB
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2019

Manual Integrations
 APPROVED

Ankita
 10/21/2019 5:01:50 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 02:46:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.323	3.482	926482	667931	14.980	15.576
2)	SA Decachlor...	9.954	8.335	971152	519884	17.357	17.718
Target Compounds							
36)	L8 AR-1262-1	7.690	6.563	175776	49903	42.821	41.873
37)	L8 AR-1262-2	8.228	7.005	273542	177636	42.423	42.276
38)	L8 AR-1262-3	8.526	7.282	191879	80143	43.635m	45.567
39)	L8 AR-1262-4	8.614	7.346	146806	127678	42.491	41.764
40)	L8 AR-1262-5	9.243	7.835	97786	54657	43.293m	41.850

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101819\
Data File : PO062143.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Oct 2019 13:54
Operator : HP/AJ
Sample : K5111-07
Misc : AR1262 LOD 40 PPB
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2019


Manual Integrations
APPROVED

Ankita
10/21/2019 5:01:50 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 02:46:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

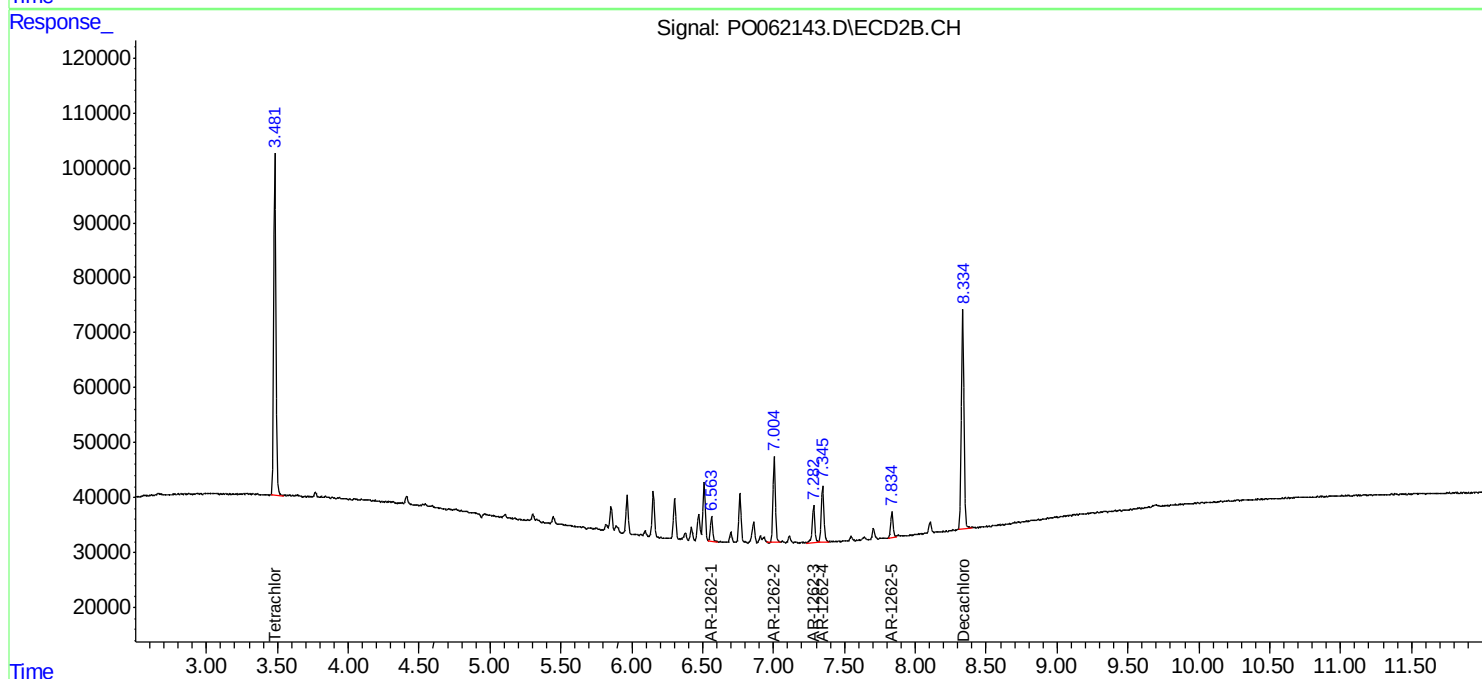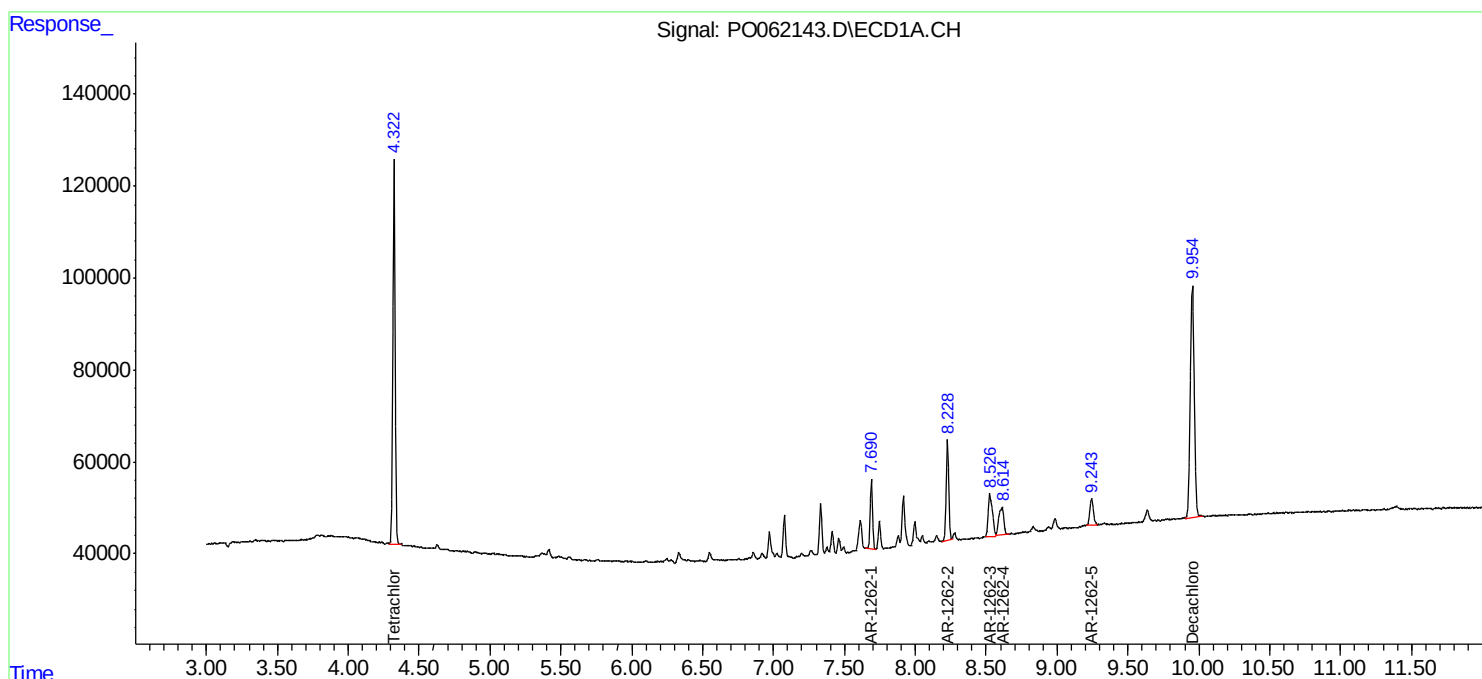

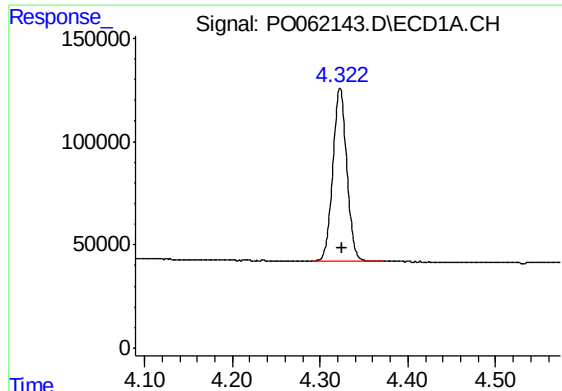


#1 Tetrachloro-m-xylene

R.T.: 4.323 min
Delta R.T.: -0.002 min
Response: 926482
Conc: 14.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2019


Manual Integrations
APPROVED

Ankita
10/21/2019 5:01:50 PM

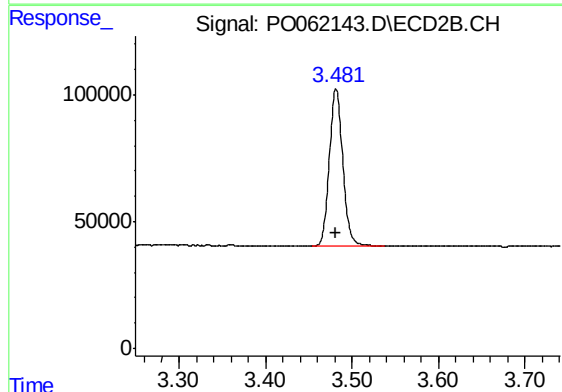


#1 Tetrachloro-m-xylene

R.T.: 3.482 min
Delta R.T.: 0.000 min
Response: 667931
Conc: 15.58 ng/ml

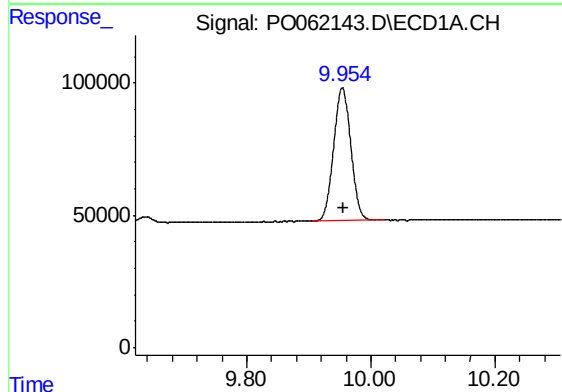


#2 Decachlorobiphenyl

R.T.: 9.954 min
Delta R.T.: -0.002 min
Response: 971152
Conc: 17.36 ng/ml

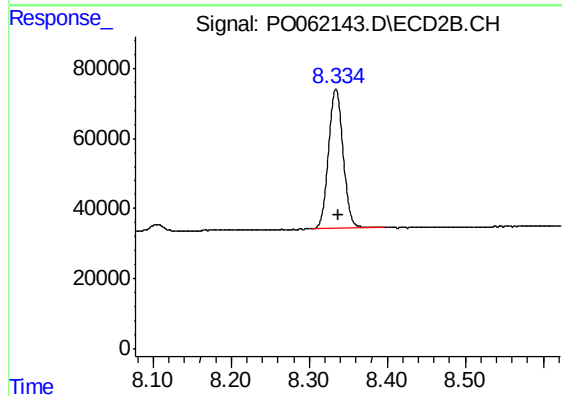

#2 Decachlorobiphenyl

R.T.: 8.335 min
Delta R.T.: -0.003 min
Response: 519884
Conc: 17.72 ng/ml

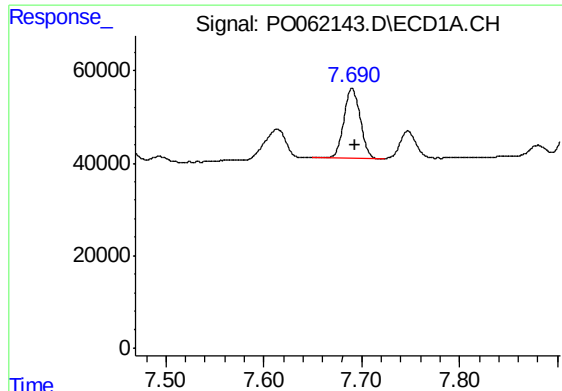


#36 AR-1262-1

R.T.: 7.690 min
Delta R.T.: -0.003 min
Response: 175776
Conc: 42.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2019


Manual Integrations
APPROVED

Ankita
10/21/2019 5:01:50 PM

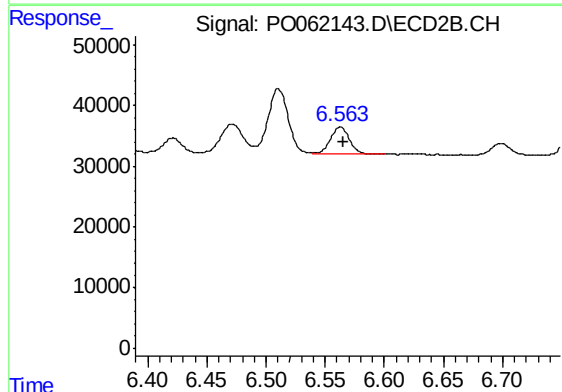


#36 AR-1262-1

R.T.: 6.563 min
Delta R.T.: -0.002 min
Response: 49903
Conc: 41.87 ng/ml

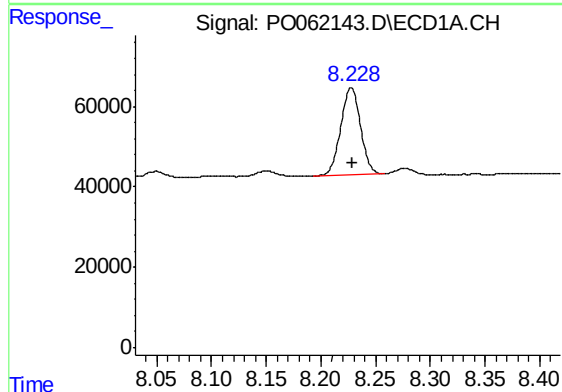


#37 AR-1262-2

R.T.: 8.228 min
Delta R.T.: -0.001 min
Response: 273542
Conc: 42.42 ng/ml

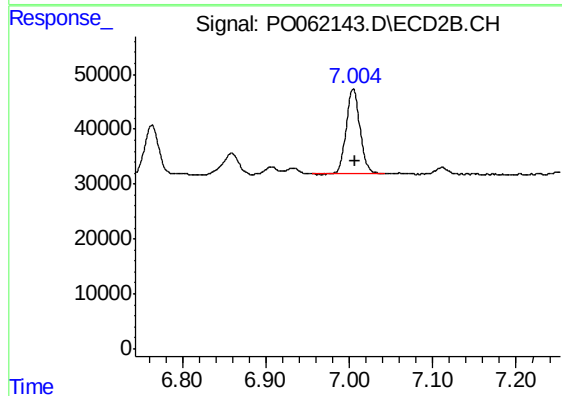

#37 AR-1262-2

R.T.: 7.005 min
Delta R.T.: -0.002 min
Response: 177636
Conc: 42.28 ng/ml

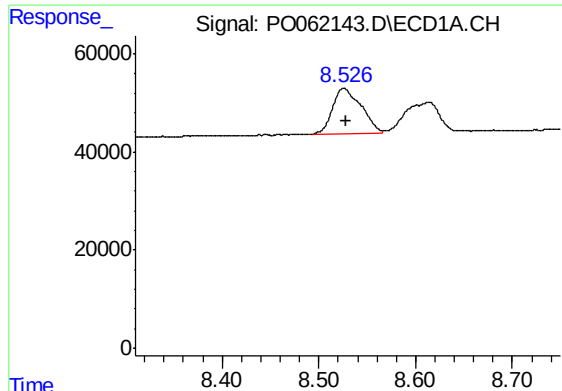


#38 AR-1262-3

R.T.: 8.526 min
Delta R.T.: -0.002 min
Response: 191879
Conc: 43.63 ng/ml m

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2019


Manual Integrations
APPROVED

Ankita
10/21/2019 5:01:50 PM

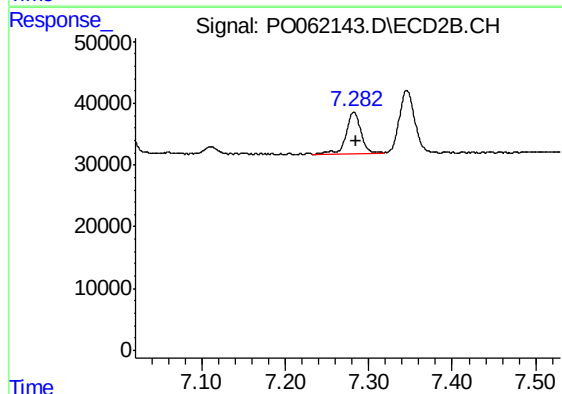


#38 AR-1262-3

R.T.: 7.282 min
Delta R.T.: -0.004 min
Response: 80143
Conc: 45.57 ng/ml

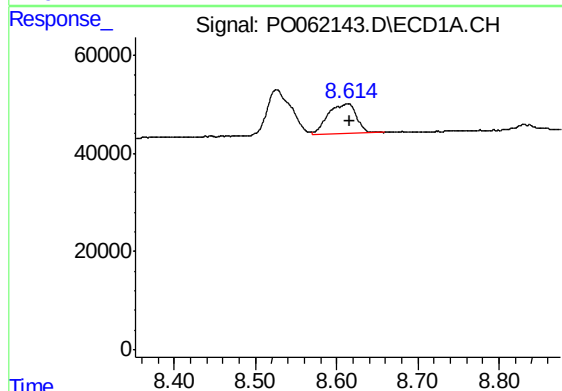


#39 AR-1262-4

R.T.: 8.614 min
Delta R.T.: -0.002 min
Response: 146806
Conc: 42.49 ng/ml

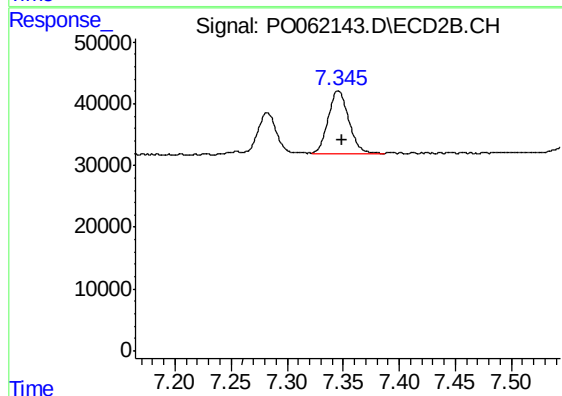

#39 AR-1262-4

R.T.: 7.346 min
Delta R.T.: -0.003 min
Response: 127678
Conc: 41.76 ng/ml

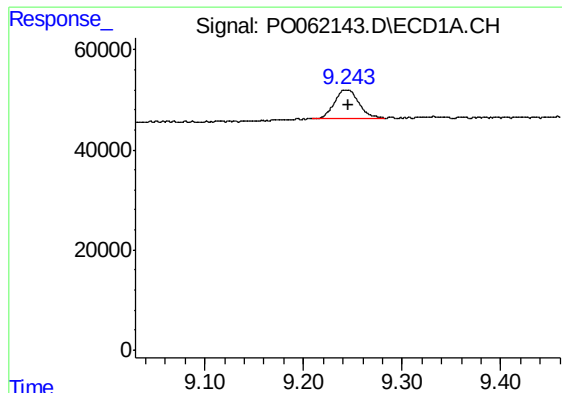


#40 AR-1262-5

R.T.: 9.243 min
Delta R.T.: -0.003 min
Response: 97786
Conc: 43.29 ng/ml m

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2019

Manual Integrations
APPROVED

Ankita
10/21/2019 5:01:50 PM

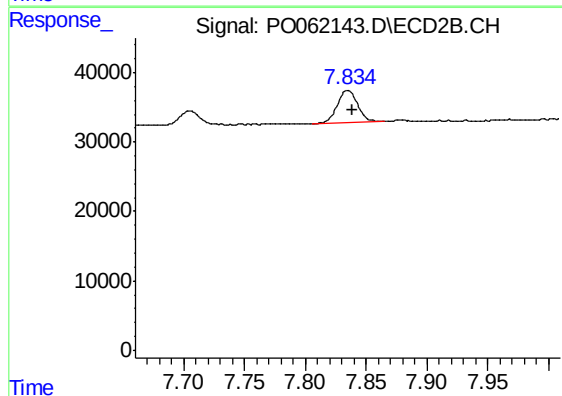

#40 AR-1262-5

R.T.: 7.835 min
Delta R.T.: -0.004 min
Response: 54657
Conc: 41.85 ng/ml