

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101819\
 Data File : P0062161.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Oct 2019 19:09
 Operator : HP/AJ
 Sample : K5432-04
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 445X-DUP-8

Manual Integrations
 APPROVED

Ankita
 10/21/2019 5:02:15 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 02:51:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.322	3.483	1071506	749570	17.325m	17.480
2)	SA Decachlor...	9.950	8.333	946080	505755	16.909	17.237

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101819\
Data File : P0062161.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Oct 2019 19:09
Operator : HP/AJ
Sample : K5432-04
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
445X-DUP-8


Manual Integrations
APPROVED

Ankita
10/21/2019 5:02:15 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 02:51:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

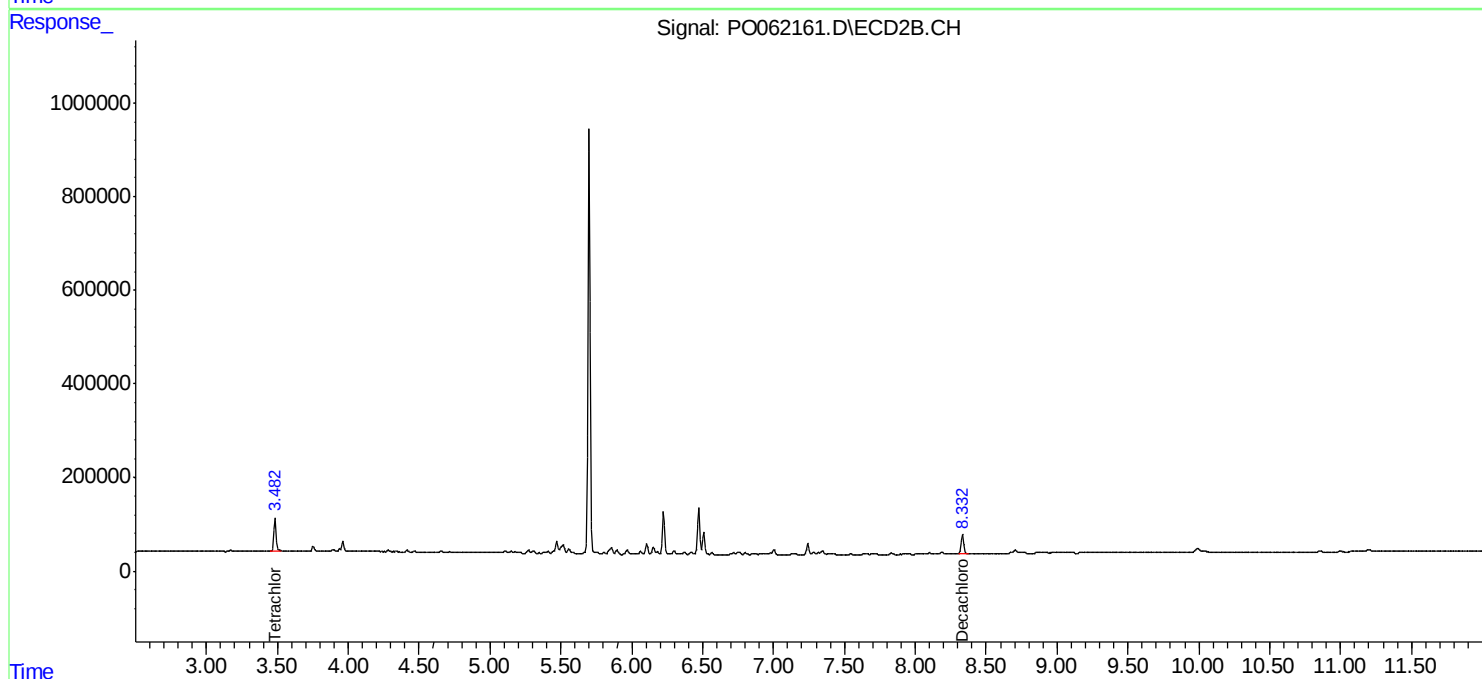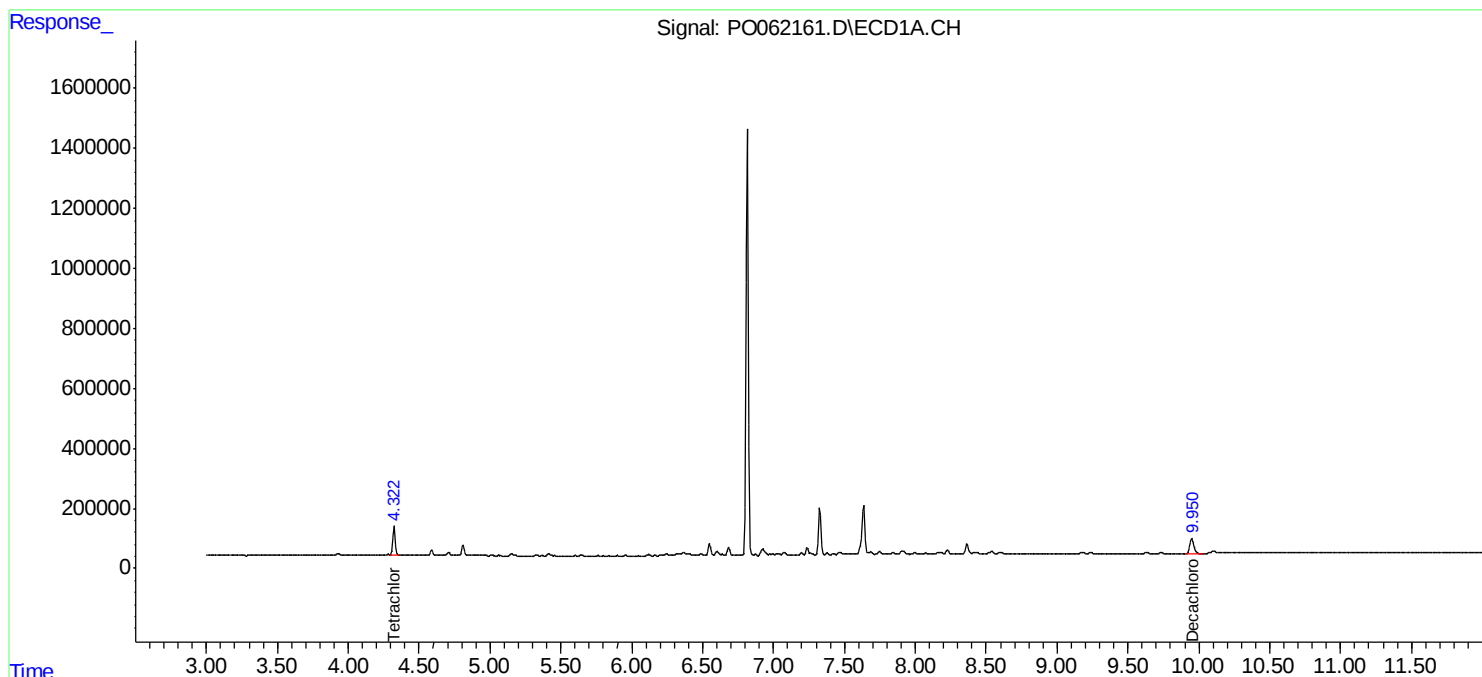

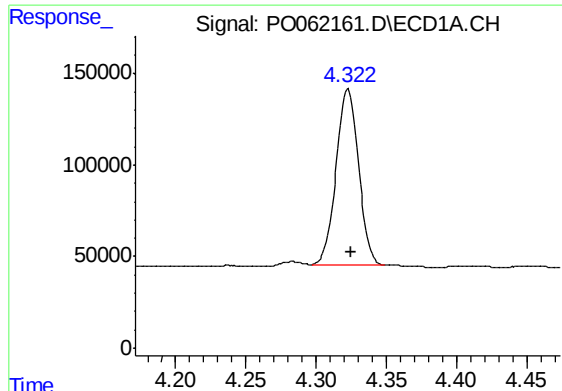


#1 Tetrachloro-m-xylene

R.T.: 4.322 min
Delta R.T.: -0.003 min
Response: 1071506
Conc: 17.33 ng/ml m

Instrument :
ECD_O
ClientSampleId :
445X-DUP-8


Manual Integrations
APPROVED

Ankita
10/21/2019 5:02:15 PM

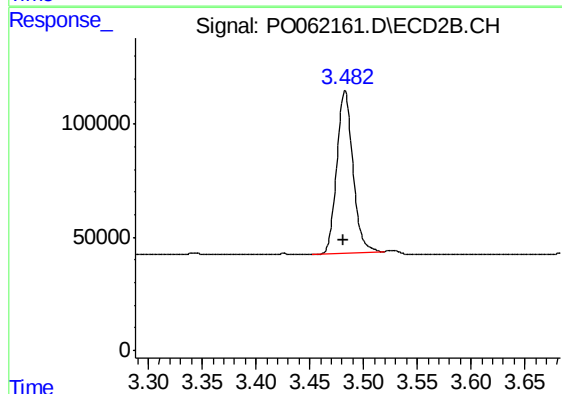


#1 Tetrachloro-m-xylene

R.T.: 3.483 min
Delta R.T.: 0.001 min
Response: 749570
Conc: 17.48 ng/ml

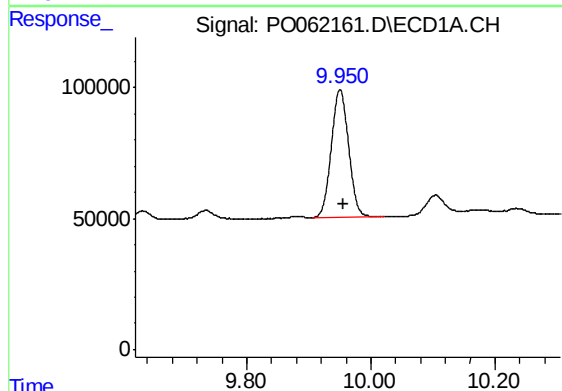

#2 Decachlorobiphenyl

R.T.: 9.950 min
Delta R.T.: -0.006 min
Response: 946080
Conc: 16.91 ng/ml

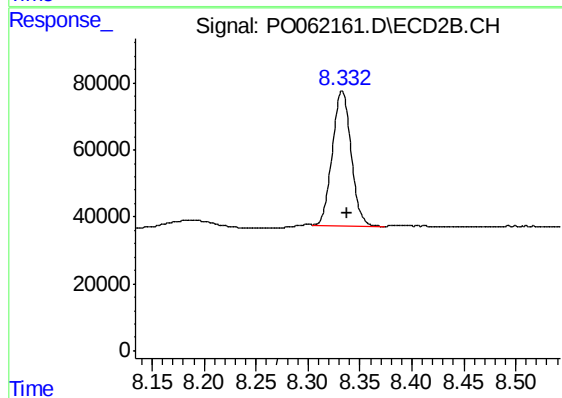

#2 Decachlorobiphenyl

R.T.: 8.333 min
Delta R.T.: -0.005 min
Response: 505755
Conc: 17.24 ng/ml