

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101819\
 Data File : P0062179.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Oct 2019 00:21
 Operator : HP/AJ
 Sample : K5429-03
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 445X-15A

Manual Integrations
 APPROVED

Ankita
 10/21/2019 5:03:06 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 02:56:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.322	3.482	1347458	941247	21.787	21.950
2)	SA Decachlor...	9.948	8.332	1071648	525715	19.153	17.917
Target Compounds							
26)	L6 AR-1254-1	6.364	5.301	42492	36460	15.941m	14.907
27)	L6 AR-1254-2	6.548	5.446	118661	30155	29.023	14.238 #
28)	L6 AR-1254-3	6.915	5.838	193956	93786	46.356	28.785m#
29)	L6 AR-1254-4	7.197	6.062	65840	52285	21.850	27.071
30)	L6 AR-1254-5	7.615	6.471	275771	226122	87.996m	85.614

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101819\
Data File : PO062179.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Oct 2019 00:21
Operator : HP/AJ
Sample : K5429-03
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
445X-15A


Manual Integrations
APPROVED

Ankita
10/21/2019 5:03:06 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 02:56:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

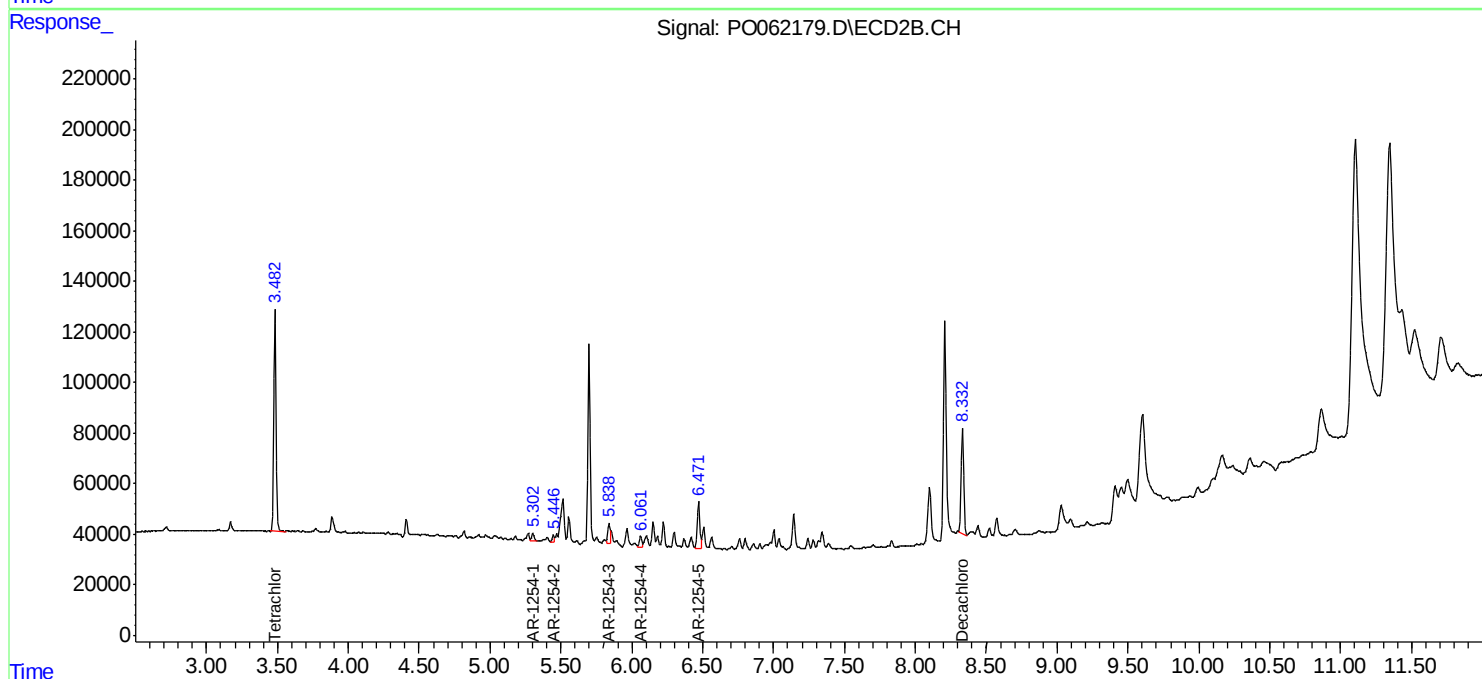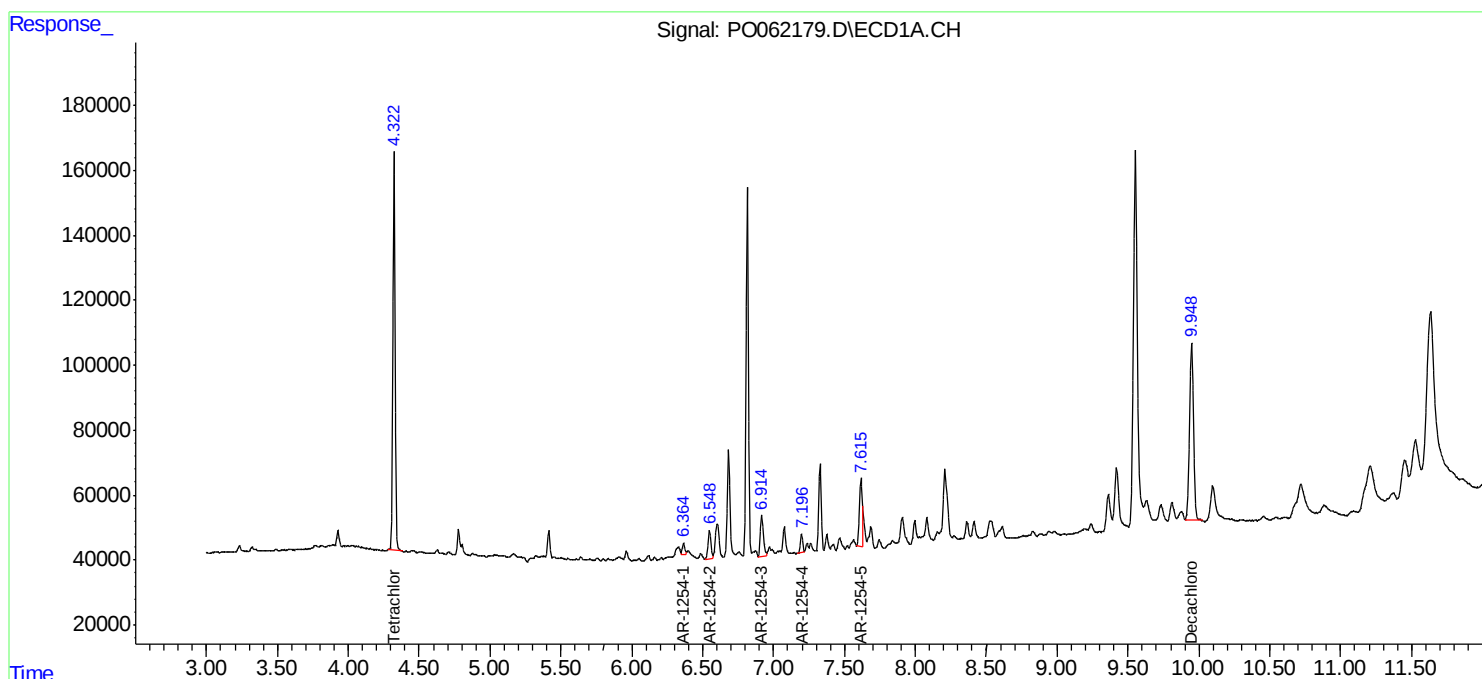

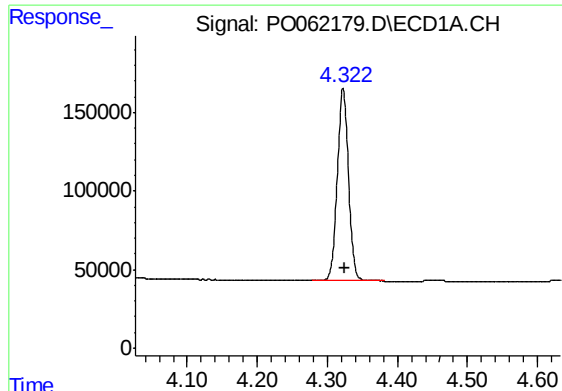


#1 Tetrachloro-m-xylene

R.T.: 4.322 min
Delta R.T.: -0.003 min
Response: 1347458
Conc: 21.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
445X-15A


Manual Integrations
APPROVED

Ankita
10/21/2019 5:03:06 PM

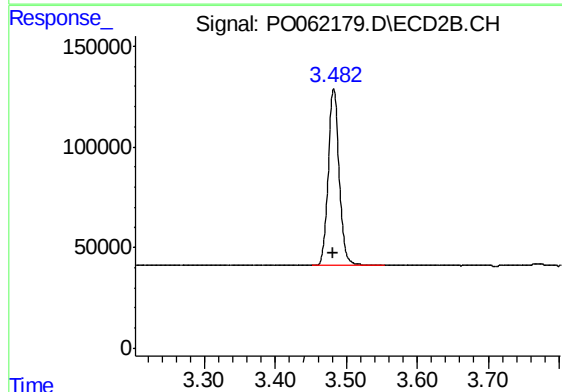


#1 Tetrachloro-m-xylene

R.T.: 3.482 min
Delta R.T.: 0.000 min
Response: 941247
Conc: 21.95 ng/ml

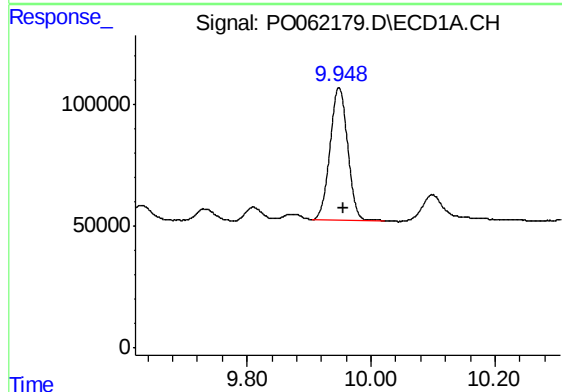


#2 Decachlorobiphenyl

R.T.: 9.948 min
Delta R.T.: -0.008 min
Response: 1071648
Conc: 19.15 ng/ml

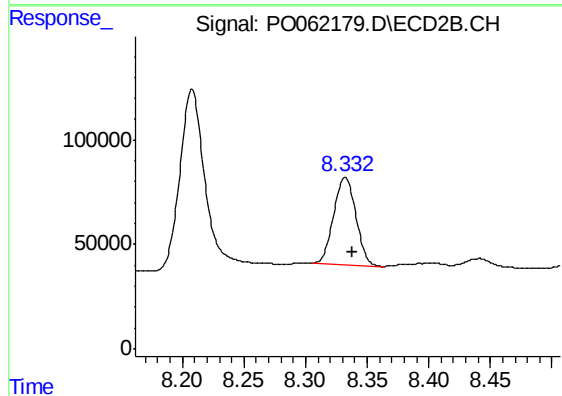

#2 Decachlorobiphenyl

R.T.: 8.332 min
Delta R.T.: -0.006 min
Response: 525715
Conc: 17.92 ng/ml

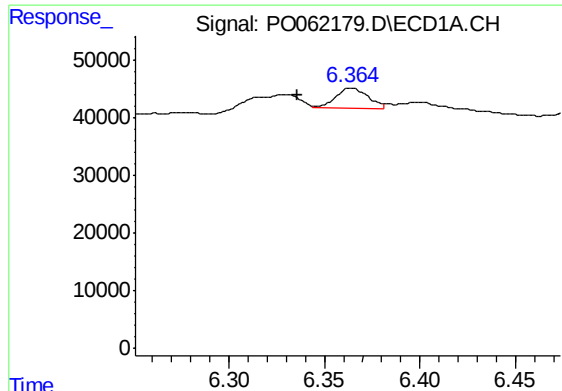


#26 AR-1254-1

R.T.: 6.364 min
Delta R.T.: 0.028 min
Response: 42492
Conc: 15.94 ng/ml m

Instrument :
ECD_O
ClientSampleId :
445X-15A


Manual Integrations
APPROVED

Ankita
10/21/2019 5:03:06 PM

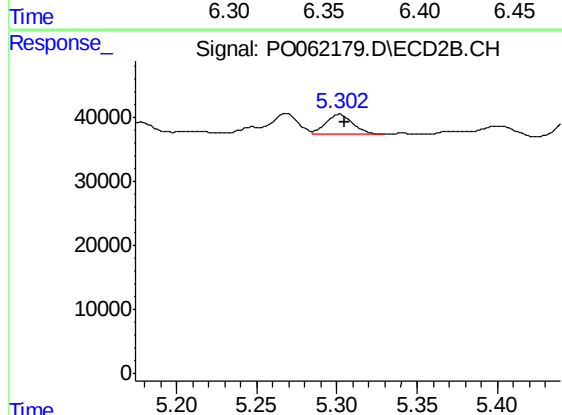


#26 AR-1254-1

R.T.: 5.301 min
Delta R.T.: -0.003 min
Response: 36460
Conc: 14.91 ng/ml

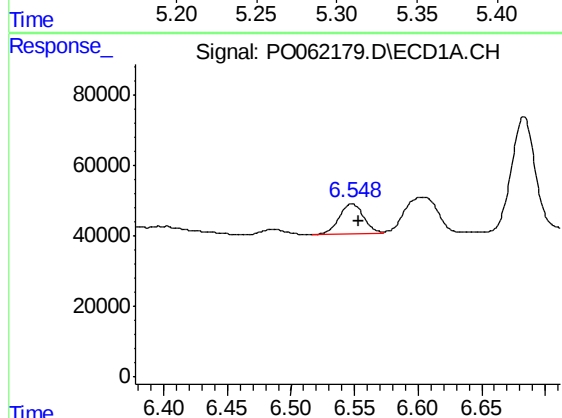


#27 AR-1254-2

R.T.: 6.548 min
Delta R.T.: -0.005 min
Response: 118661
Conc: 29.02 ng/ml

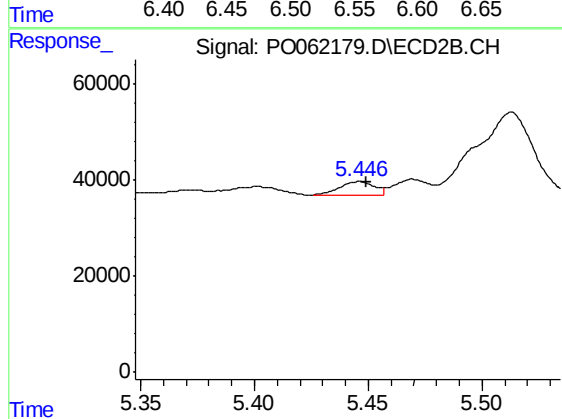

#27 AR-1254-2

R.T.: 5.446 min
Delta R.T.: -0.003 min
Response: 30155
Conc: 14.24 ng/ml

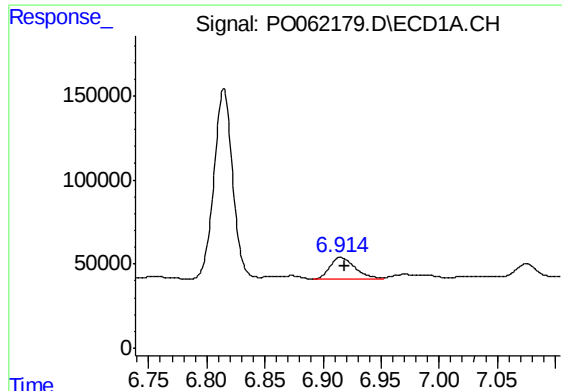


#28 AR-1254-3

R.T.: 6.915 min
Delta R.T.: -0.003 min
Response: 193956
Conc: 46.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
445X-15A


Manual Integrations
APPROVED

Ankita
10/21/2019 5:03:06 PM

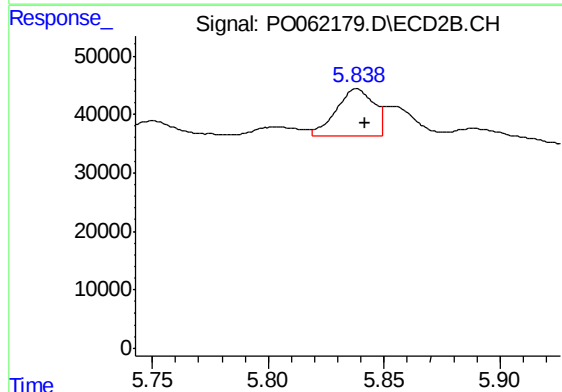


#28 AR-1254-3

R.T.: 5.838 min
Delta R.T.: -0.004 min
Response: 93786
Conc: 28.78 ng/ml m

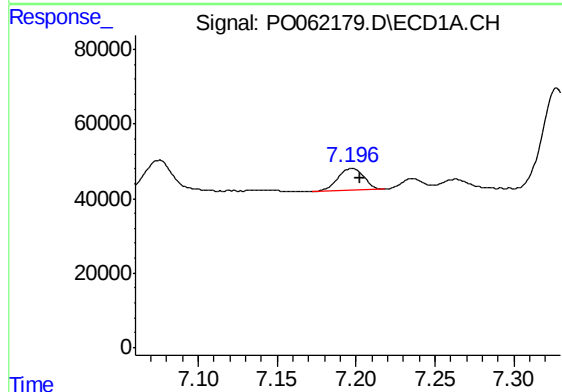


#29 AR-1254-4

R.T.: 7.197 min
Delta R.T.: -0.006 min
Response: 65840
Conc: 21.85 ng/ml

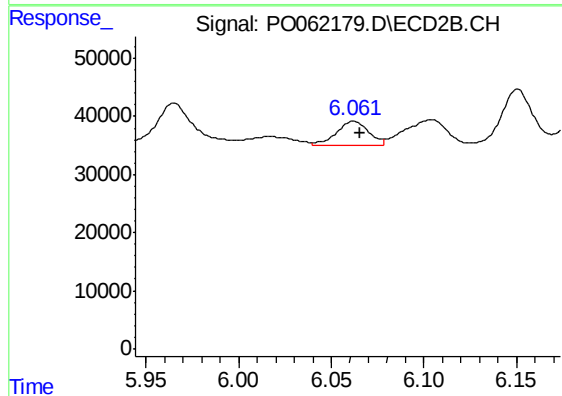

#29 AR-1254-4

R.T.: 6.062 min
Delta R.T.: -0.004 min
Response: 52285
Conc: 27.07 ng/ml

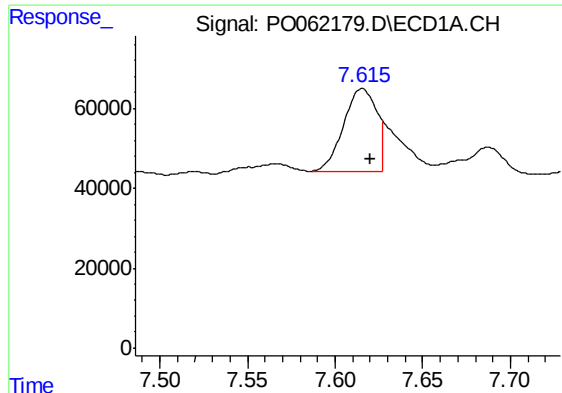


#30 AR-1254-5

R.T.: 7.615 min
Delta R.T.: -0.005 min
Response: 275771
Conc: 88.00 ng/ml m

Instrument :
ECD_O
ClientSampleId :
445X-15A

Manual Integrations
APPROVED

Ankita
10/21/2019 5:03:06 PM

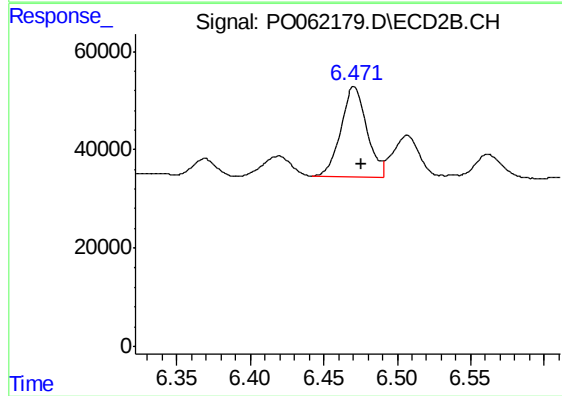

#30 AR-1254-5

R.T.: 6.471 min
Delta R.T.: -0.005 min
Response: 226122
Conc: 85.61 ng/ml