

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101819\
 Data File : P0062192.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Oct 2019 4:12
 Operator : HP/AJ
 Sample : K5430-16
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 445X-26A

Manual Integrations
 APPROVED

Ankita
 10/21/2019 5:03:54 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 05:17:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.320	3.481	1128544	838795	18.247m	19.561
2)	SA Decachlor...	9.947	8.331	991296	546406	17.717	18.622
Target Compounds							
31)	L7 AR-1260-1	7.073	5.964	219144	285608	76.970m	134.420 #
32)	L7 AR-1260-2	7.326	6.150	1191689	357278	347.375m	140.792 #
33)	L7 AR-1260-3	7.686	6.298	291531	175658	110.173m	77.790 #
34)	L7 AR-1260-4	7.908	6.760	465191	186566	166.315m	106.254 #
35)	L7 AR-1260-5	8.223	7.001	484565	371775	92.552m	103.201

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101819\
Data File : PO062192.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Oct 2019 4:12
Operator : HP/AJ
Sample : K5430-16
Misc :
ALS Vial : 45 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
445X-26A


Manual Integrations
APPROVED

Ankita
10/21/2019 5:03:54 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 05:17:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

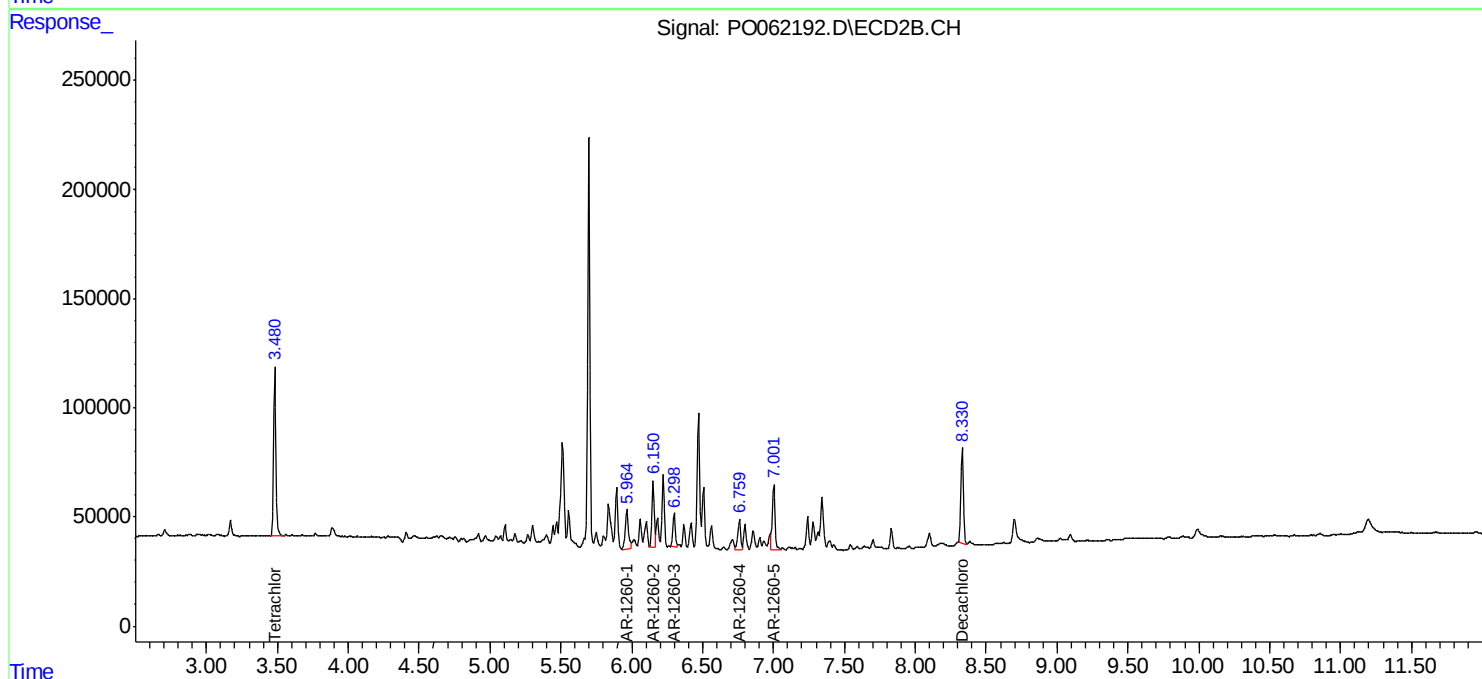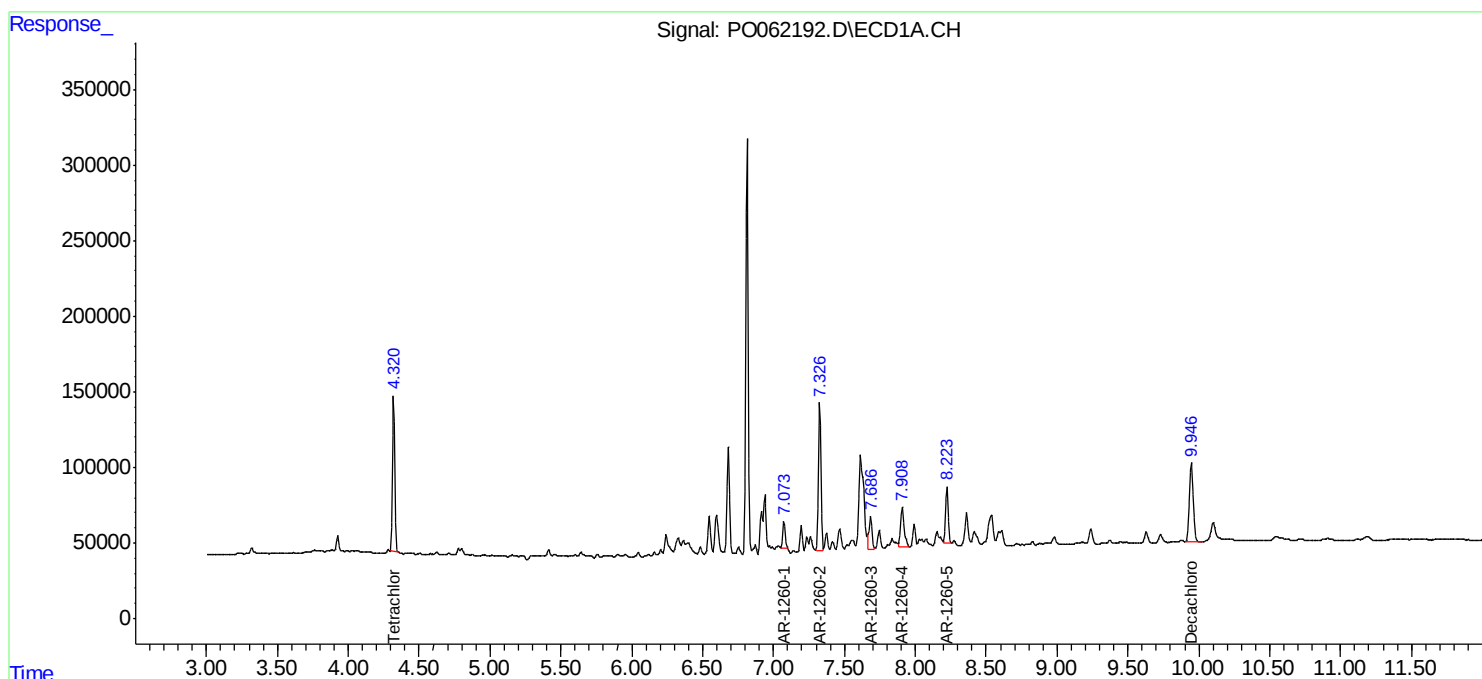

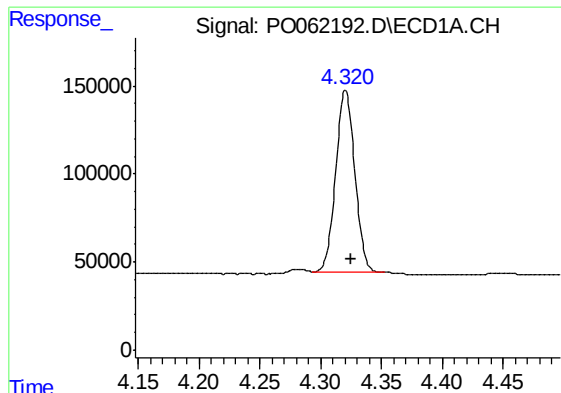


#1 Tetrachloro-m-xylene

R.T.: 4.320 min
Delta R.T.: -0.005 min
Response: 1128544
Conc: 18.25 ng/ml m

Instrument :
ECD_O
ClientSampleId :
445X-26A


Manual Integrations
APPROVED

Ankita
10/21/2019 5:03:54 PM

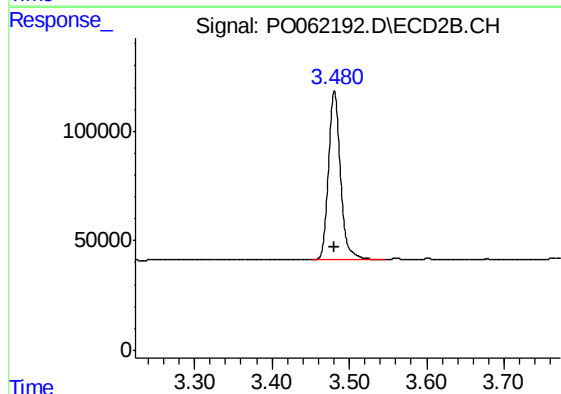


#1 Tetrachloro-m-xylene

R.T.: 3.481 min
Delta R.T.: 0.000 min
Response: 838795
Conc: 19.56 ng/ml

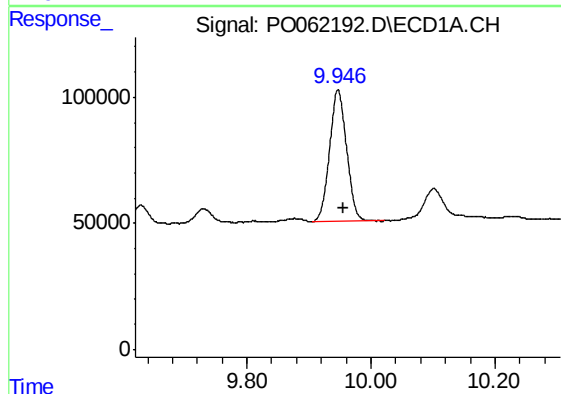


#2 Decachlorobiphenyl

R.T.: 9.947 min
Delta R.T.: -0.010 min
Response: 991296
Conc: 17.72 ng/ml

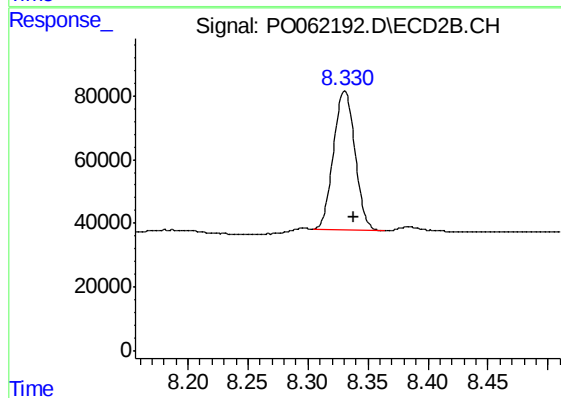

#2 Decachlorobiphenyl

R.T.: 8.331 min
Delta R.T.: -0.007 min
Response: 546406
Conc: 18.62 ng/ml

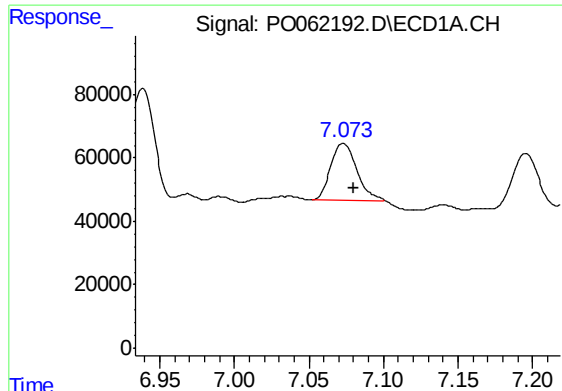


#31 AR-1260-1

R.T.: 7.073 min
Delta R.T.: -0.007 min
Response: 219144
Conc: 76.97 ng/ml m

Instrument :
ECD_O
ClientSampleId :
445X-26A


Manual Integrations
APPROVED

Ankita
10/21/2019 5:03:54 PM

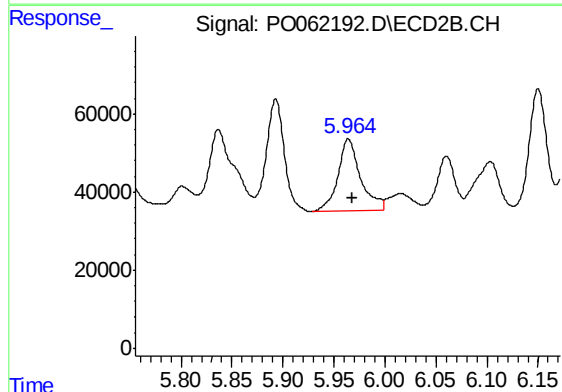


#31 AR-1260-1

R.T.: 5.964 min
Delta R.T.: -0.004 min
Response: 285608
Conc: 134.42 ng/ml

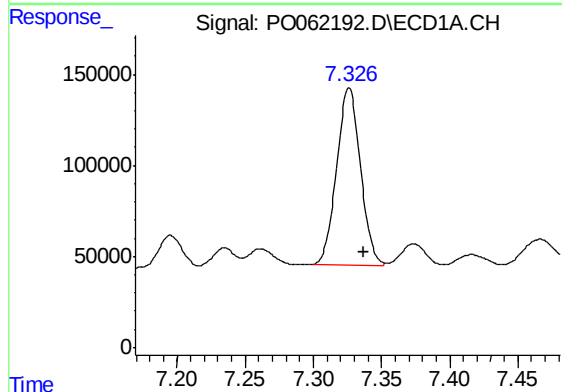


#32 AR-1260-2

R.T.: 7.326 min
Delta R.T.: -0.011 min
Response: 1191689
Conc: 347.38 ng/ml m

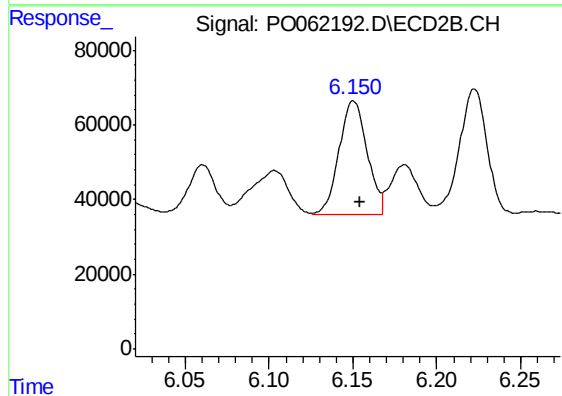

#32 AR-1260-2

R.T.: 6.150 min
Delta R.T.: -0.004 min
Response: 357278
Conc: 140.79 ng/ml

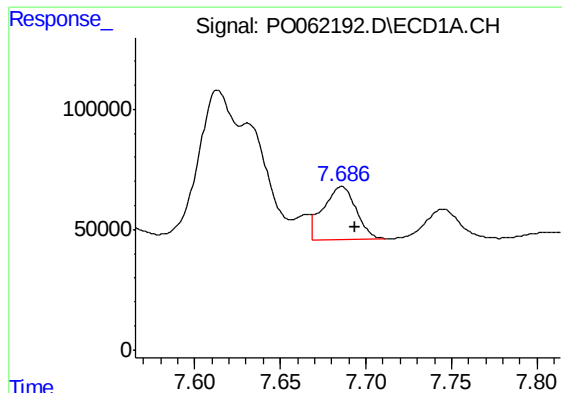


#33 AR-1260-3

R.T.: 7.686 min
Delta R.T.: -0.008 min
Response: 291531
Conc: 110.17 ng/ml m

Instrument :
ECD_O
ClientSampleId :
445X-26A


Manual Integrations
APPROVED

Ankita
10/21/2019 5:03:54 PM

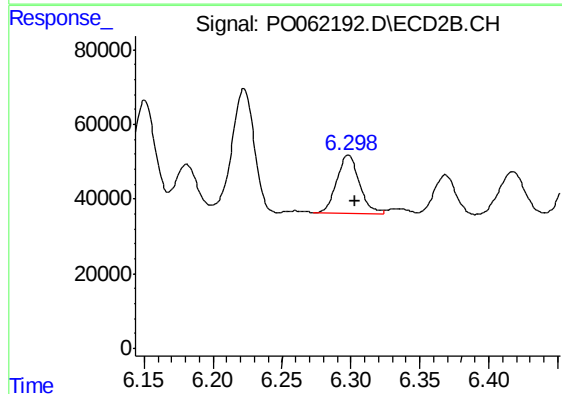


#33 AR-1260-3

R.T.: 6.298 min
Delta R.T.: -0.005 min
Response: 175658
Conc: 77.79 ng/ml

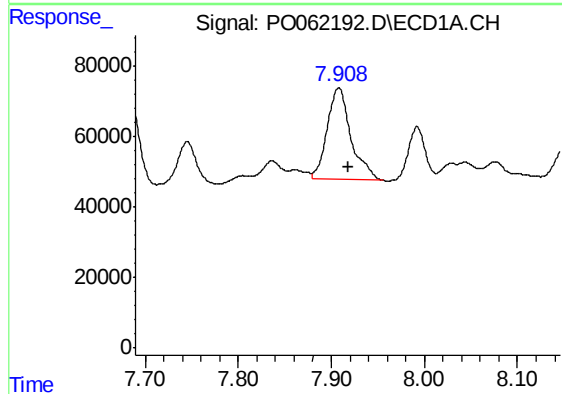


#34 AR-1260-4

R.T.: 7.908 min
Delta R.T.: -0.010 min
Response: 465191
Conc: 166.32 ng/ml m

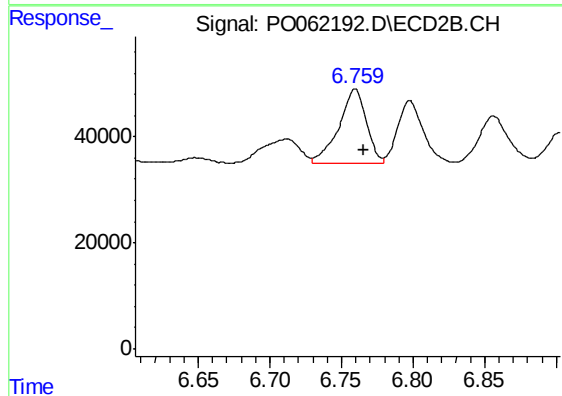

#34 AR-1260-4

R.T.: 6.760 min
Delta R.T.: -0.006 min
Response: 186566
Conc: 106.25 ng/ml

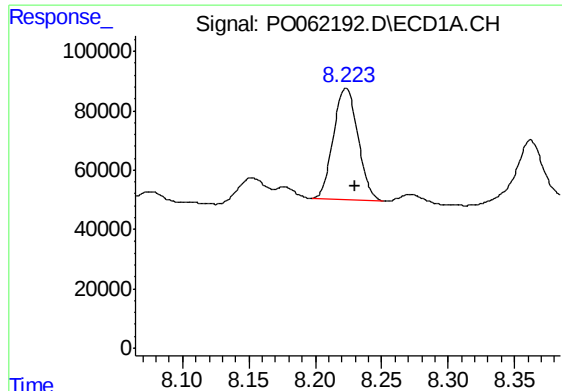


#35 AR-1260-5

R.T.: 8.223 min
Delta R.T.: -0.008 min
Response: 484565
Conc: 92.55 ng/ml m

Instrument :
ECD_O
ClientSampleId :
445X-26A

Manual Integrations
APPROVED

Ankita
10/21/2019 5:03:54 PM

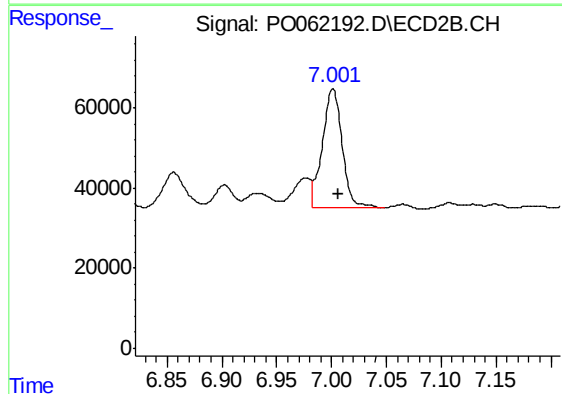

#35 AR-1260-5

R.T.: 7.001 min
Delta R.T.: -0.005 min
Response: 371775
Conc: 103.20 ng/ml