

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101819\
 Data File : P0062199.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Oct 2019 6:07
 Operator : HP/AJ
 Sample : K5428-20
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 445X-14A

Manual Integrations
 APPROVED

Ankita
 10/21/2019 5:04:07 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 06:42:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.321	3.481	1365565	897636	22.080	20.933
2)	SA Decachlor...	9.948	8.330	747891	403429	13.366	13.749
Target Compounds							
26)	L6 AR-1254-1	6.328	5.300	60369	46265	22.647m	18.916
27)	L6 AR-1254-2	6.547	5.444	134389	41613	32.870	19.649 #
28)	L6 AR-1254-3	6.913	5.836	206686	115826	49.398	35.550m#
29)	L6 AR-1254-4	7.197	6.061	110131	89956	36.548	46.575 #
30)	L6 AR-1254-5	7.614	6.469	258112	257881	82.361m	97.638

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101819\
Data File : PO062199.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Oct 2019 6:07
Operator : HP/AJ
Sample : K5428-20
Misc :
ALS Vial : 52 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
445X-14A


Manual Integrations
APPROVED

Ankita
10/21/2019 5:04:07 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 06:42:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

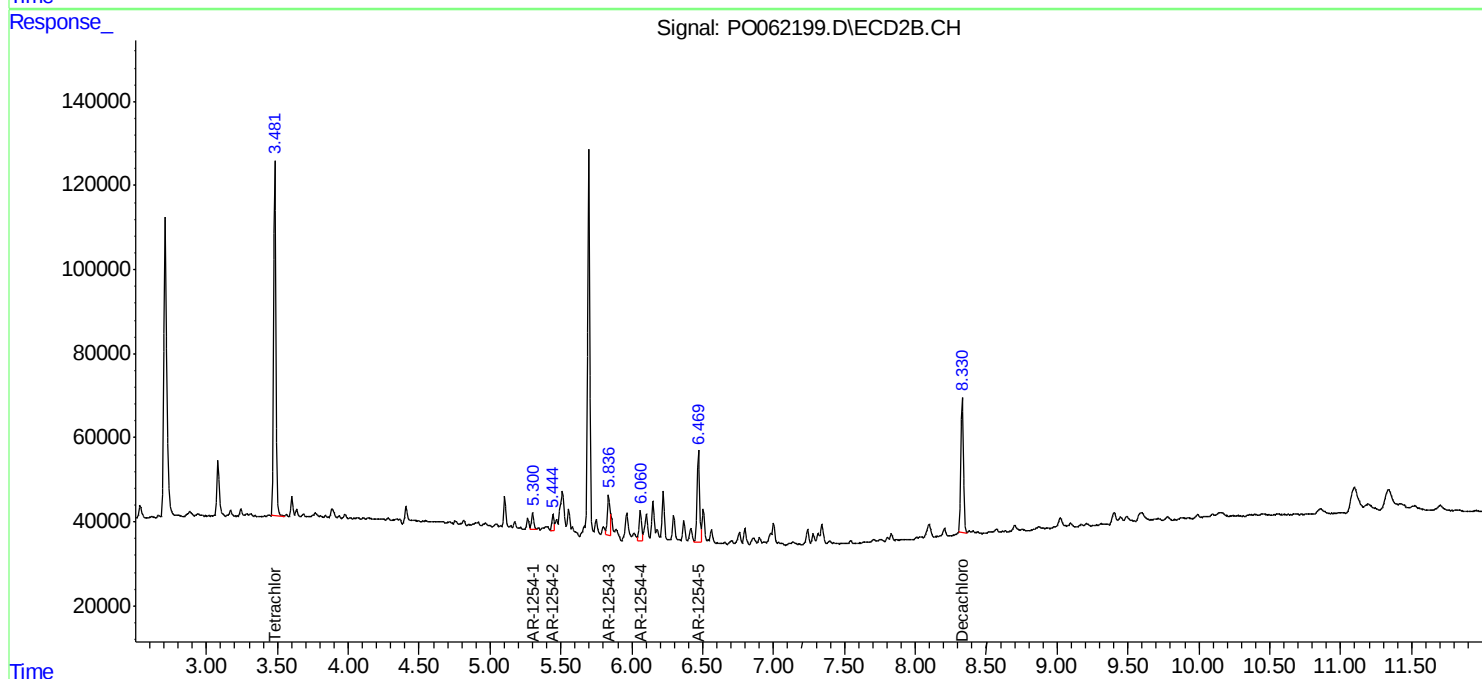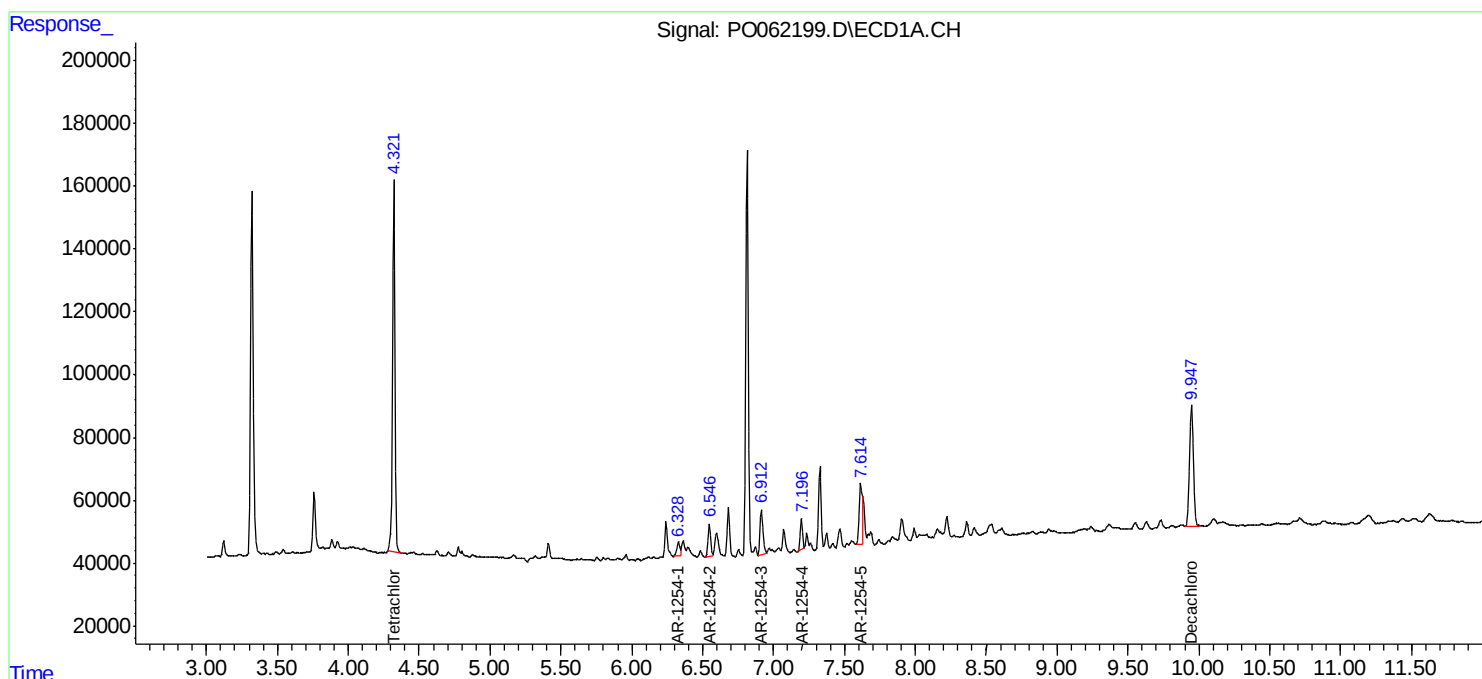

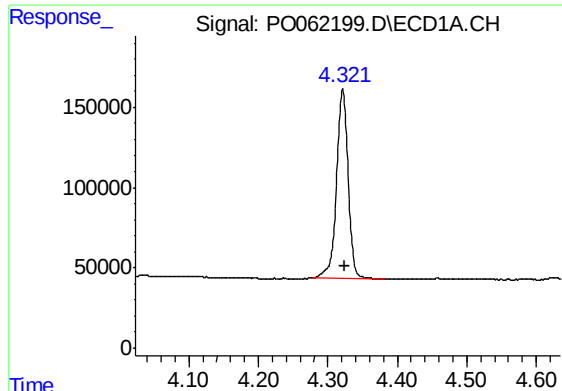


#1 Tetrachloro-m-xylene

R.T.: 4.321 min
Delta R.T.: -0.004 min
Response: 1365565
Conc: 22.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
445X-14A


Manual Integrations
APPROVED

Ankita
10/21/2019 5:04:07 PM

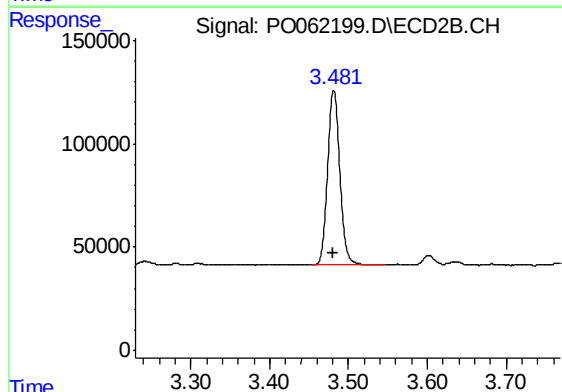


#1 Tetrachloro-m-xylene

R.T.: 3.481 min
Delta R.T.: 0.000 min
Response: 897636
Conc: 20.93 ng/ml

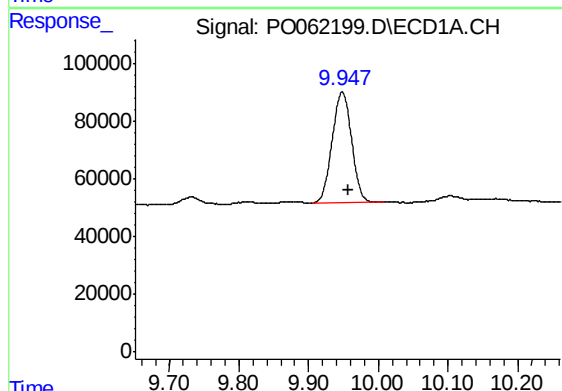


#2 Decachlorobiphenyl

R.T.: 9.948 min
Delta R.T.: -0.008 min
Response: 747891
Conc: 13.37 ng/ml

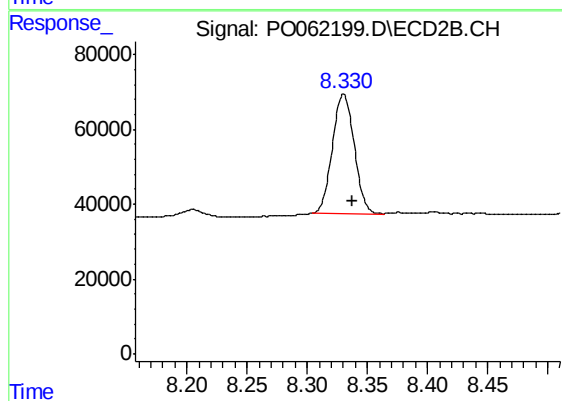

#2 Decachlorobiphenyl

R.T.: 8.330 min
Delta R.T.: -0.008 min
Response: 403429
Conc: 13.75 ng/ml

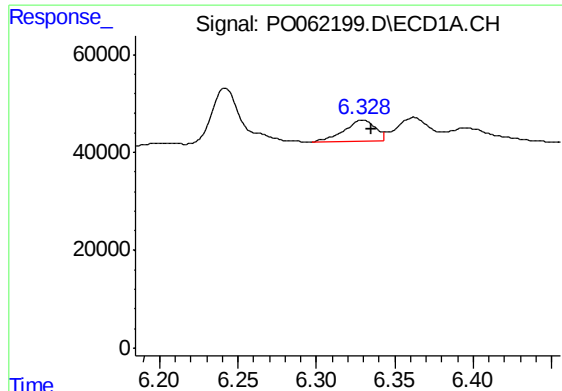


#26 AR-1254-1

R.T.: 6.328 min
Delta R.T.: -0.007 min
Response: 60369
Conc: 22.65 ng/ml m

Instrument :
ECD_O
ClientSampleId :
445X-14A


Manual Integrations
APPROVED

Ankita
10/21/2019 5:04:07 PM

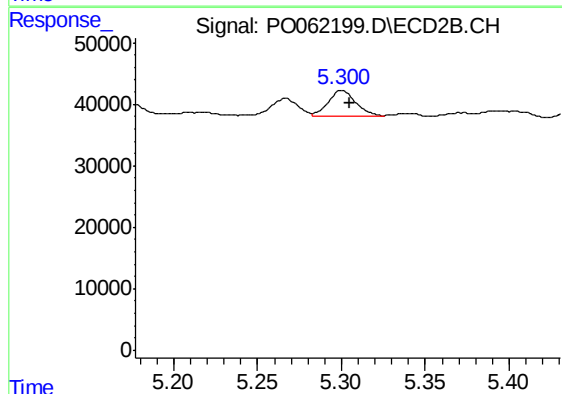


#26 AR-1254-1

R.T.: 5.300 min
Delta R.T.: -0.005 min
Response: 46265
Conc: 18.92 ng/ml

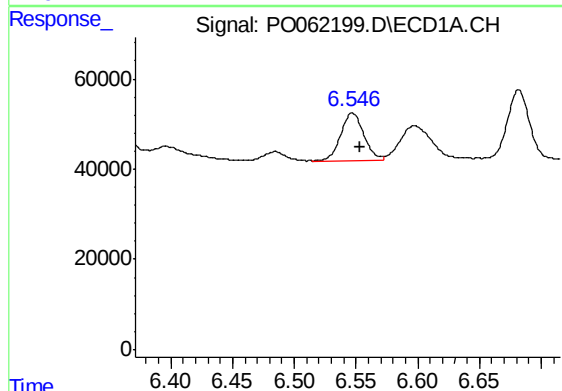


#27 AR-1254-2

R.T.: 6.547 min
Delta R.T.: -0.006 min
Response: 134389
Conc: 32.87 ng/ml

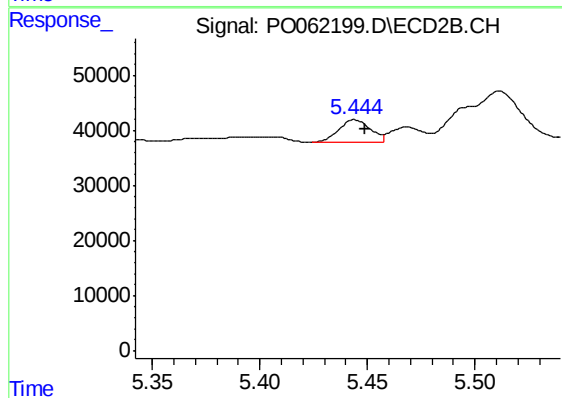

#27 AR-1254-2

R.T.: 5.444 min
Delta R.T.: -0.005 min
Response: 41613
Conc: 19.65 ng/ml

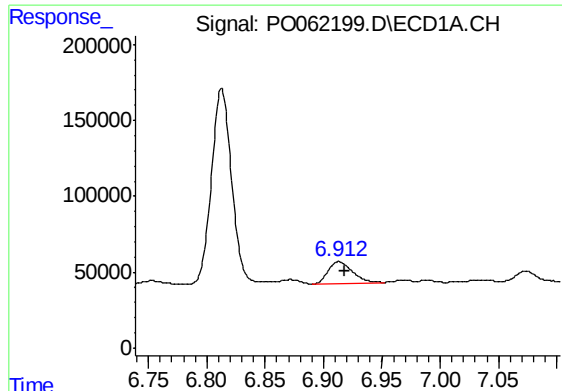


#28 AR-1254-3

R.T.: 6.913 min
Delta R.T.: -0.005 min
Response: 206686
Conc: 49.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
445X-14A


Manual Integrations
APPROVED

Ankita
10/21/2019 5:04:07 PM

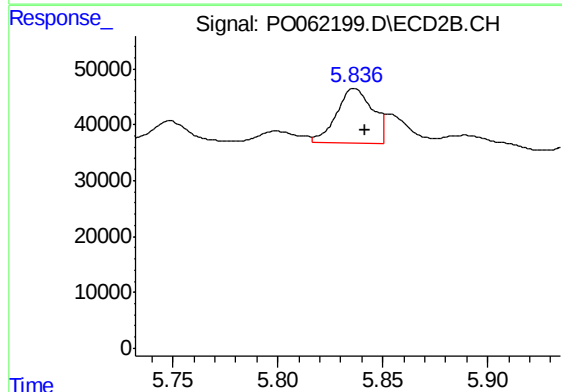


#28 AR-1254-3

R.T.: 5.836 min
Delta R.T.: -0.006 min
Response: 115826
Conc: 35.55 ng/ml m

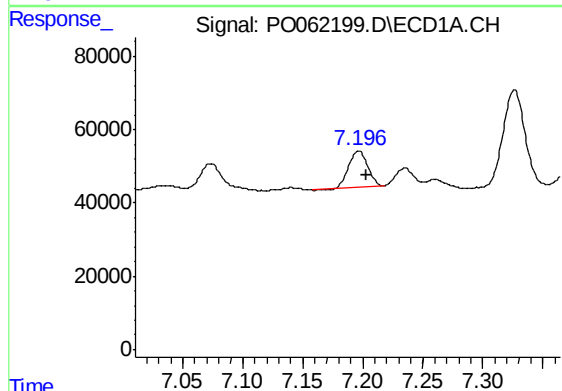


#29 AR-1254-4

R.T.: 7.197 min
Delta R.T.: -0.006 min
Response: 110131
Conc: 36.55 ng/ml

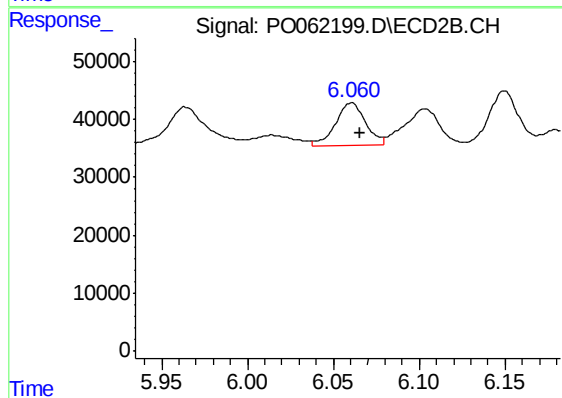

#29 AR-1254-4

R.T.: 6.061 min
Delta R.T.: -0.005 min
Response: 89956
Conc: 46.58 ng/ml

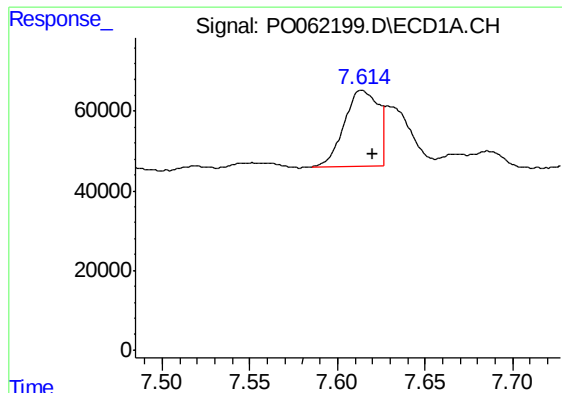


#30 AR-1254-5

R.T.: 7.614 min
Delta R.T.: -0.006 min
Response: 258112
Conc: 82.36 ng/ml m

Instrument :
ECD_O
ClientSampleId :
445X-14A

Manual Integrations
APPROVED

Ankita
10/21/2019 5:04:07 PM

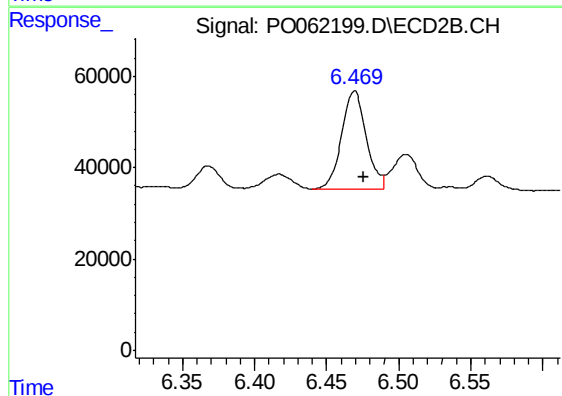

#30 AR-1254-5

R.T.: 6.469 min
Delta R.T.: -0.006 min
Response: 257881
Conc: 97.64 ng/ml