

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101819\
 Data File : P0062220.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Oct 2019 11:51
 Operator : HP/AJ
 Sample : K5431-17
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 445X-DUP-1

Manual Integrations
 APPROVED

Ankita
 10/21/2019 5:04:26 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 00:56:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.322	3.481	1328956	913714	21.488	21.308m
2)	SA Decachlor...	9.949	8.331	742905	452038	13.277	15.406m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101819\
Data File : PO062220.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Oct 2019 11:51
Operator : HP/AJ
Sample : K5431-17
Misc :
ALS Vial : 71 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
445X-DUP-1


Manual Integrations
APPROVED

Ankita
10/21/2019 5:04:26 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 00:56:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

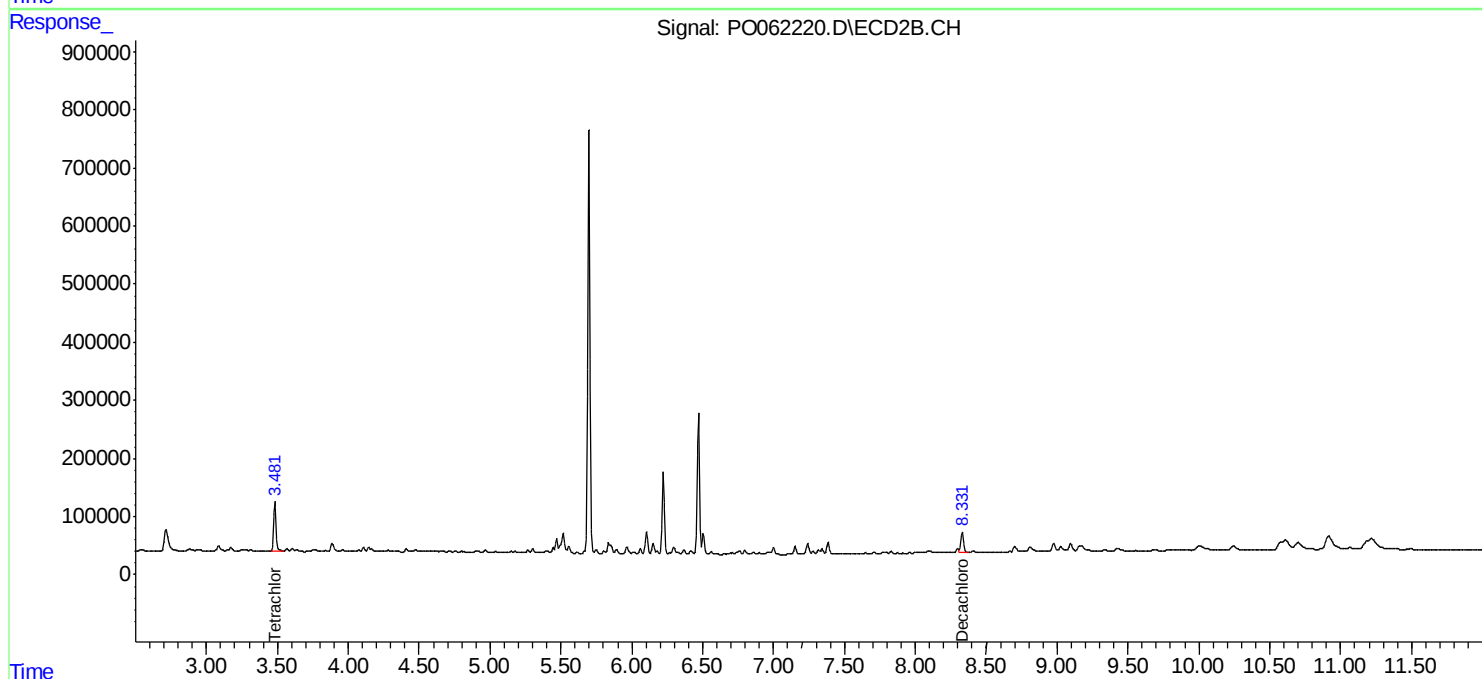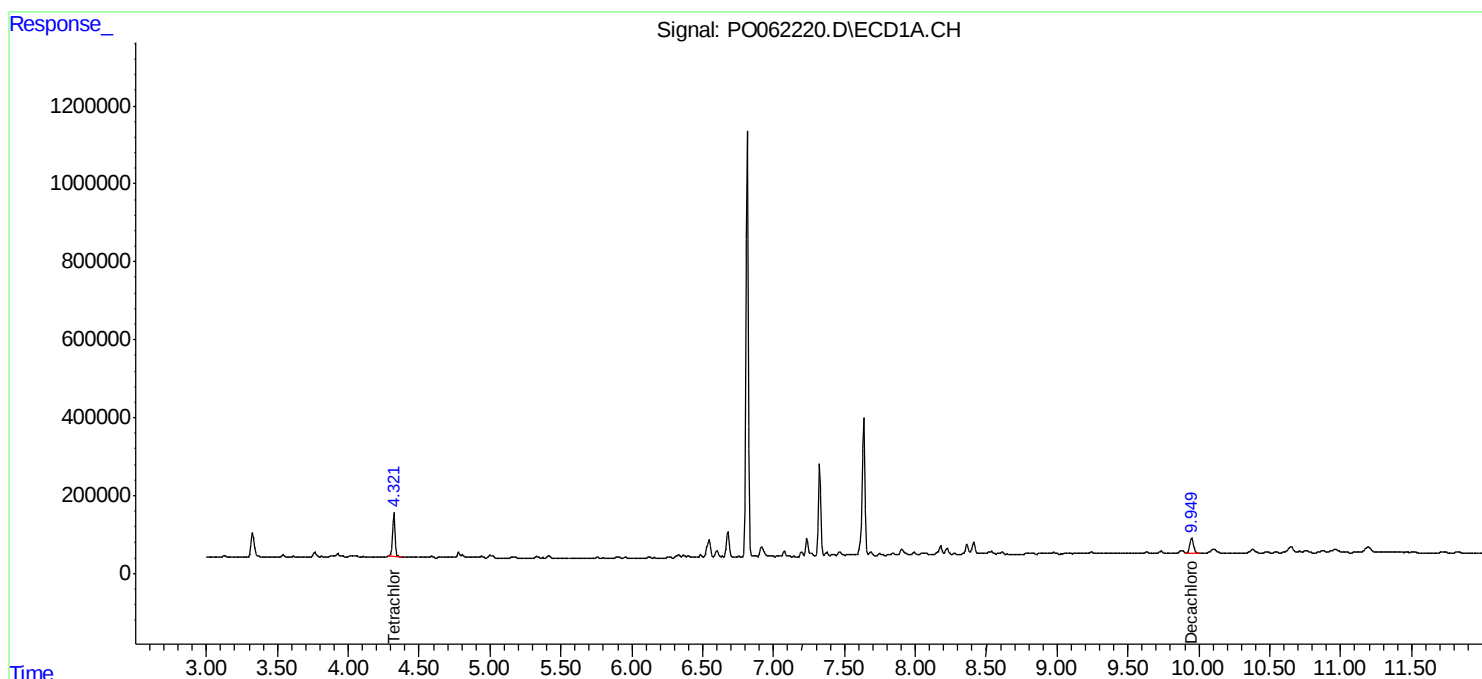

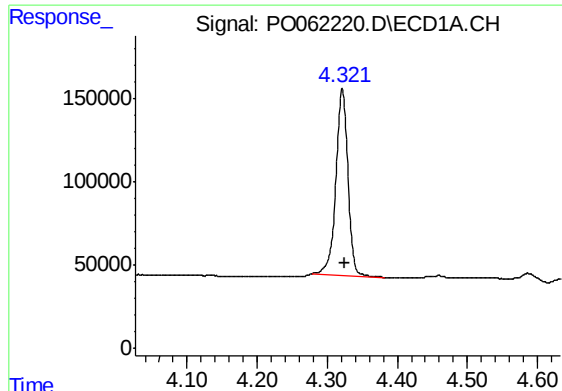

#1 Tetrachloro-m-xylene

R.T.: 4.322 min
Delta R.T.: -0.003 min
Response: 1328956
Conc: 21.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
445X-DUP-1

Manual Integrations
APPROVED

Ankita
10/21/2019 5:04:26 PM

#1 Tetrachloro-m-xylene

R.T.: 3.481 min
Delta R.T.: 0.000 min
Response: 913714
Conc: 21.31 ng/ml m

#2 Decachlorobiphenyl

R.T.: 9.949 min
Delta R.T.: -0.008 min
Response: 742905
Conc: 13.28 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.331 min
Delta R.T.: -0.007 min
Response: 452038
Conc: 15.41 ng/ml m