

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101819\
 Data File : P0062222.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Oct 2019 15:21
 Operator : HP/AJ
 Sample : K5428-02DL 4X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 445X-8ADL

Manual Integrations
 APPROVED

Ankita
 10/21/2019 5:04:30 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 00:57:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.312	3.471	221818	180935	3.587	4.219
2)	SA Decachlor...	9.935	8.320	218599	147394	3.907	5.023m#
Target Compounds							
26)	L6 AR-1254-1	6.319	5.292	707048	596036	265.247m	243.698
27)	L6 AR-1254-2	6.537	5.436	1419715	853452	347.248	402.977
28)	L6 AR-1254-3	6.903	5.828	2083362	1597407	497.925	490.279
29)	L6 AR-1254-4	7.187	6.053	1605315	1055936	532.738	546.714
30)	L6 AR-1254-5	7.604	6.462	2800536	2591948	893.627m	981.353

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101819\
Data File : PO062222.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Oct 2019 15:21
Operator : HP/AJ
Sample : K5428-02DL 4X
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
445X-8ADL


Manual Integrations
APPROVED

Ankita
10/21/2019 5:04:30 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 00:57:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

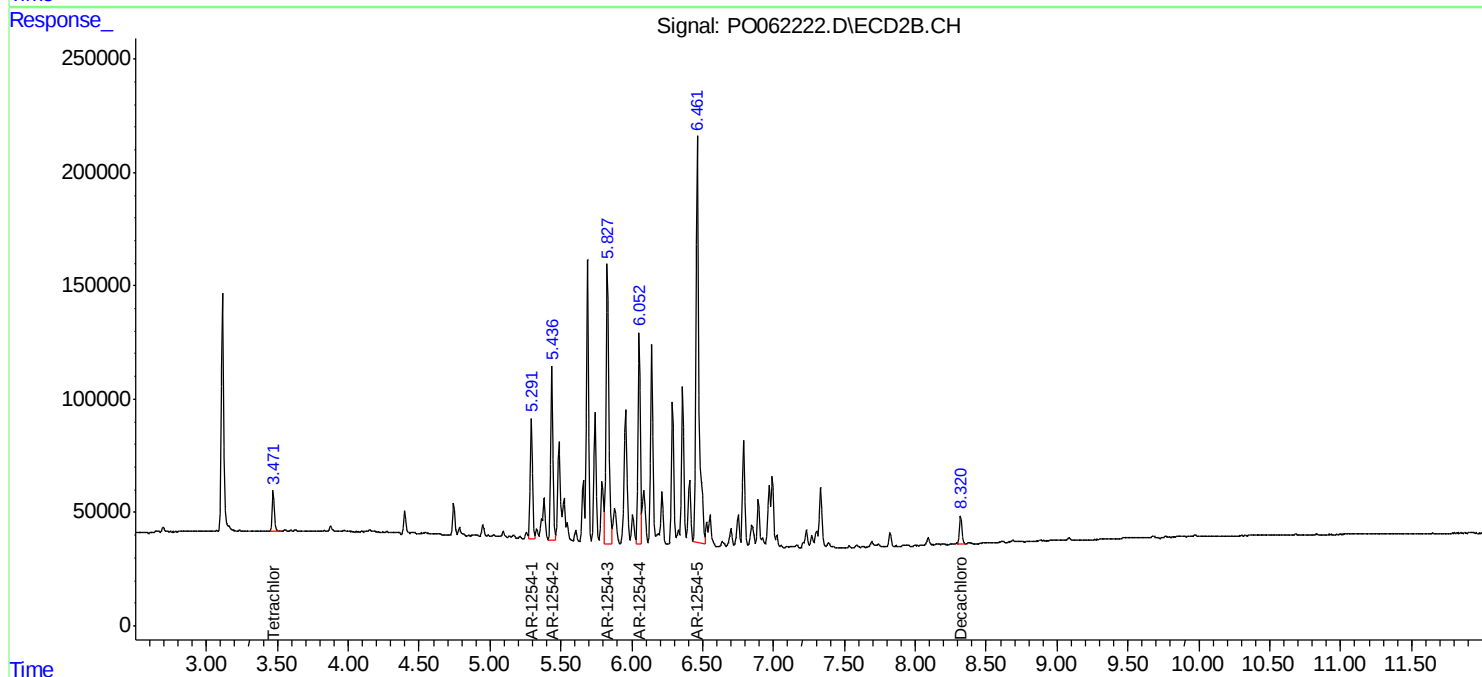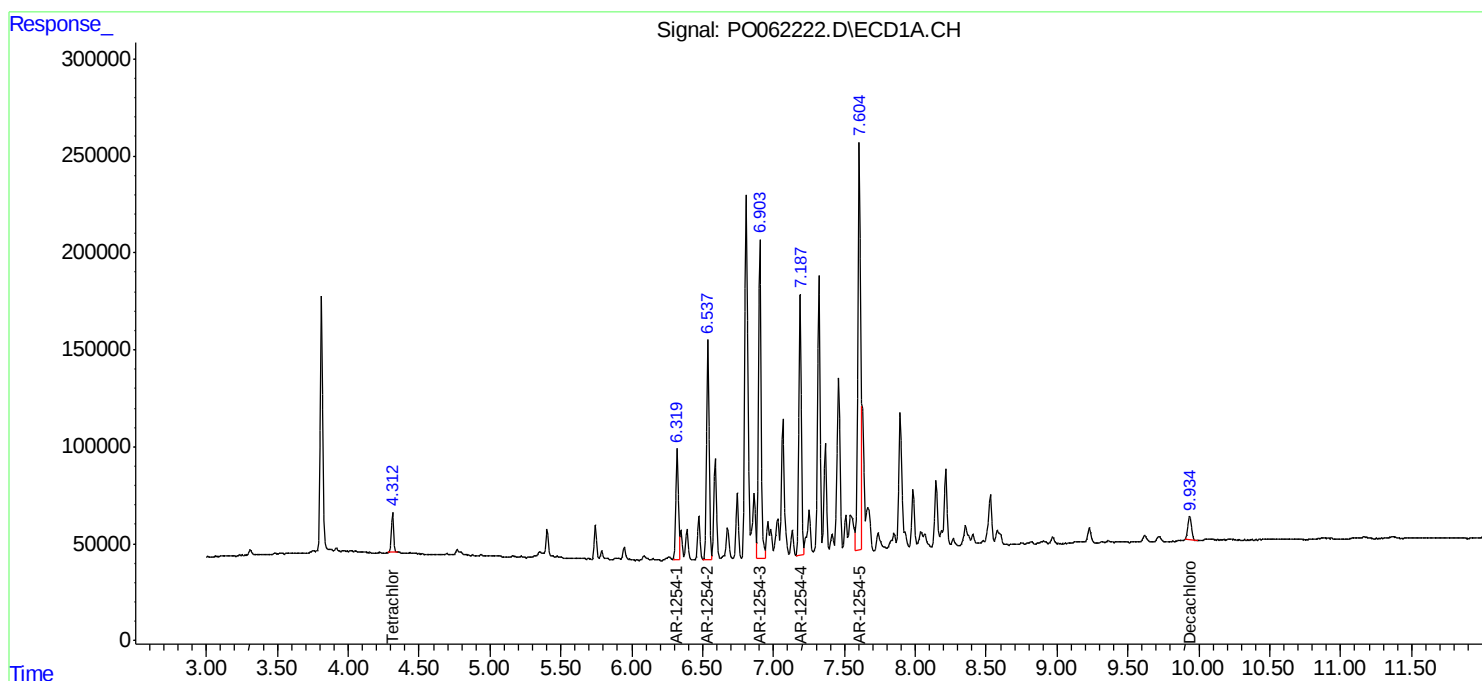

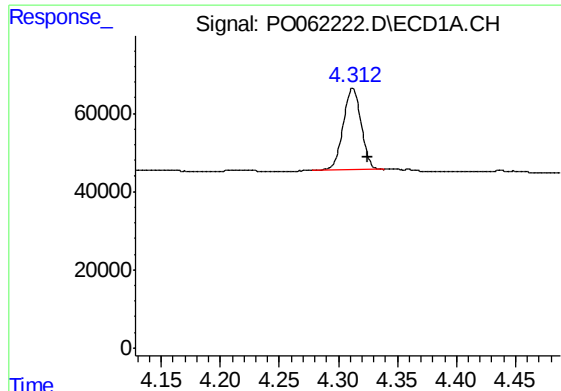


#1 Tetrachloro-m-xylene

R.T.: 4.312 min
Delta R.T.: -0.013 min
Response: 221818
Conc: 3.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
445X-8ADL


Manual Integrations
APPROVED

Ankita
10/21/2019 5:04:30 PM

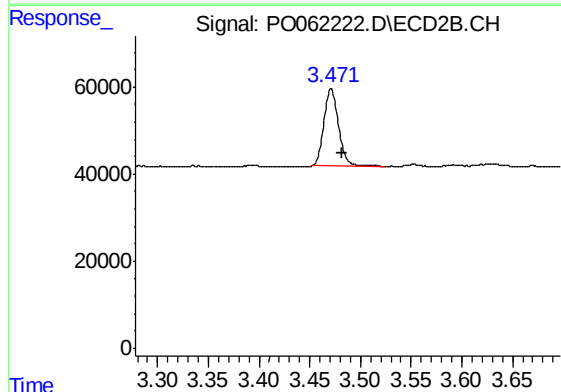


#1 Tetrachloro-m-xylene

R.T.: 3.471 min
Delta R.T.: -0.010 min
Response: 180935
Conc: 4.22 ng/ml

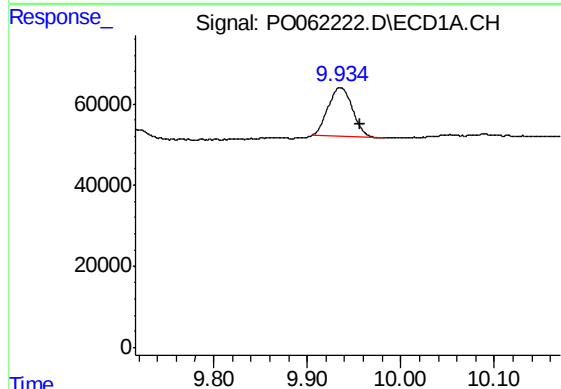


#2 Decachlorobiphenyl

R.T.: 9.935 min
Delta R.T.: -0.021 min
Response: 218599
Conc: 3.91 ng/ml

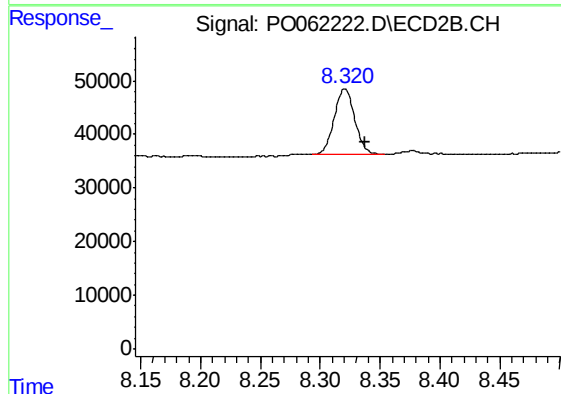

#2 Decachlorobiphenyl

R.T.: 8.320 min
Delta R.T.: -0.018 min
Response: 147394
Conc: 5.02 ng/ml m

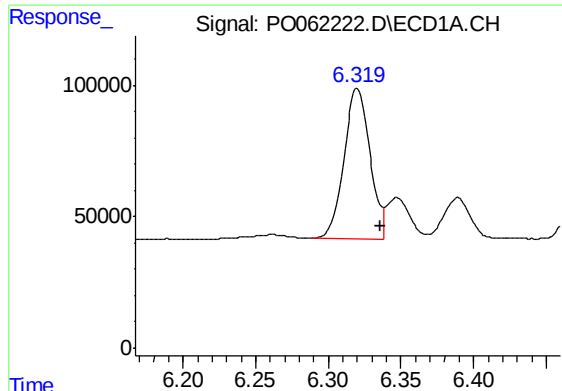


#26 AR-1254-1

R.T.: 6.319 min
Delta R.T.: -0.016 min
Response: 707048
Conc: 265.25 ng/ml m

Instrument :
ECD_O
ClientSampleId :
445X-8ADL


Manual Integrations
APPROVED

Ankita
10/21/2019 5:04:30 PM

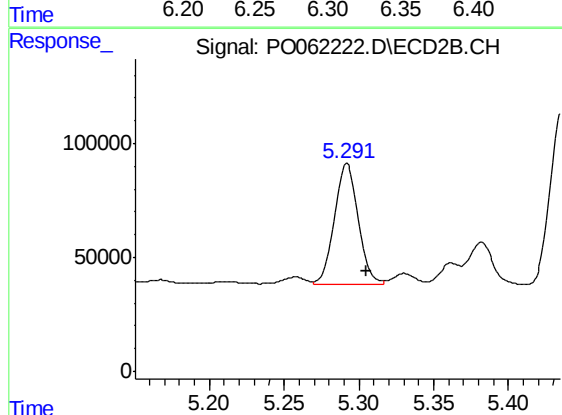


#26 AR-1254-1

R.T.: 5.292 min
Delta R.T.: -0.013 min
Response: 596036
Conc: 243.70 ng/ml

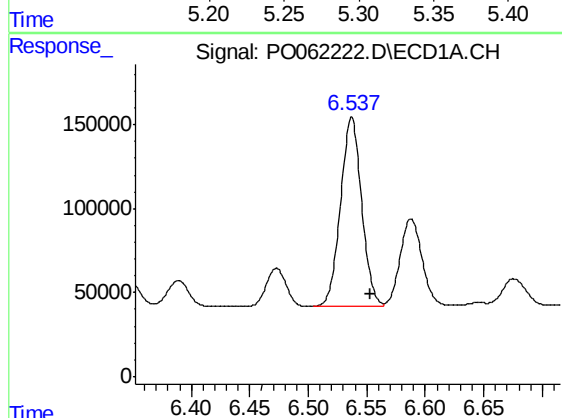


#27 AR-1254-2

R.T.: 6.537 min
Delta R.T.: -0.016 min
Response: 1419715
Conc: 347.25 ng/ml

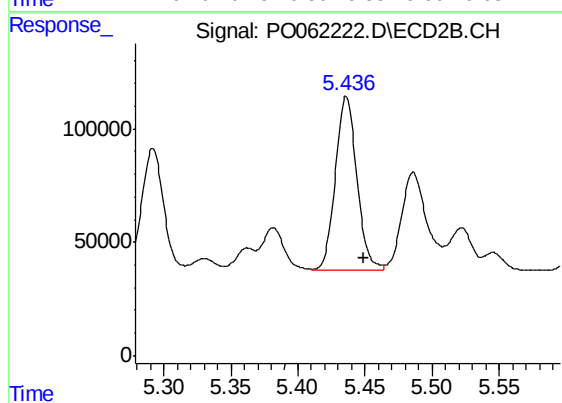

#27 AR-1254-2

R.T.: 5.436 min
Delta R.T.: -0.013 min
Response: 853452
Conc: 402.98 ng/ml

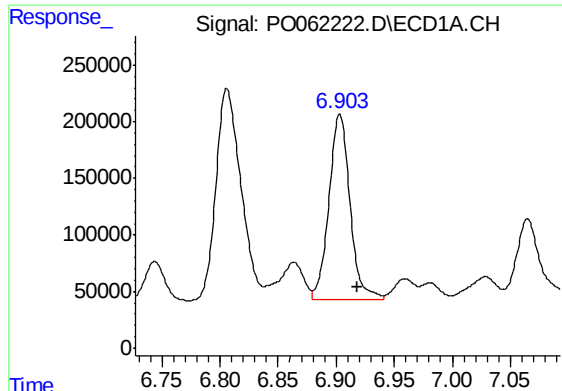


#28 AR-1254-3

R.T.: 6.903 min
Delta R.T.: -0.015 min
Response: 2083362
Conc: 497.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
445X-8ADL


Manual Integrations
APPROVED

Ankita
10/21/2019 5:04:30 PM

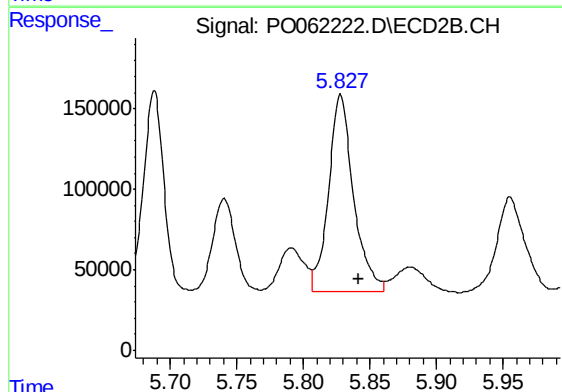


#28 AR-1254-3

R.T.: 5.828 min
Delta R.T.: -0.014 min
Response: 1597407
Conc: 490.28 ng/ml

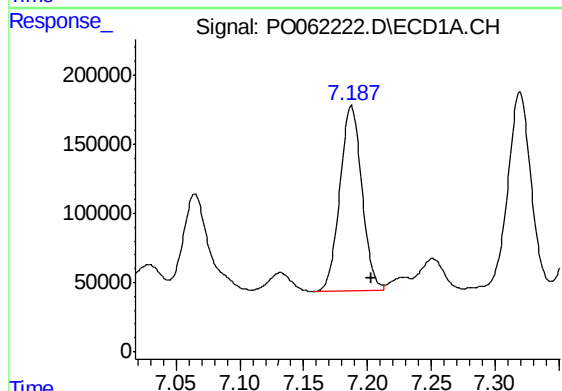


#29 AR-1254-4

R.T.: 7.187 min
Delta R.T.: -0.015 min
Response: 1605315
Conc: 532.74 ng/ml

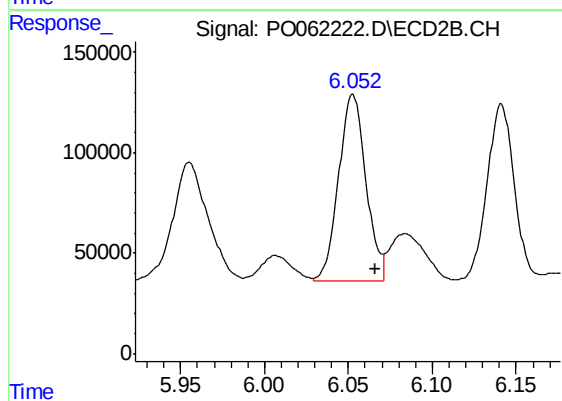

#29 AR-1254-4

R.T.: 6.053 min
Delta R.T.: -0.013 min
Response: 1055936
Conc: 546.71 ng/ml

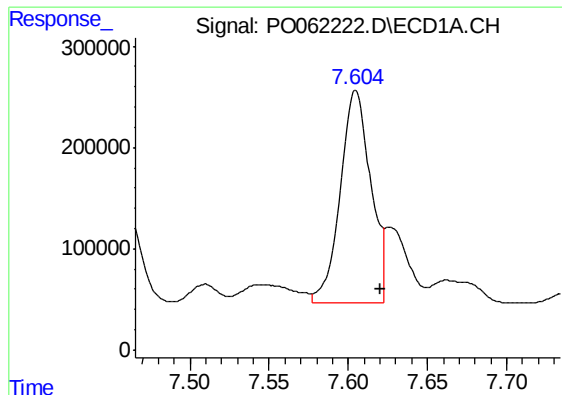


#30 AR-1254-5

R.T.: 7.604 min
Delta R.T.: -0.016 min
Response: 2800536
Conc: 893.63 ng/ml m

Instrument :
ECD_O
ClientSampleId :
445X-8ADL

Manual Integrations
APPROVED

Ankita
10/21/2019 5:04:30 PM

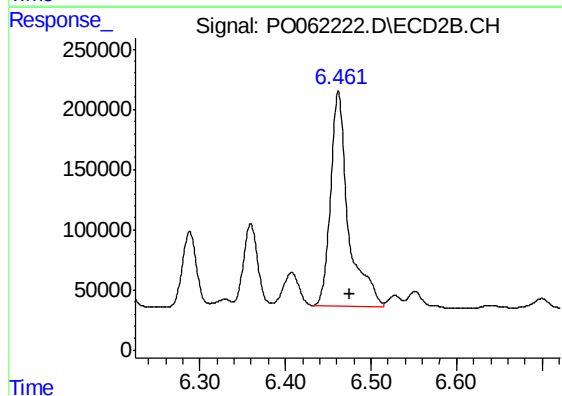

#30 AR-1254-5

R.T.: 6.462 min
Delta R.T.: -0.014 min
Response: 2591948
Conc: 981.35 ng/ml