

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101819\
 Data File : P0062223.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Oct 2019 15:38
 Operator : HP/AJ
 Sample : K5428-05DL 10X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 445X-9ADL

Manual Integrations
 APPROVED

Ankita
 10/21/2019 5:04:32 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 00:57:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.311	3.471	102807	78466	1.662	1.830
2)	SA Decachlor...	9.934	8.321	103534	62439	1.850	2.128m
Target Compounds							
26)	L6 AR-1254-1	6.320	5.291	566452	451927	212.503m	184.777
27)	L6 AR-1254-2	6.537	5.436	1147470	703474	280.659	332.162
28)	L6 AR-1254-3	6.902	5.828	1858001	1409613	444.064	432.641
29)	L6 AR-1254-4	7.187	6.052	1375499	915883	456.472	474.201
30)	L6 AR-1254-5	7.604	6.461	2622964	2457925	836.966m	930.610

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101819\
Data File : PO062223.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Oct 2019 15:38
Operator : HP/AJ
Sample : K5428-05DL 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
445X-9ADL


Manual Integrations
APPROVED

Ankita
10/21/2019 5:04:32 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 00:57:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

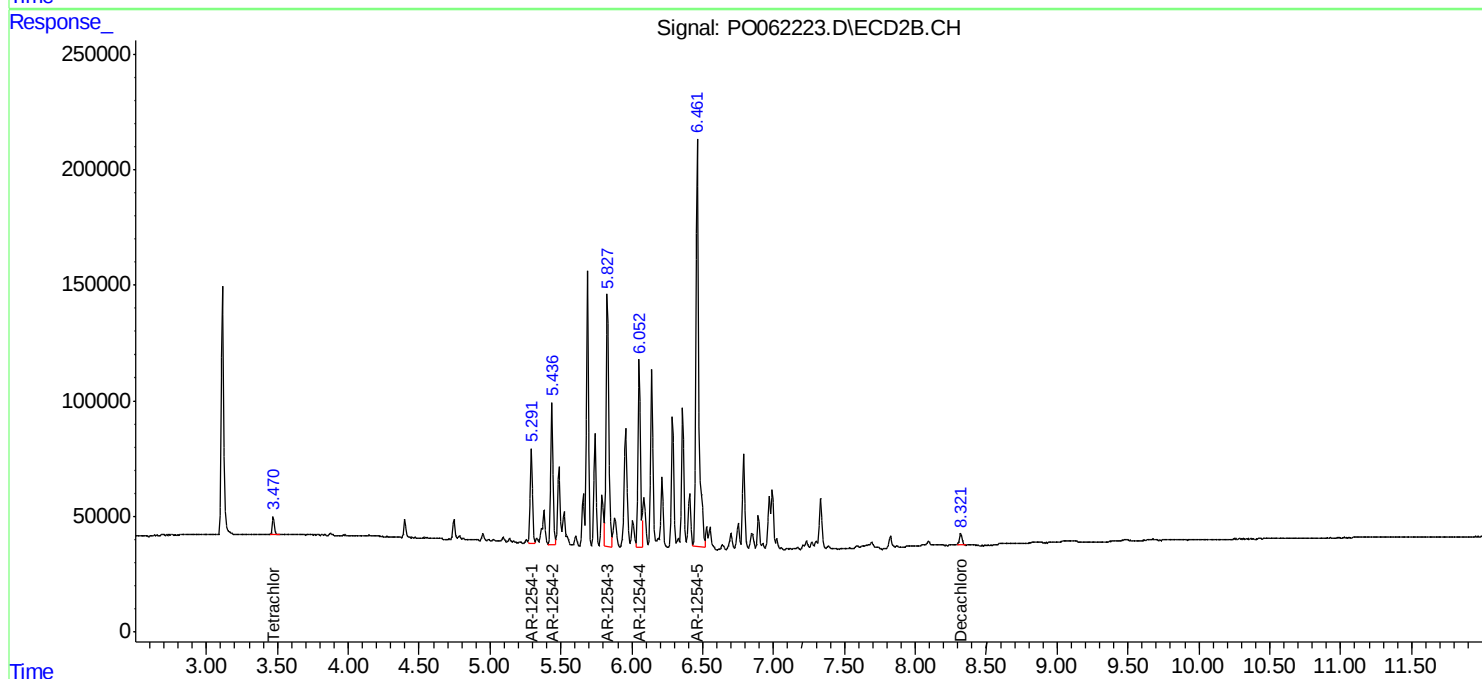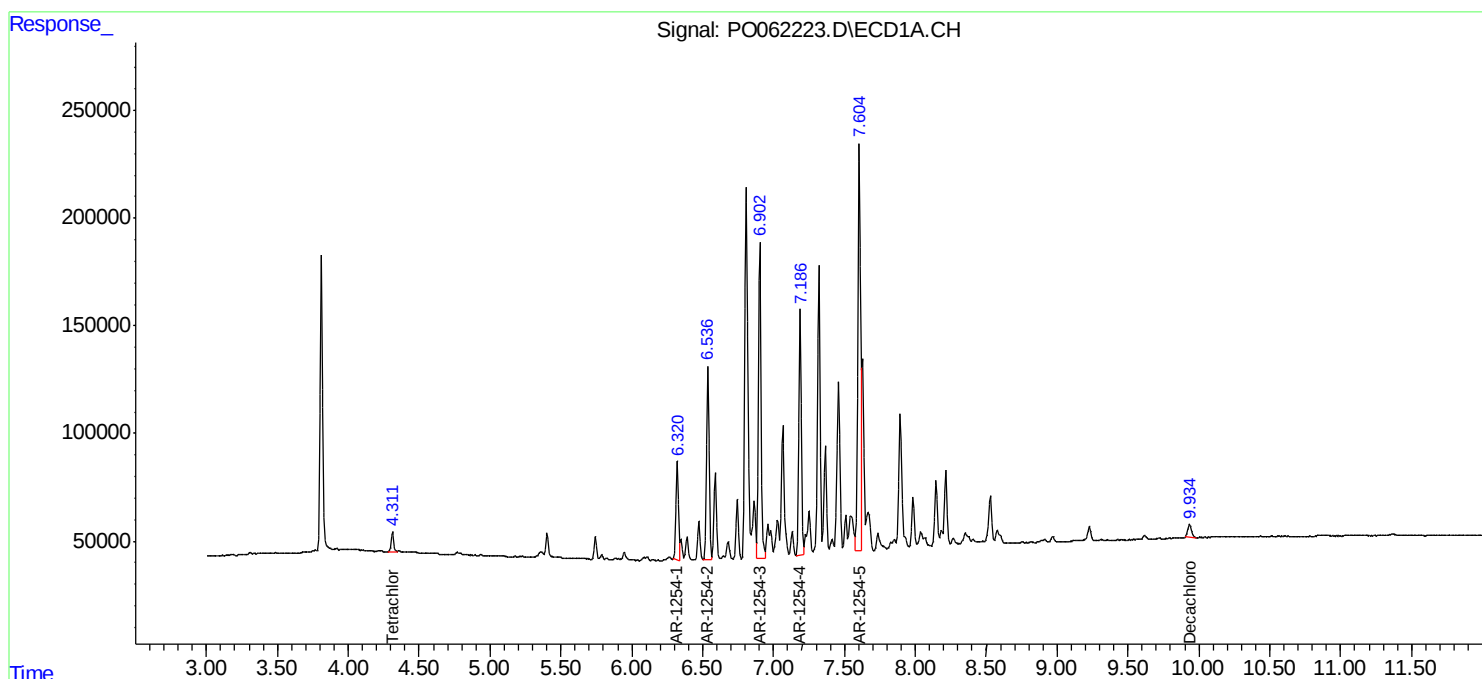

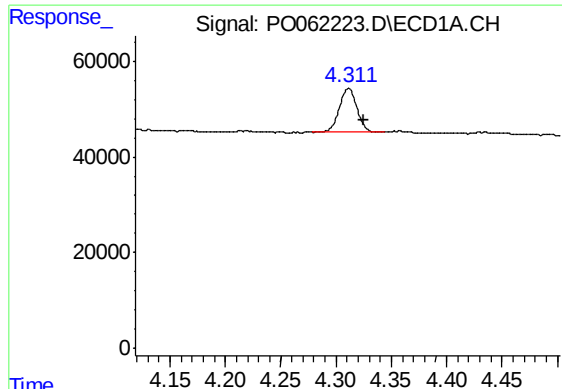


#1 Tetrachloro-m-xylene

R.T.: 4.311 min
Delta R.T.: -0.014 min
Response: 102807
Conc: 1.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
445X-9ADL


Manual Integrations
APPROVED

Ankita
10/21/2019 5:04:32 PM

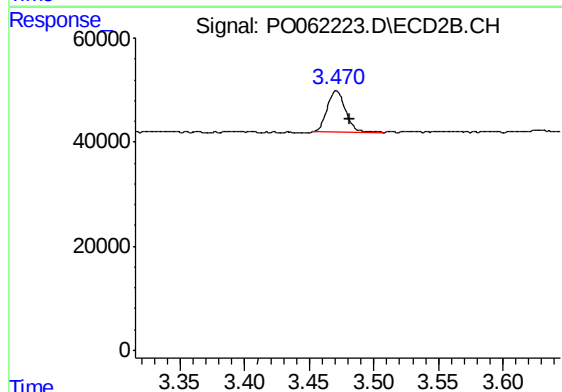


#1 Tetrachloro-m-xylene

R.T.: 3.471 min
Delta R.T.: -0.010 min
Response: 78466
Conc: 1.83 ng/ml

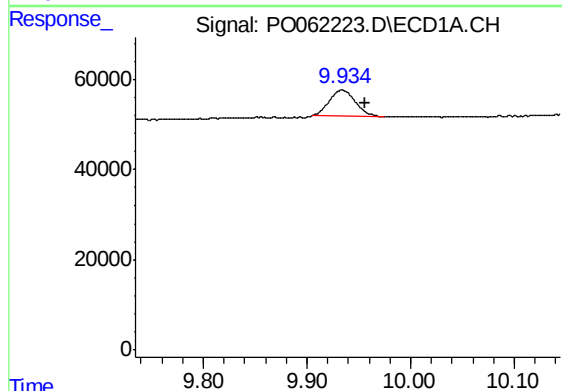


#2 Decachlorobiphenyl

R.T.: 9.934 min
Delta R.T.: -0.023 min
Response: 103534
Conc: 1.85 ng/ml

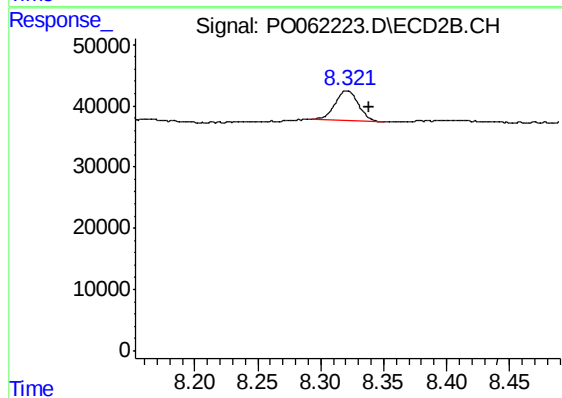

#2 Decachlorobiphenyl

R.T.: 8.321 min
Delta R.T.: -0.017 min
Response: 62439
Conc: 2.13 ng/ml m

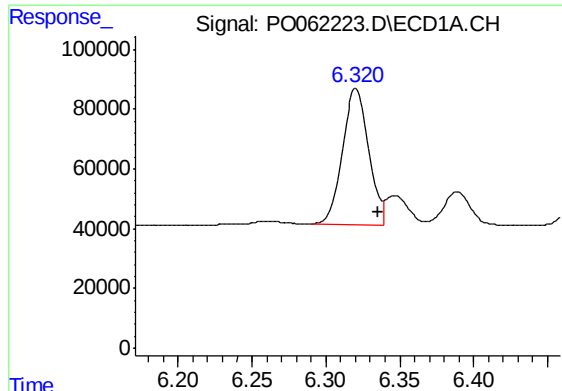


#26 AR-1254-1

R.T.: 6.320 min
Delta R.T.: -0.016 min
Response: 566452
Conc: 212.50 ng/ml m

Instrument :
ECD_O
ClientSampleId :
445X-9ADL


Manual Integrations
APPROVED

Ankita
10/21/2019 5:04:32 PM

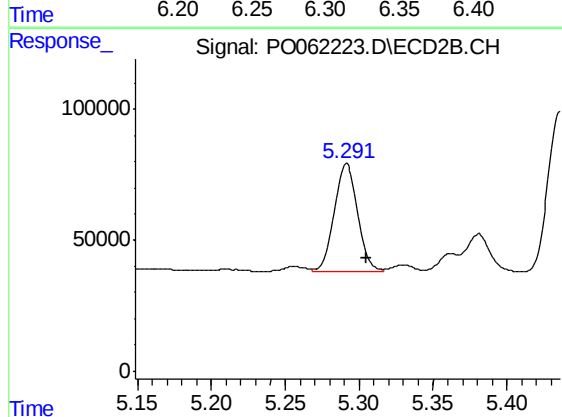


#26 AR-1254-1

R.T.: 5.291 min
Delta R.T.: -0.013 min
Response: 451927
Conc: 184.78 ng/ml

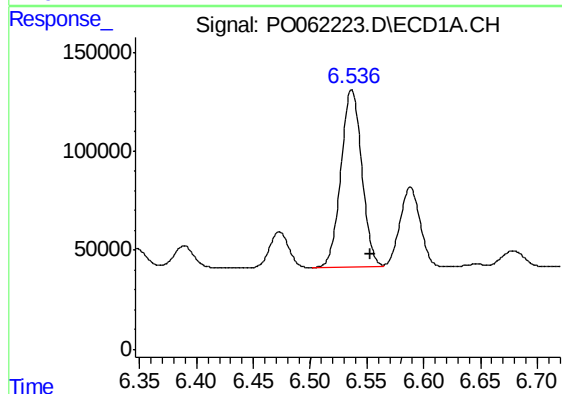


#27 AR-1254-2

R.T.: 6.537 min
Delta R.T.: -0.017 min
Response: 1147470
Conc: 280.66 ng/ml

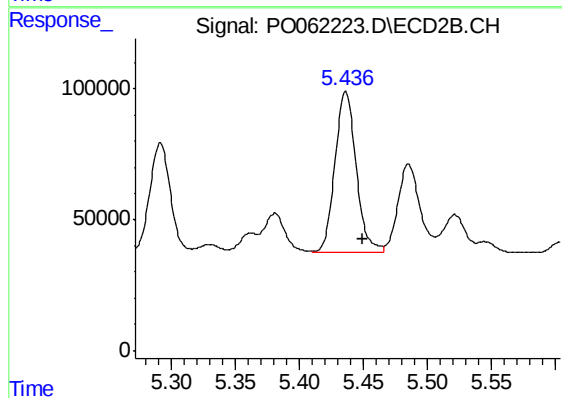

#27 AR-1254-2

R.T.: 5.436 min
Delta R.T.: -0.013 min
Response: 703474
Conc: 332.16 ng/ml

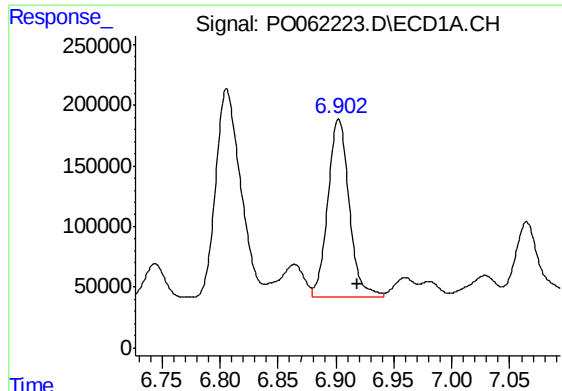


#28 AR-1254-3

R.T.: 6.902 min
Delta R.T.: -0.016 min
Response: 1858001
Conc: 444.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
445X-9ADL


Manual Integrations
APPROVED

Ankita
10/21/2019 5:04:32 PM

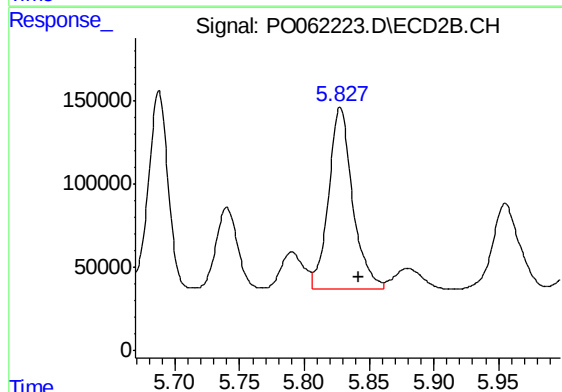


#28 AR-1254-3

R.T.: 5.828 min
Delta R.T.: -0.014 min
Response: 1409613
Conc: 432.64 ng/ml

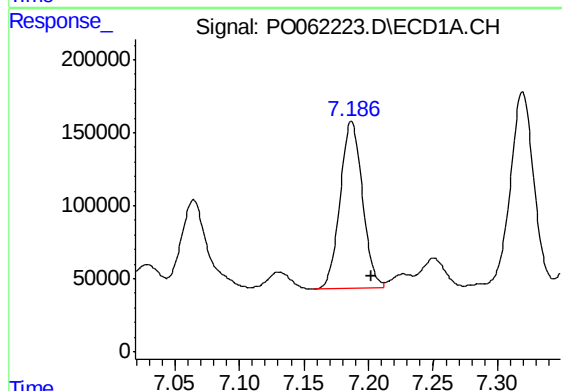


#29 AR-1254-4

R.T.: 7.187 min
Delta R.T.: -0.016 min
Response: 1375499
Conc: 456.47 ng/ml

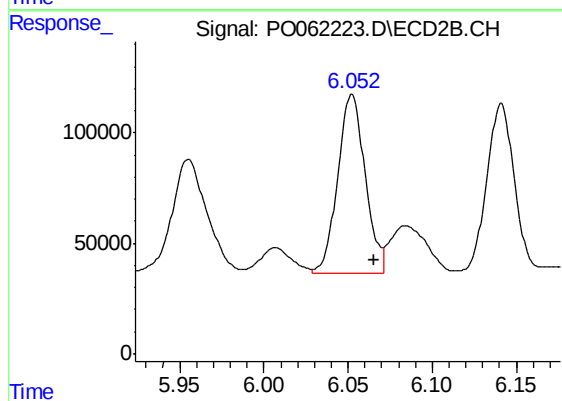

#29 AR-1254-4

R.T.: 6.052 min
Delta R.T.: -0.013 min
Response: 915883
Conc: 474.20 ng/ml

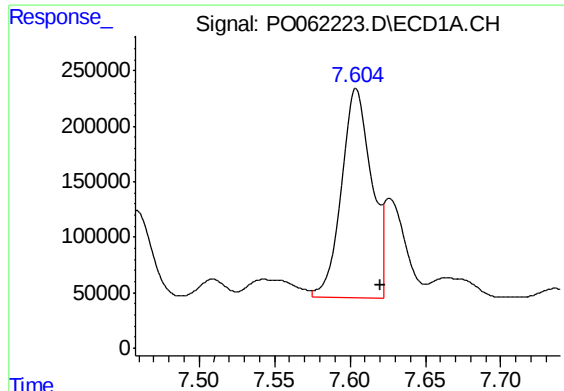


#30 AR-1254-5

R.T.: 7.604 min
Delta R.T.: -0.017 min
Response: 2622964
Conc: 836.97 ng/ml m

Instrument :
ECD_O
ClientSampleId :
445X-9ADL

Manual Integrations
APPROVED

Ankita
10/21/2019 5:04:32 PM

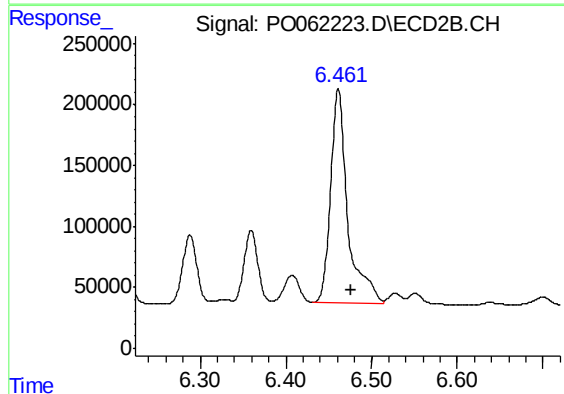

#30 AR-1254-5

R.T.: 6.461 min
Delta R.T.: -0.014 min
Response: 2457925
Conc: 930.61 ng/ml