

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101918\
 Data File : PO050282.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Oct 2018 19:29
 Operator : SM/SJ
 Sample : J5575-18
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SSSI-1015-S-DH-24-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 23:03:22 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101818.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 19 02:02:26 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.363	3.359	5909250	4262487	19.804	21.681
2) SA Decachlor...	10.100	8.116	3296102	3368421	15.190	17.622

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101918\
Data File : PO050282.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Oct 2018 19:29
Operator : SM/SJ
Sample : J5575-18
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SSSI-1015-S-DH-24-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 23:03:22 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101818.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 19 02:02:26 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

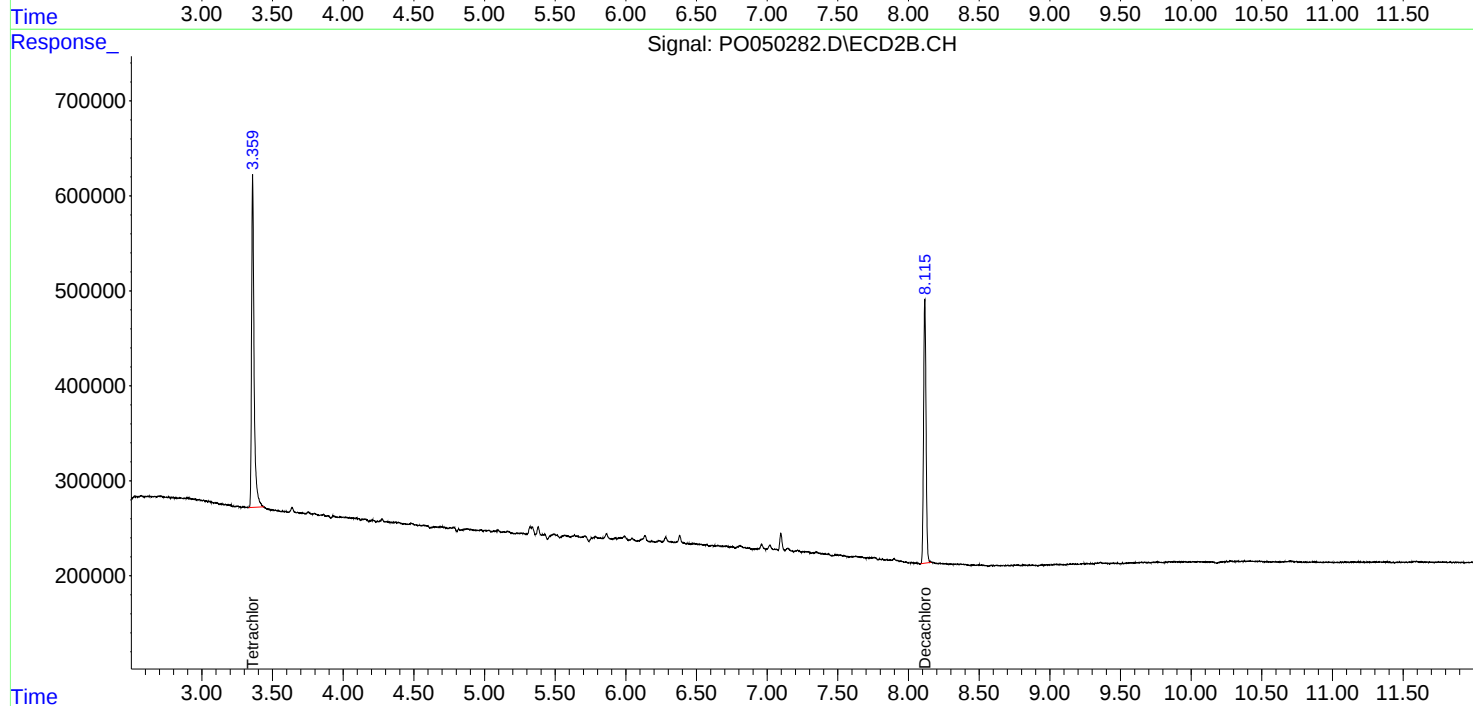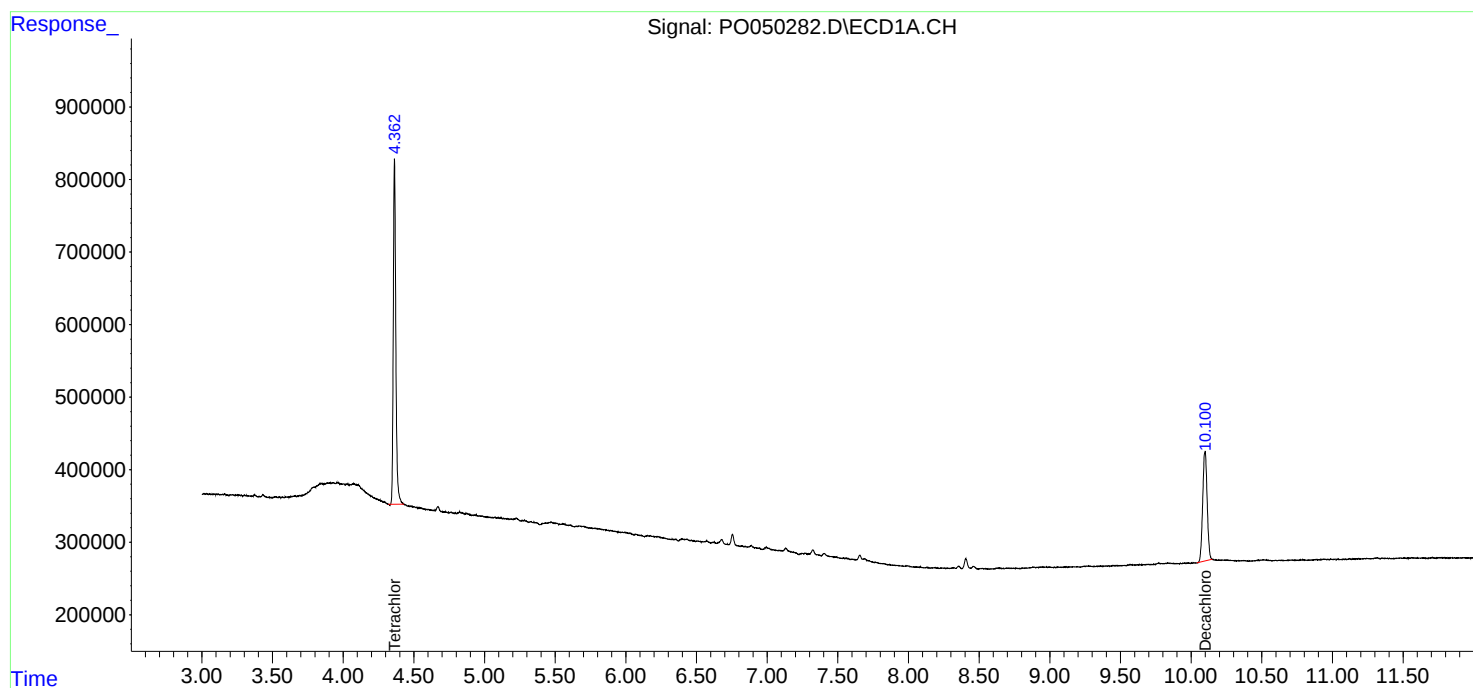


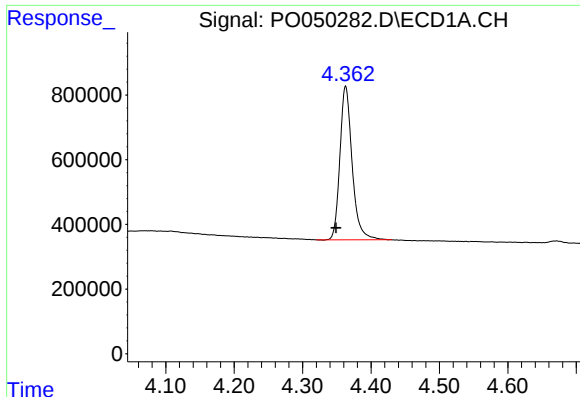

#1 Tetrachloro-m-xylene


R.T.: 4.363 min
Delta R.T.: 0.014 min
Response: 5909250
Conc: 19.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
SSSI-1015-S-DH-24-B

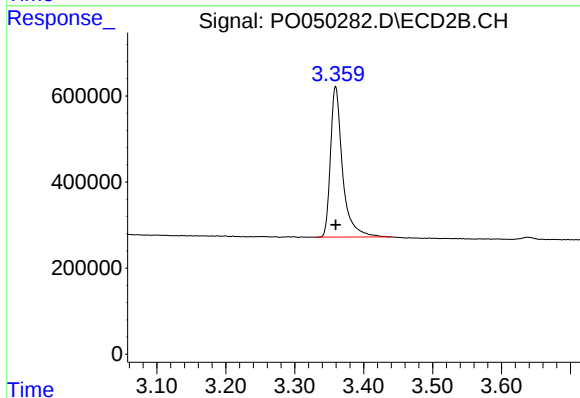


#1 Tetrachloro-m-xylene

R.T.: 3.359 min
Delta R.T.: 0.000 min
Response: 4262487
Conc: 21.68 ng/ml

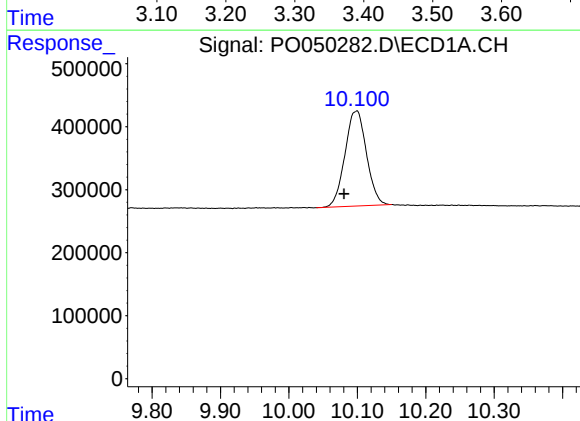

#2 Decachlorobiphenyl

R.T.: 10.100 min
Delta R.T.: 0.019 min
Response: 3296102
Conc: 15.19 ng/ml

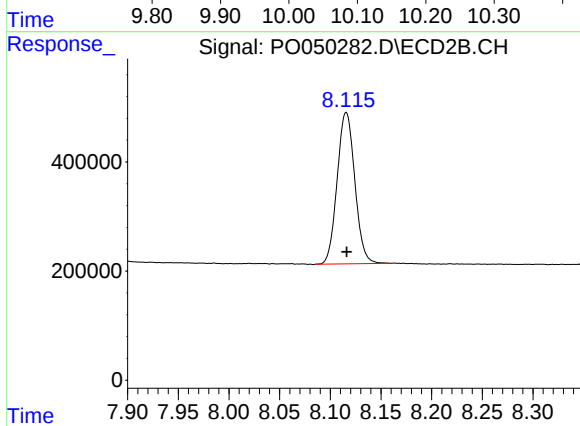

#2 Decachlorobiphenyl

R.T.: 8.116 min
Delta R.T.: 0.000 min
Response: 3368421
Conc: 17.62 ng/ml