

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101918\
 Data File : P0050290.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Oct 2018 22:00
 Operator : SM/SJ
 Sample : J5575-12
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SSSI-1015-S-DH-25-T

Manual Integrations
 APPROVED

sohil
 10/22/2018 5:10:04 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 23:05:44 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101818.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 19 02:02:26 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.364	3.359	4726493	3433063	15.840	17.462
2) SA Decachlor...	10.100	8.115	3115880	3171125	14.360m	16.590

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101918\
Data File : P0050290.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Oct 2018 22:00
Operator : SM/SJ
Sample : J5575-12
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SSSI-1015-S-DH-25-T


Manual Integrations
APPROVED

sohil
10/22/2018 5:10:04 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 23:05:44 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101818.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 19 02:02:26 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

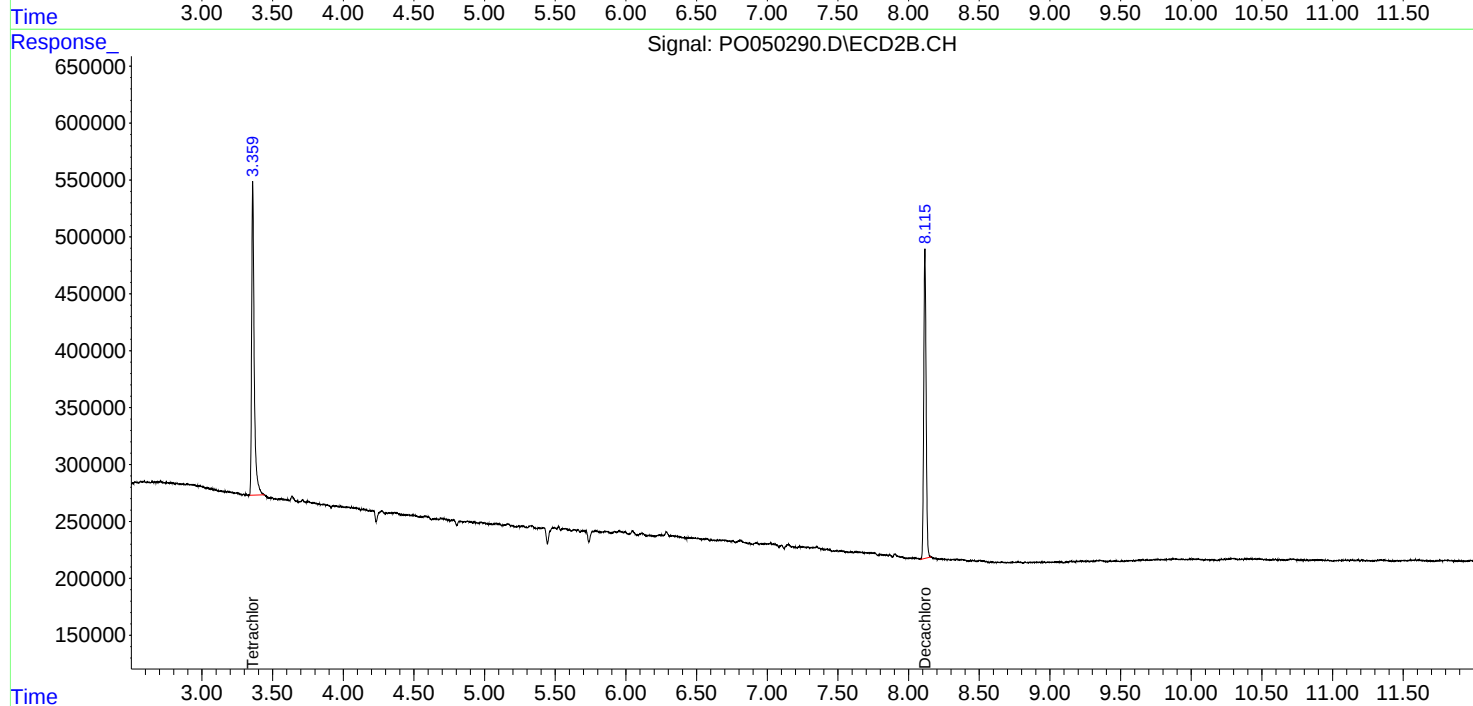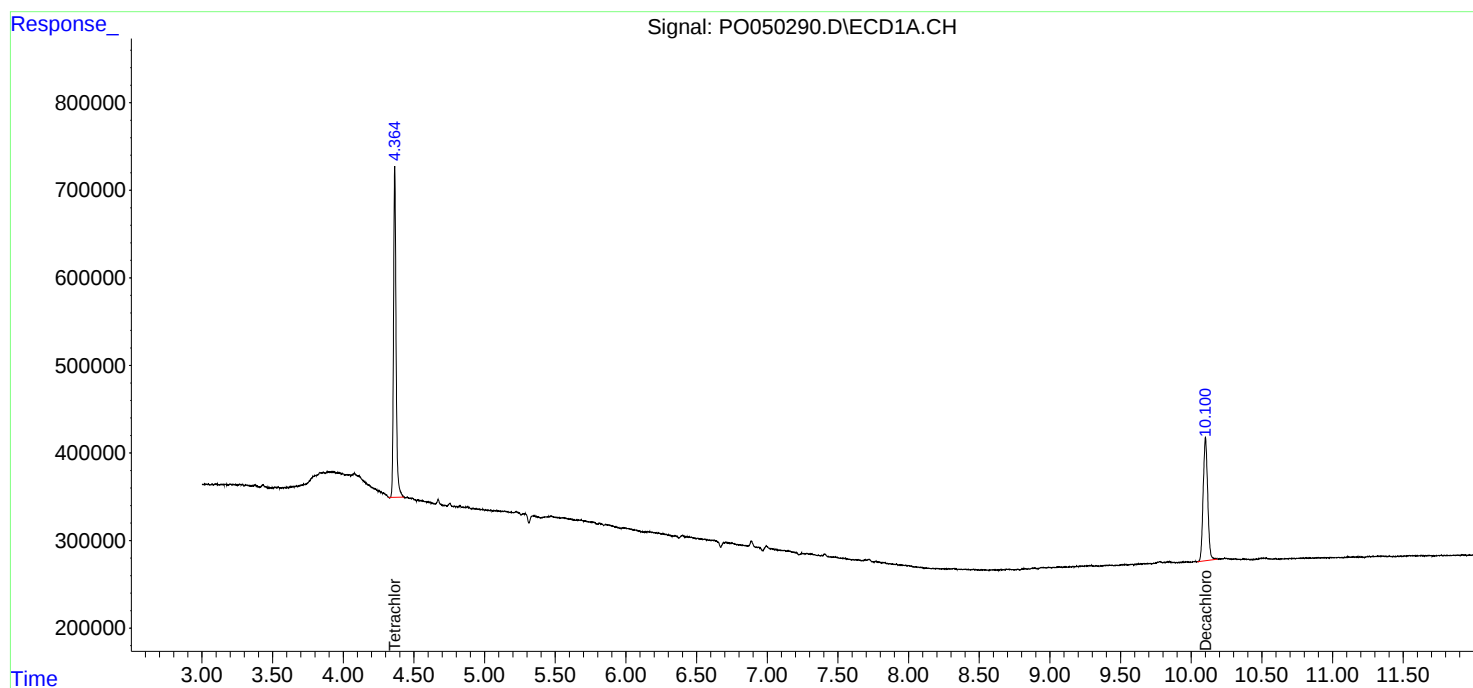

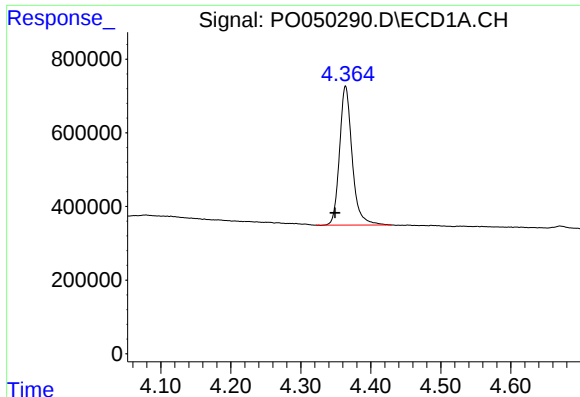


#1 Tetrachloro-m-xylene

R.T.: 4.364 min
Delta R.T.: 0.015 min
Response: 4726493
Conc: 15.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
SSSI-1015-S-DH-25-T


Manual Integrations
APPROVED

sohil
10/22/2018 5:10:04 PM

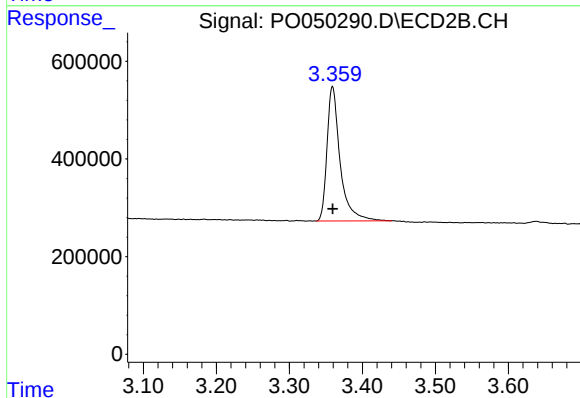


#1 Tetrachloro-m-xylene

R.T.: 3.359 min
Delta R.T.: 0.000 min
Response: 3433063
Conc: 17.46 ng/ml

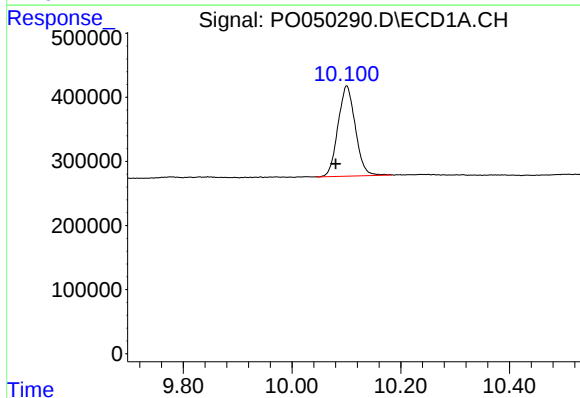

#2 Decachlorobiphenyl

R.T.: 10.100 min
Delta R.T.: 0.020 min
Response: 3115880
Conc: 14.36 ng/ml m

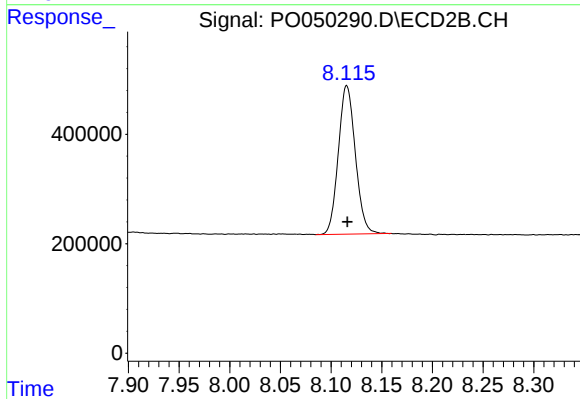

#2 Decachlorobiphenyl

R.T.: 8.115 min
Delta R.T.: 0.000 min
Response: 3171125
Conc: 16.59 ng/ml