

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101918\
 Data File : P0050299.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Oct 2018 1:47
 Operator : SM/SJ
 Sample : J5585-06
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SSSI-1017-S-DH-19A

Manual Integrations
 APPROVED

sohil
 10/22/2018 5:10:13 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 04:35:01 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101818.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 19 02:02:26 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.366	3.359	6259349	4658295	20.977	23.694
2) SA Decachlor...	10.103	8.116	3744669	3904492	17.258m	20.427

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101918\
Data File : PO050299.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Oct 2018 1:47
Operator : SM/SJ
Sample : J5585-06
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SSSI-1017-S-DH-19A


Manual Integrations
APPROVED

sohil
10/22/2018 5:10:13 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 04:35:01 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101818.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 19 02:02:26 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

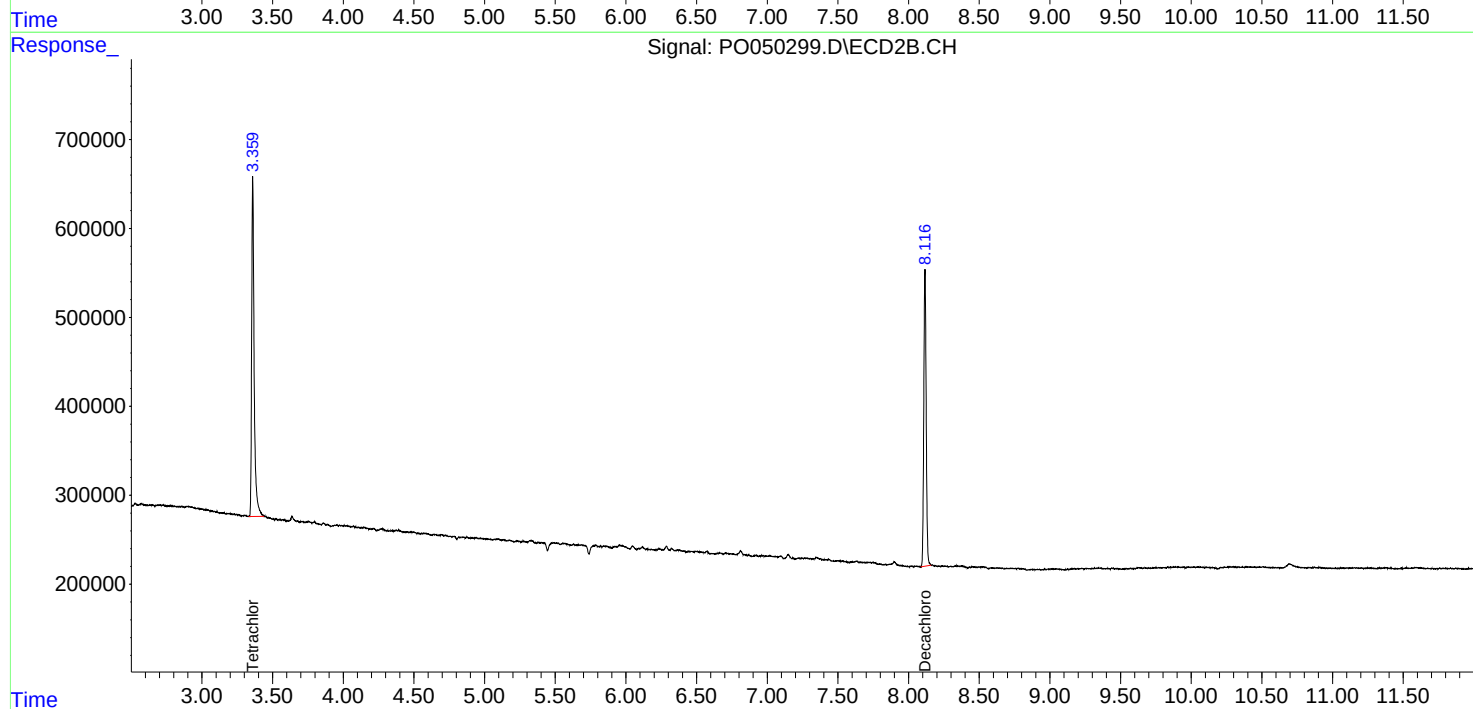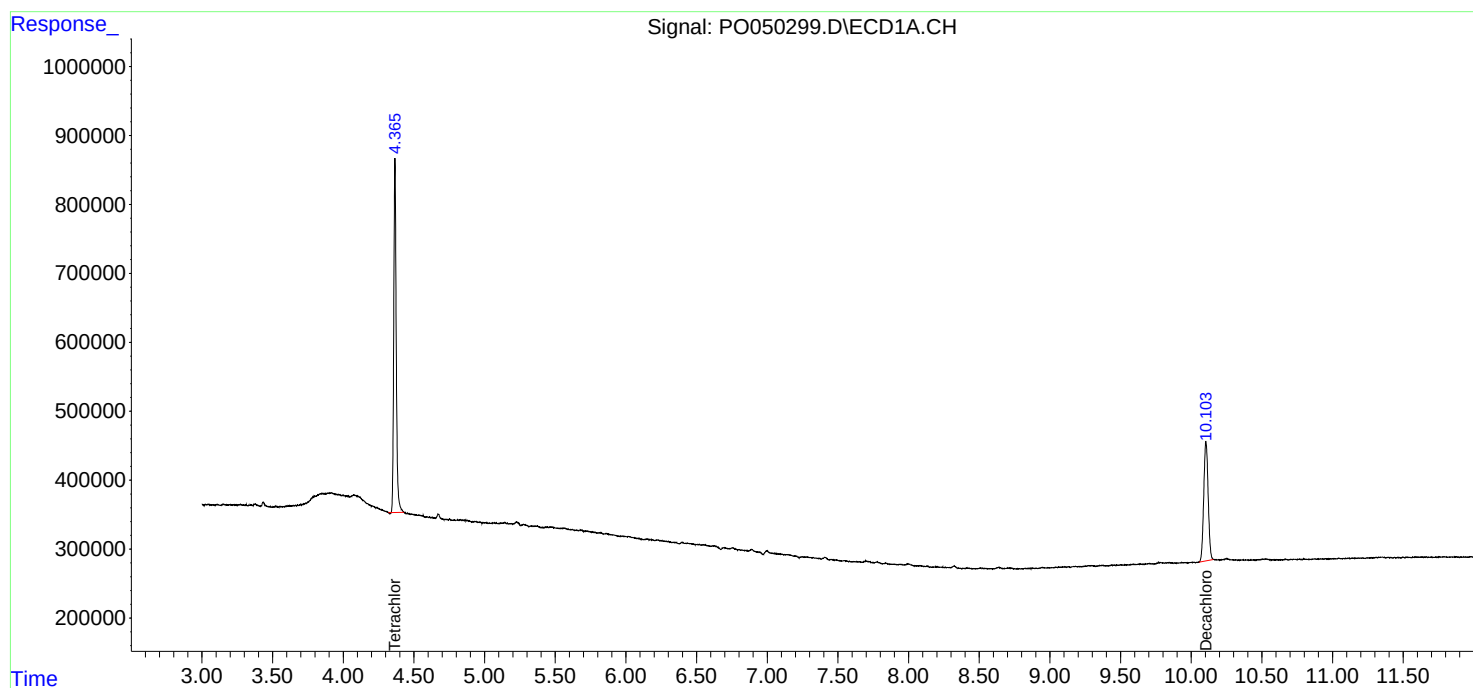

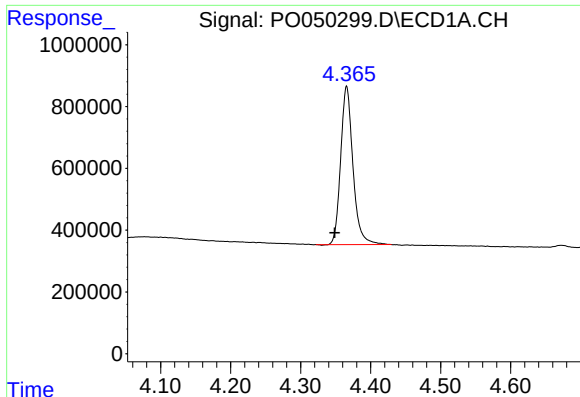


#1 Tetrachloro-m-xylene

R.T.: 4.366 min
Delta R.T.: 0.017 min
Response: 6259349
Conc: 20.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
SSSI-1017-S-DH-19A


Manual Integrations
APPROVED

sohil
10/22/2018 5:10:13 PM

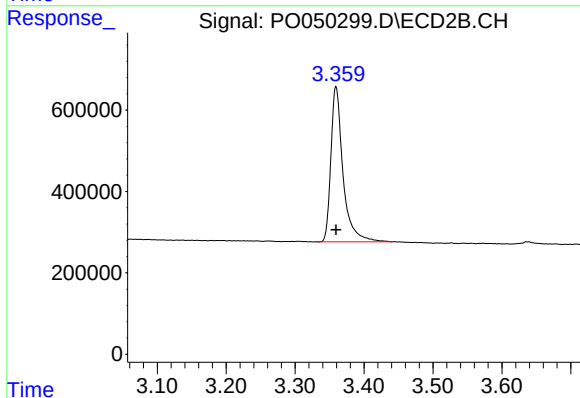


#1 Tetrachloro-m-xylene

R.T.: 3.359 min
Delta R.T.: 0.000 min
Response: 4658295
Conc: 23.69 ng/ml

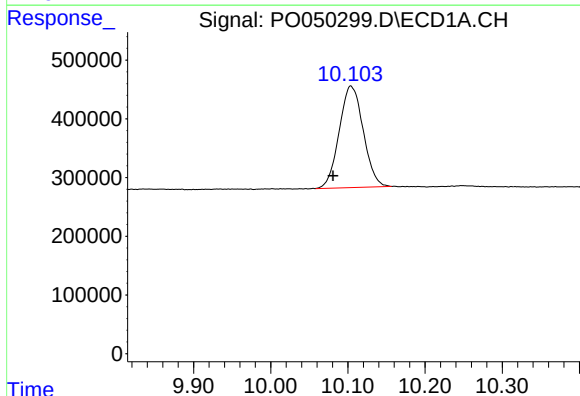

#2 Decachlorobiphenyl

R.T.: 10.103 min
Delta R.T.: 0.023 min
Response: 3744669
Conc: 17.26 ng/ml m

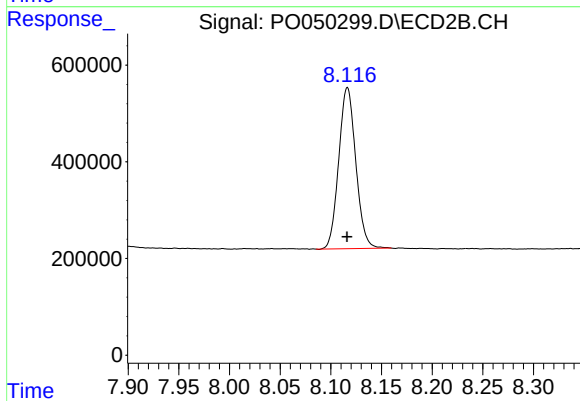

#2 Decachlorobiphenyl

R.T.: 8.116 min
Delta R.T.: 0.000 min
Response: 3904492
Conc: 20.43 ng/ml