

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101918\
 Data File : P0050306.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Oct 2018 3:59
 Operator : SM/SJ
 Sample : J5575-06
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SSSI-1015-S-DH-26

Manual Integrations
 APPROVED

sohil
 10/22/2018 5:10:27 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 04:36:13 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101818.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 19 02:02:26 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.365	3.359	6759781	4983614	22.654	25.349
2) SA Decachlor...	10.104	8.116	4063800	4247835	18.728m	22.223

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101918\
Data File : P0050306.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Oct 2018 3:59
Operator : SM/SJ
Sample : J5575-06
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SSSI-1015-S-DH-26


Manual Integrations
APPROVED

sohil
10/22/2018 5:10:27 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 04:36:13 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101818.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 19 02:02:26 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

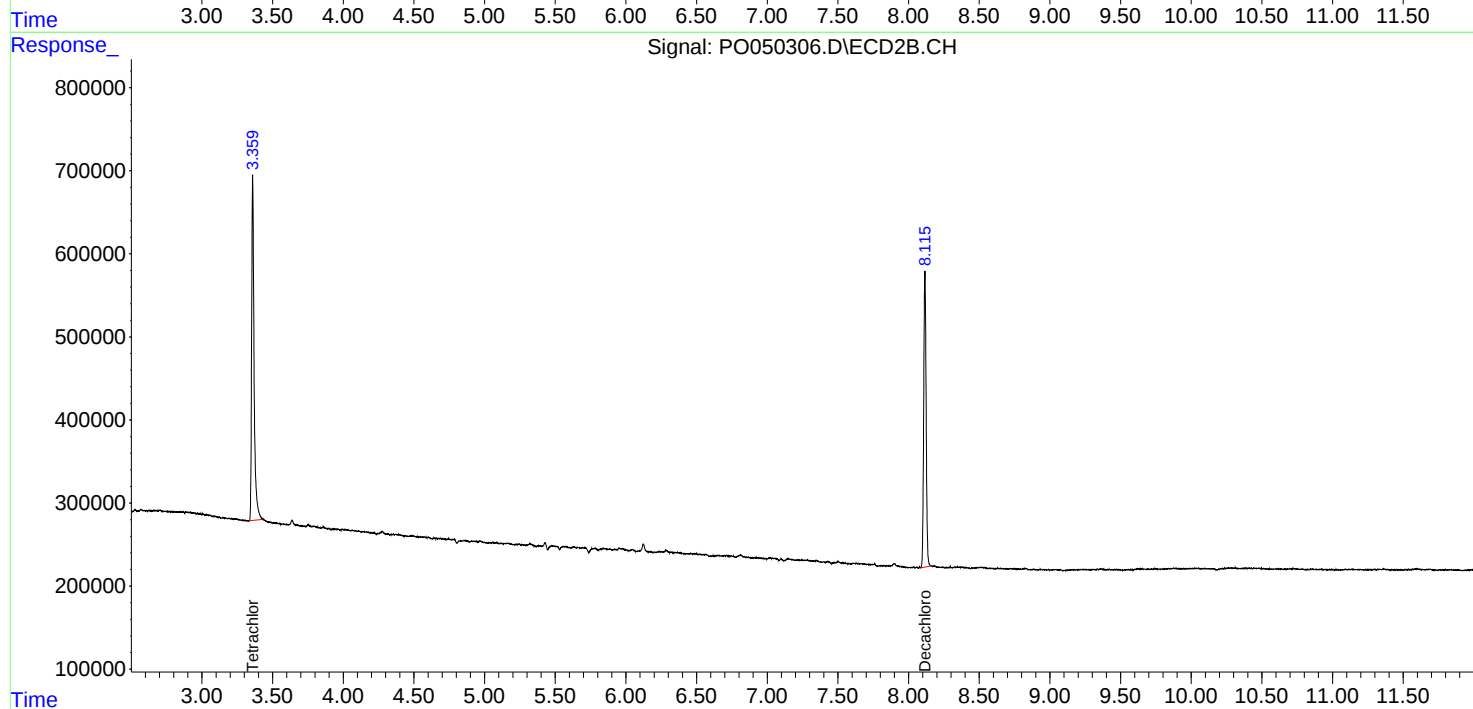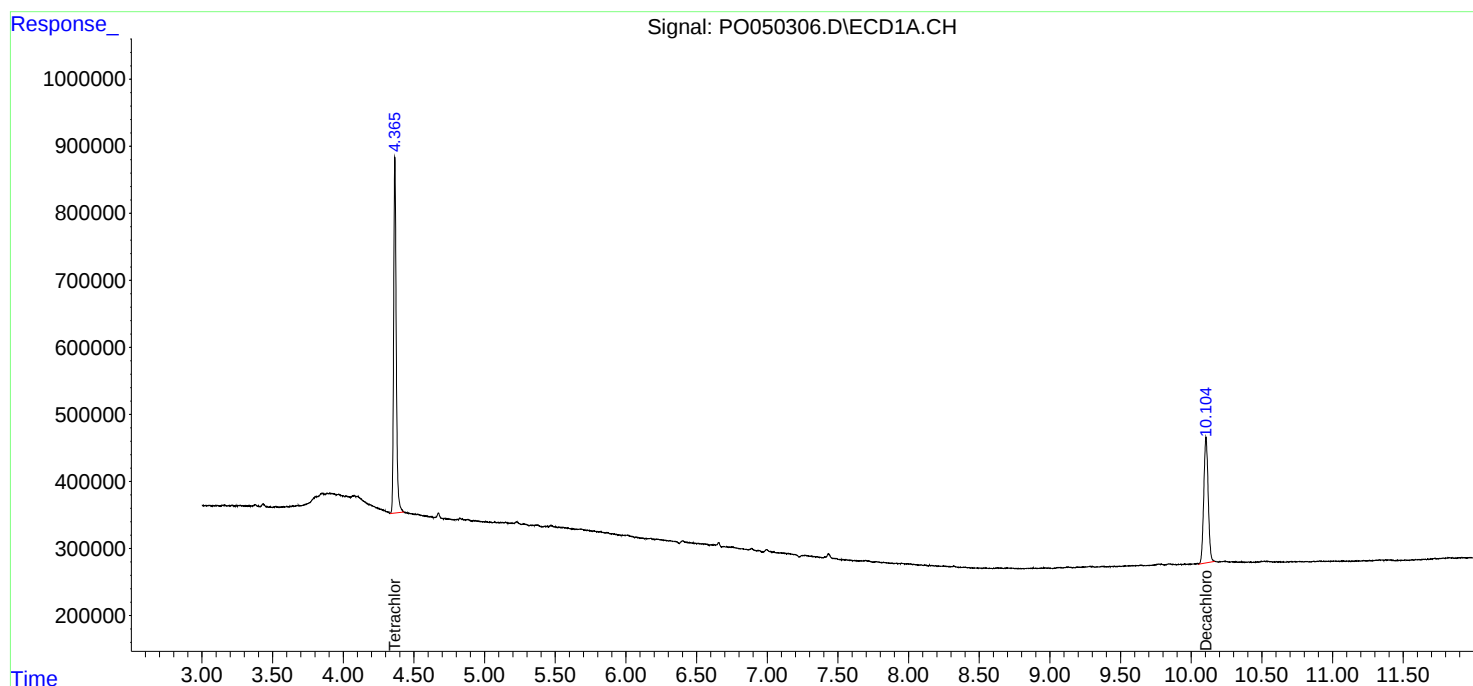

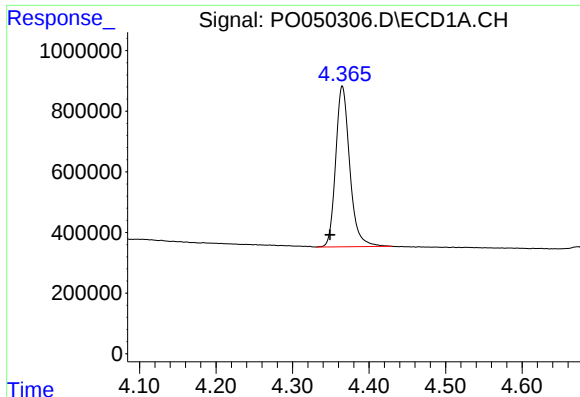


#1 Tetrachloro-m-xylene

R.T.: 4.365 min
Delta R.T.: 0.016 min
Response: 6759781
Conc: 22.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
SSSI-1015-S-DH-26


Manual Integrations
APPROVED

sohil
10/22/2018 5:10:27 PM

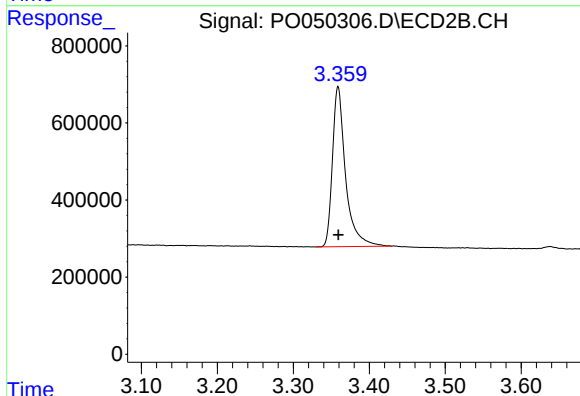


#1 Tetrachloro-m-xylene

R.T.: 3.359 min
Delta R.T.: 0.000 min
Response: 4983614
Conc: 25.35 ng/ml

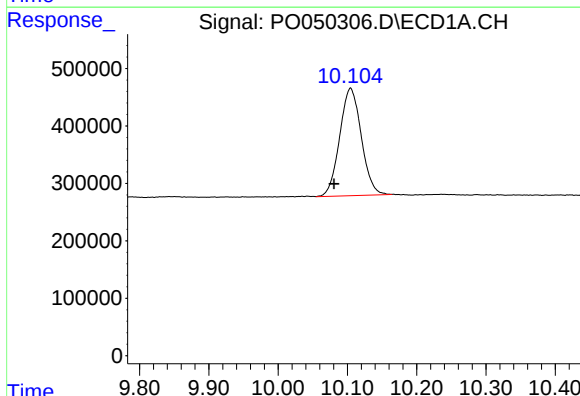

#2 Decachlorobiphenyl

R.T.: 10.104 min
Delta R.T.: 0.024 min
Response: 4063800
Conc: 18.73 ng/ml m

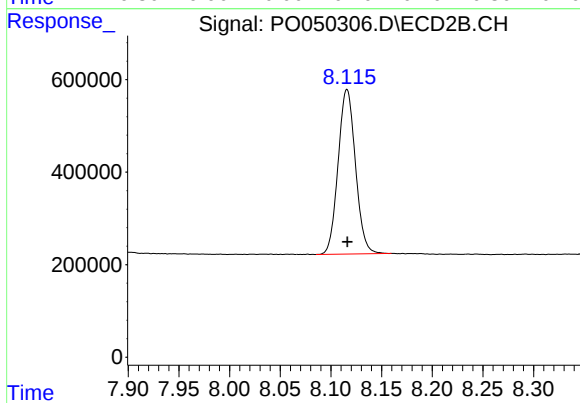

#2 Decachlorobiphenyl

R.T.: 8.116 min
Delta R.T.: 0.000 min
Response: 4247835
Conc: 22.22 ng/ml