

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101920\
 Data File : P0072498.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Oct 2020 15:42
 Operator : DD\AJ
 Sample : PB132445BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB132445BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 01:56:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 14 17:47:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.318	3.501	1719235	851697	20.270	20.220
2)	SA Decachlor...	9.919	8.667	2018203	957808	18.297	18.528
Target Compounds							
26)	L6 AR-1254-1	6.496f	0.000	196367	0	46.484	N.D. #
28)	L6 AR-1254-3	7.145f	0.000	306018	0	45.024	N.D. #
33)	L7 AR-1260-3	7.898	0.000	219437	0	34.240	N.D. #
35)	L7 AR-1260-5	8.439	0.000	111663	0	7.686	N.D. #
36)	L8 AR-1262-1	7.898	0.000	219437	0	23.138	N.D. #
37)	L8 AR-1262-2	8.439	0.000	111663	0	6.986	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101920\
Data File : P0072498.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Oct 2020 15:42
Operator : DD\AJ
Sample : PB132445BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB132445BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 01:56:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 14 17:47:24 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

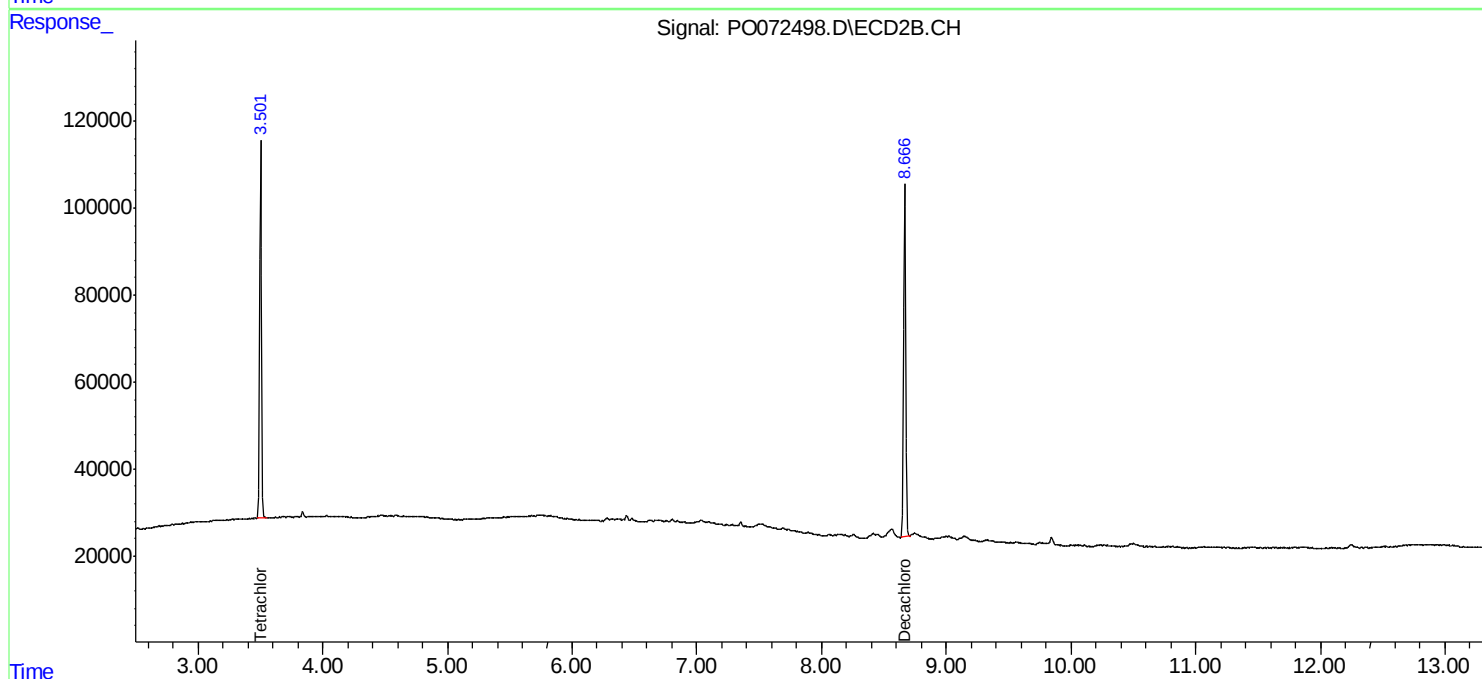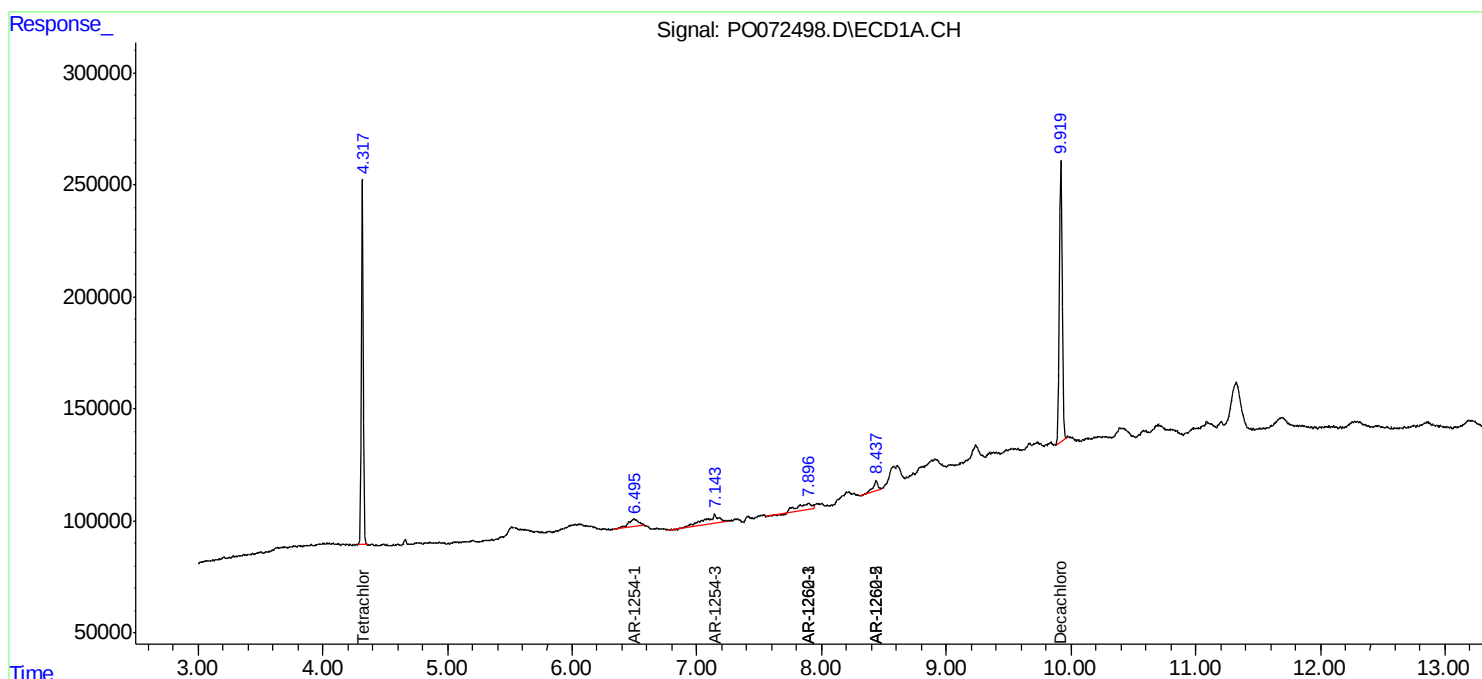


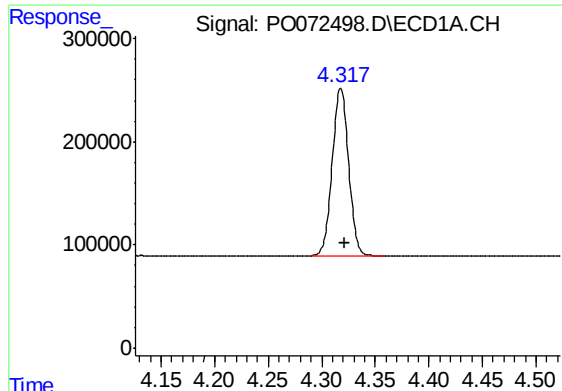

#1 Tetrachloro-m-xylene


R.T.: 4.318 min
Delta R.T.: -0.003 min
Response: 1719235
Conc: 20.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB132445BL

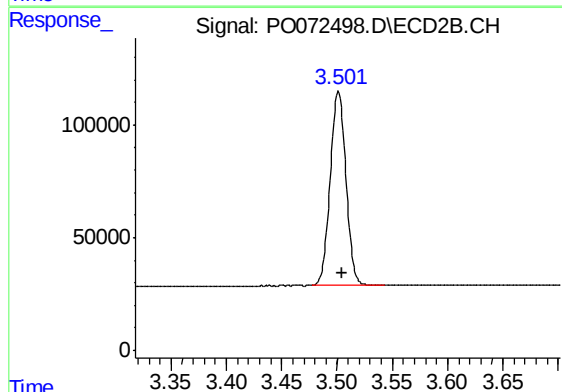


#1 Tetrachloro-m-xylene

R.T.: 3.501 min
Delta R.T.: -0.003 min
Response: 851697
Conc: 20.22 ng/ml

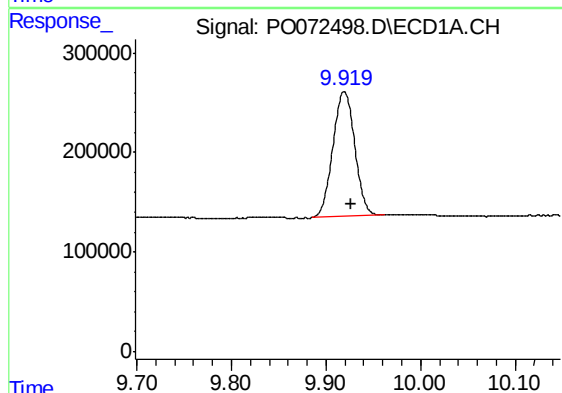


#2 Decachlorobiphenyl

R.T.: 9.919 min
Delta R.T.: -0.007 min
Response: 2018203
Conc: 18.30 ng/ml

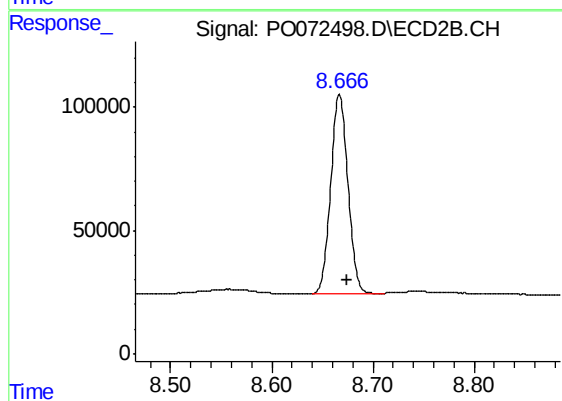

#2 Decachlorobiphenyl


R.T.: 8.667 min
Delta R.T.: -0.008 min
Response: 957808
Conc: 18.53 ng/ml

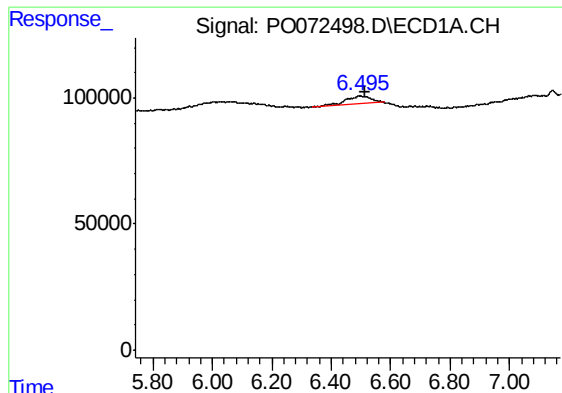

#26 AR-1254-1


R.T.: 6.496 min
Delta R.T.: -0.019 min
Response: 196367
Conc: 46.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB132445BL

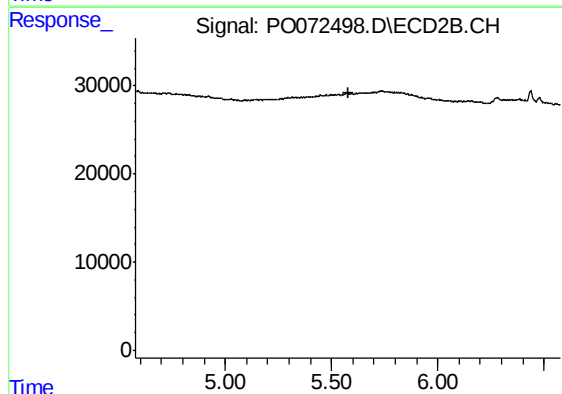


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 5.578 min
Response: 0
Conc: N.D.

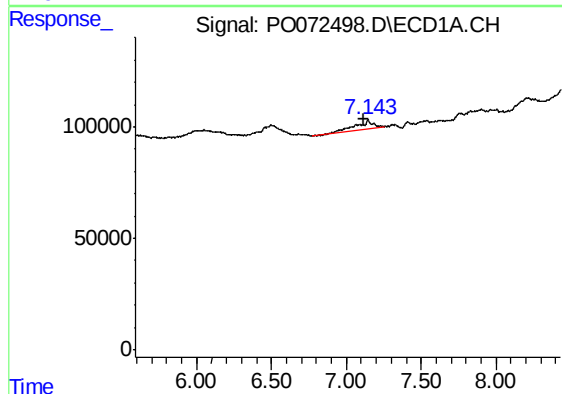


#28 AR-1254-3

R.T.: 7.145 min
Delta R.T.: 0.026 min
Response: 306018
Conc: 45.02 ng/ml

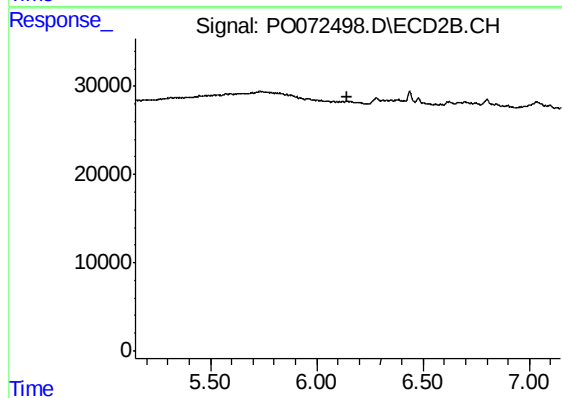

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.146 min
Response: 0
Conc: N.D.

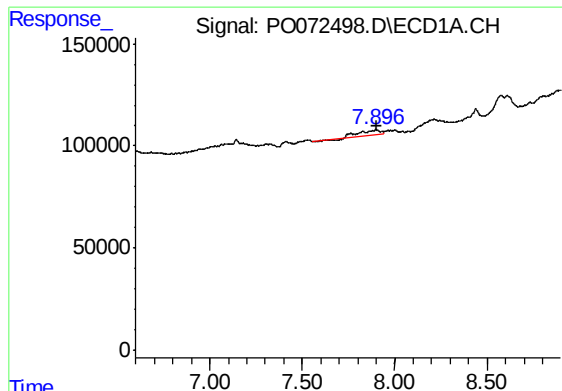

#33 AR-1260-3


R.T.: 7.898 min
Delta R.T.: -0.006 min
Response: 219437
Conc: 34.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB132445BL

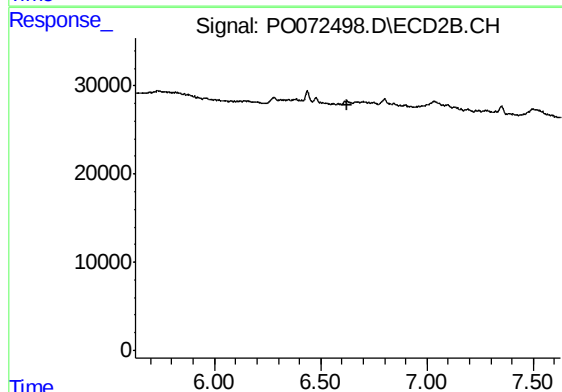


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 6.628 min
Response: 0
Conc: N.D.

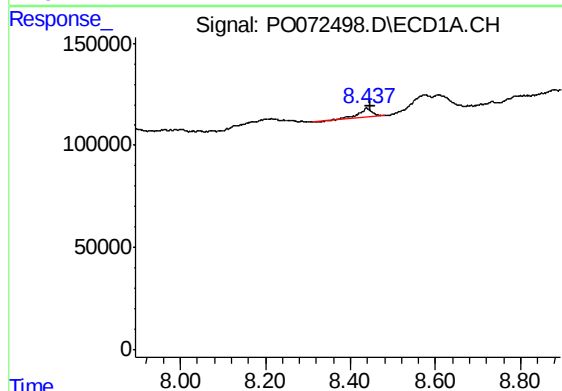


#35 AR-1260-5

R.T.: 8.439 min
Delta R.T.: -0.007 min
Response: 111663
Conc: 7.69 ng/ml

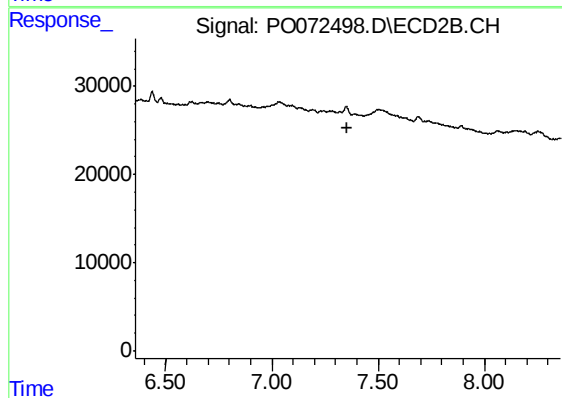

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 7.358 min
Response: 0
Conc: N.D.

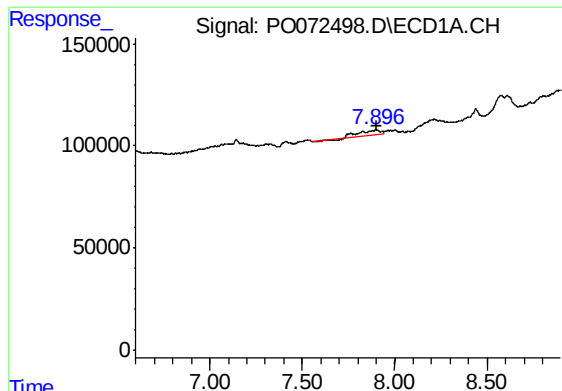

#36 AR-1262-1


R.T.: 7.898 min
Delta R.T.: -0.005 min
Response: 219437
Conc: 23.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB132445BL

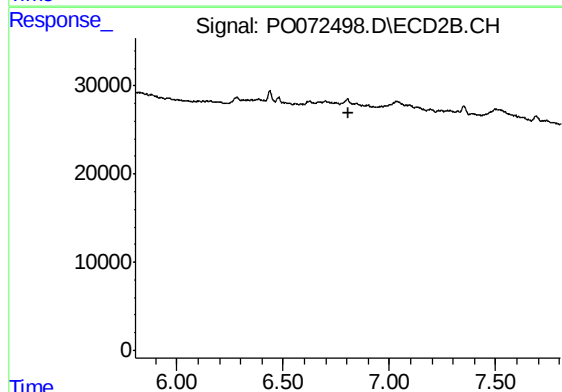


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 6.805 min
Response: 0
Conc: N.D.

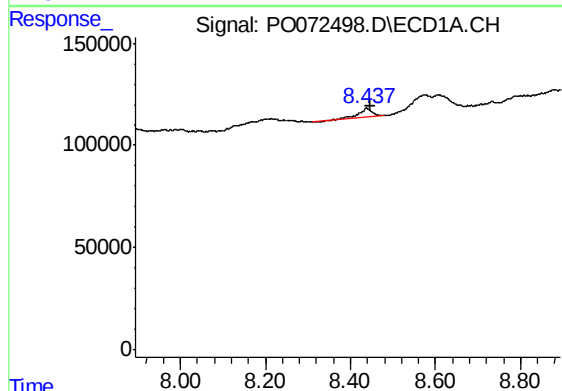

#37 AR-1262-2

R.T.: 8.439 min
Delta R.T.: -0.007 min
Response: 111663
Conc: 6.99 ng/ml

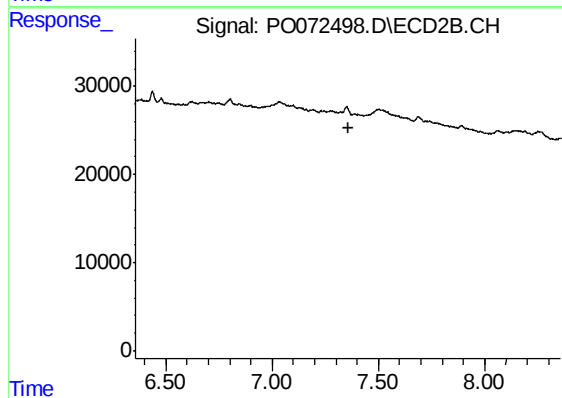

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.357 min
Response: 0
Conc: N.D.