

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101920\
 Data File : P0072507.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Oct 2020 18:16
 Operator : DD\AJ
 Sample : PB132443BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB132443BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 02:01:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 14 17:47:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.319	3.503	1758001	857630	20.727	20.361
2)	SA Decachlor...	9.918	8.668	2095819	1022734	19.000	19.784
Target Compounds							
28)	L6 AR-1254-3	7.144f	0.000	30102	0	4.429	N.D. #
33)	L7 AR-1260-3	7.903	0.000	67363	0	10.511	N.D. #
35)	L7 AR-1260-5	8.444	0.000	18100	0	1.246	N.D. #
36)	L8 AR-1262-1	7.903	0.000	67363	0	7.103	N.D. #
37)	L8 AR-1262-2	8.444	0.000	18100	0	1.132	N.D. #
39)	L8 AR-1262-4	8.776f	0.000	103190	0	25.821	N.D. #
42)	L9 AR-1268-2	8.776f	0.000	103190	0	6.250	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101920\
Data File : P0072507.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Oct 2020 18:16
Operator : DD\AJ
Sample : PB132443BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB132443BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 02:01:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 14 17:47:24 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

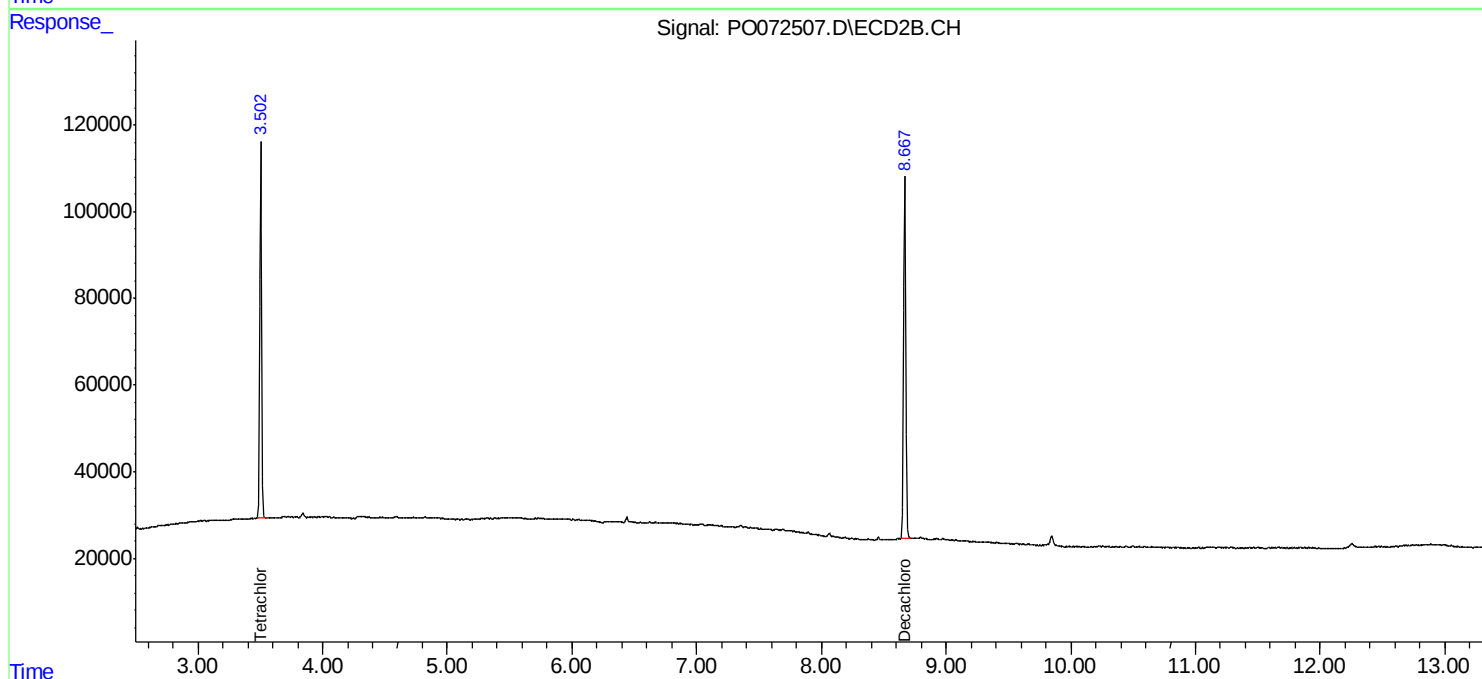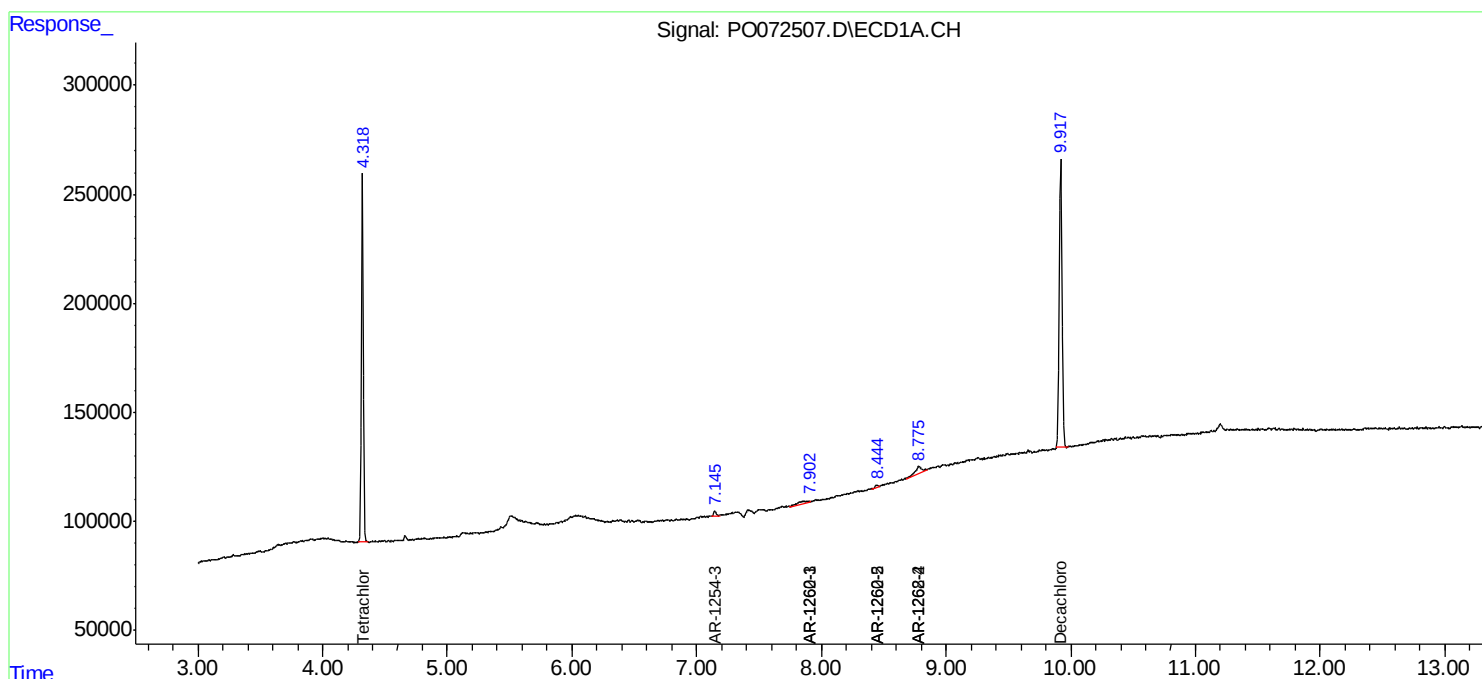


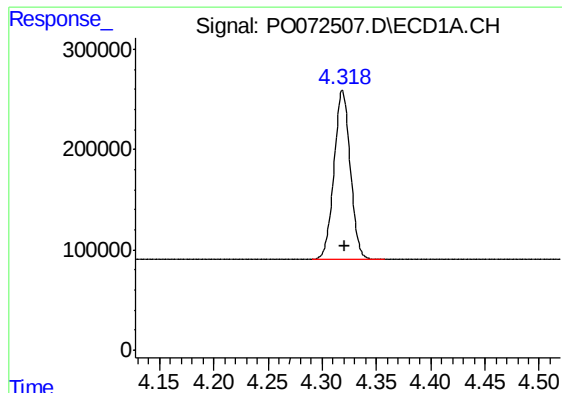

#1 Tetrachloro-m-xylene


R.T.: 4.319 min
Delta R.T.: -0.002 min
Response: 1758001
Conc: 20.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB132443BL

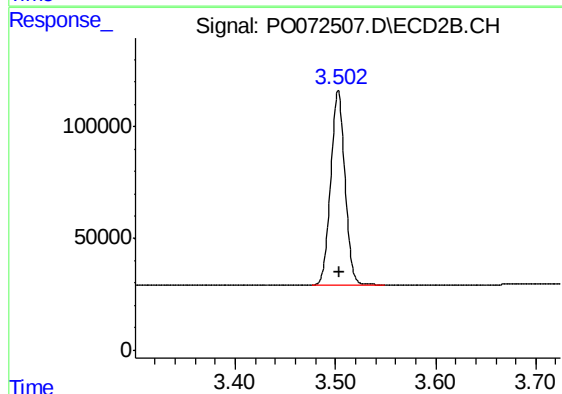


#1 Tetrachloro-m-xylene

R.T.: 3.503 min
Delta R.T.: -0.001 min
Response: 857630
Conc: 20.36 ng/ml

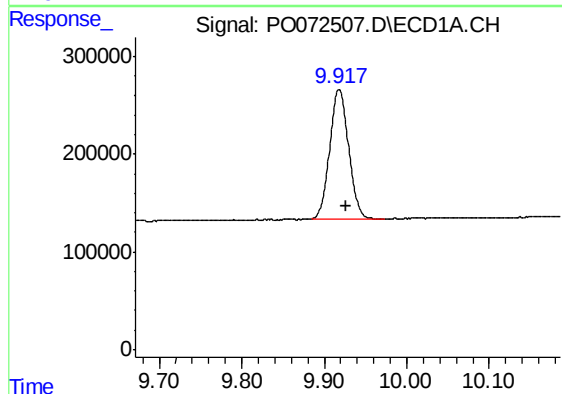


#2 Decachlorobiphenyl

R.T.: 9.918 min
Delta R.T.: -0.008 min
Response: 2095819
Conc: 19.00 ng/ml

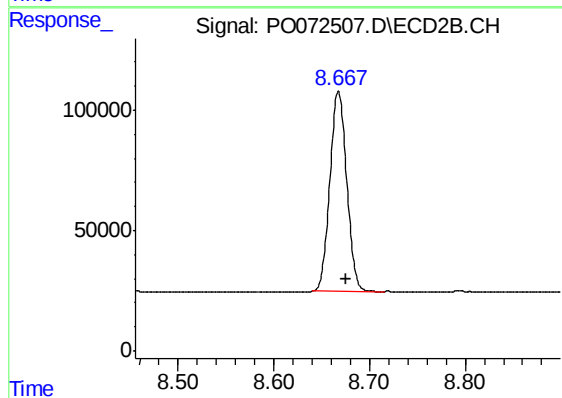

#2 Decachlorobiphenyl


R.T.: 8.668 min
Delta R.T.: -0.008 min
Response: 1022734
Conc: 19.78 ng/ml

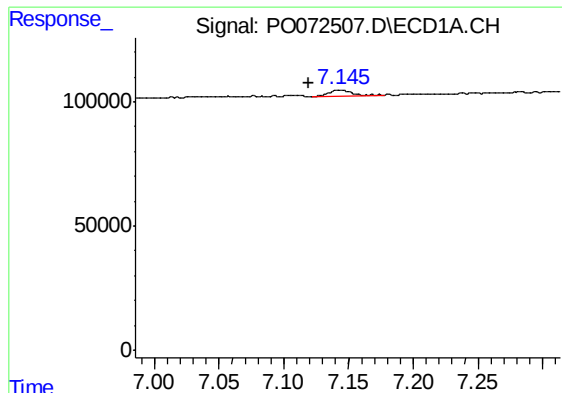

#28 AR-1254-3


R.T.: 7.144 min
Delta R.T.: 0.025 min
Response: 30102
Conc: 4.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB132443BL

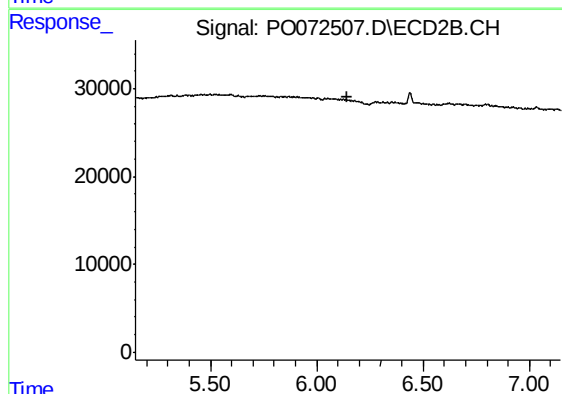


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.146 min
Response: 0
Conc: N.D.

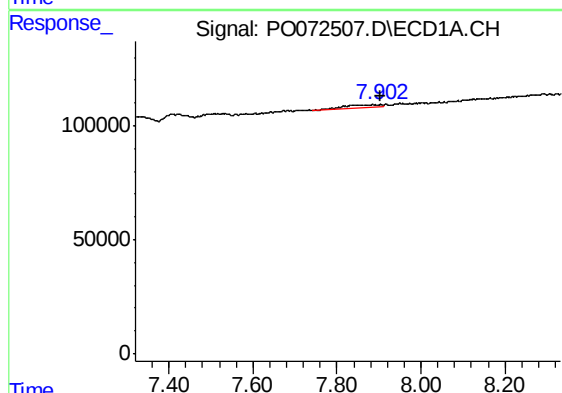


#33 AR-1260-3

R.T.: 7.903 min
Delta R.T.: -0.001 min
Response: 67363
Conc: 10.51 ng/ml

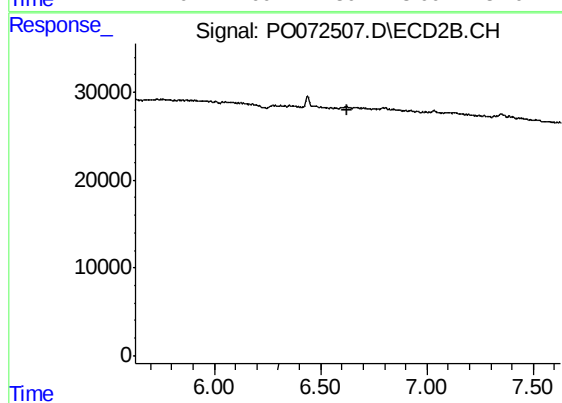

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 6.628 min
Response: 0
Conc: N.D.

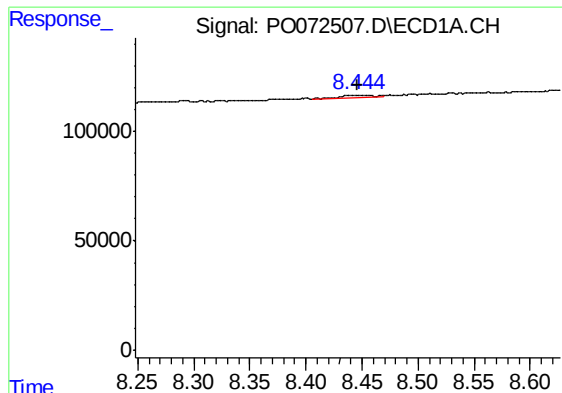

#35 AR-1260-5


R.T.: 8.444 min
Delta R.T.: -0.001 min
Response: 18100
Conc: 1.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB132443BL

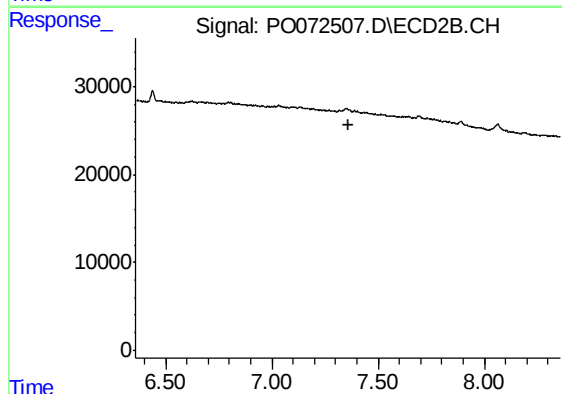


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.358 min
Response: 0
Conc: N.D.

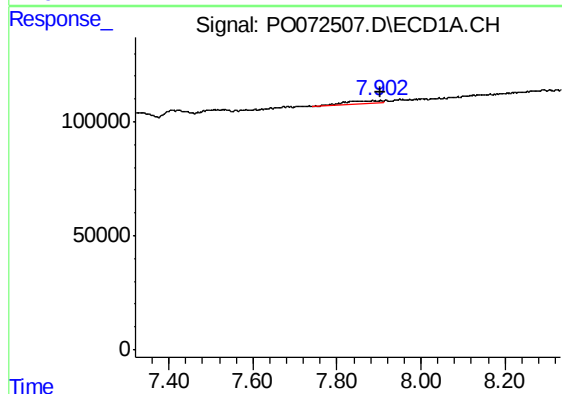


#36 AR-1262-1

R.T.: 7.903 min
Delta R.T.: 0.000 min
Response: 67363
Conc: 7.10 ng/ml

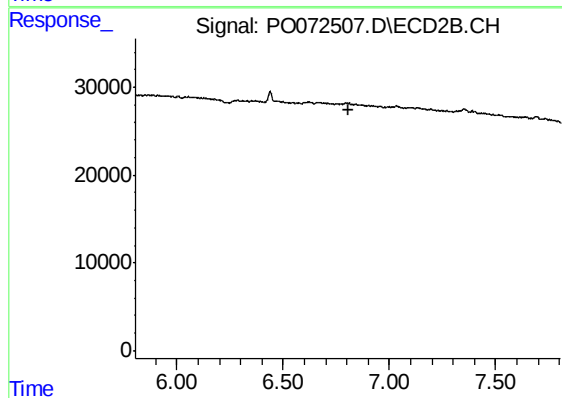

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T. : 6.805 min
Response: 0
Conc: N.D.

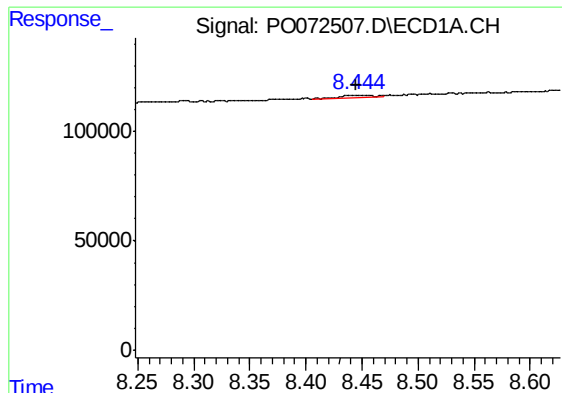

#37 AR-1262-2


R.T.: 8.444 min
Delta R.T.: -0.001 min
Response: 18100
Conc: 1.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB132443BL

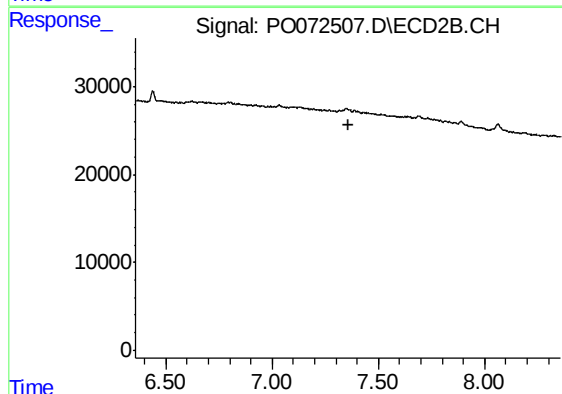


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.357 min
Response: 0
Conc: N.D.

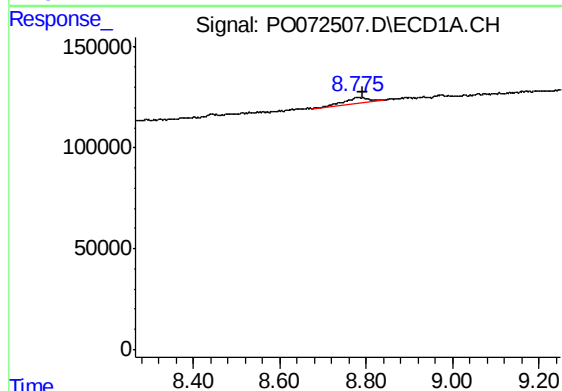


#39 AR-1262-4

R.T.: 8.776 min
Delta R.T.: -0.017 min
Response: 103190
Conc: 25.82 ng/ml

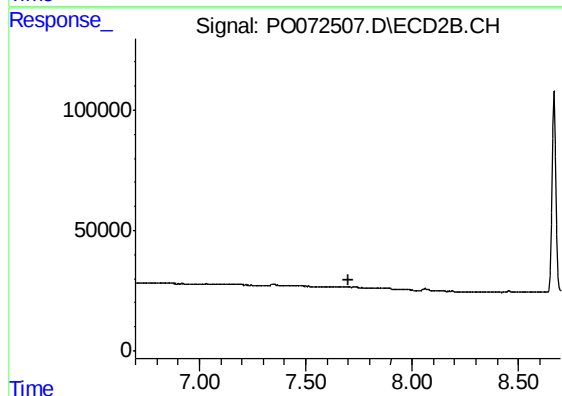

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 7.698 min
Response: 0
Conc: N.D.

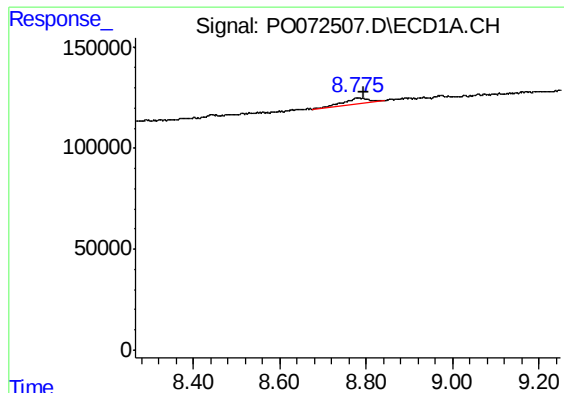

#42 AR-1268-2

R.T.: 8.776 min
Delta R.T.: -0.018 min
Response: 103190
Conc: 6.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB132443BL

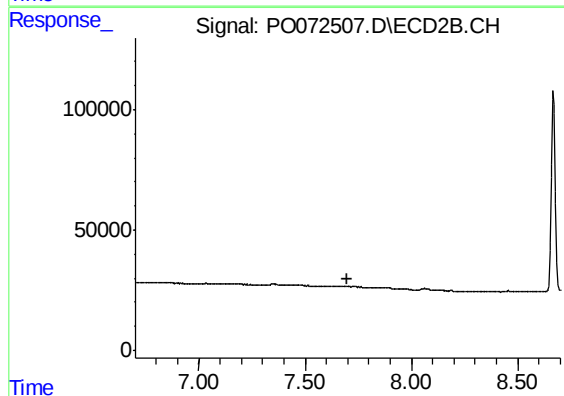

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 7.701 min
Response: 0
Conc: N.D.