

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101920\
 Data File : PO072479.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Oct 2020 9:53
 Operator : DD\AJ
 Sample : L4413-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 30688

Manual Integrations
 APPROVED

Ankita
 10/20/2020 1:05:44 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 17:14:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 14 17:47:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.321	3.504	1857937	983144	21.905	23.340m
2) SA Decachlor...	9.938	8.688	1791094	850334	16.238	16.449m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101920\
Data File : P0072479.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Oct 2020 9:53
Operator : DD\AJ
Sample : L4413-01
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
30688


Manual Integrations
APPROVED

Ankita
10/20/2020 1:05:44 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 17:14:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 14 17:47:24 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

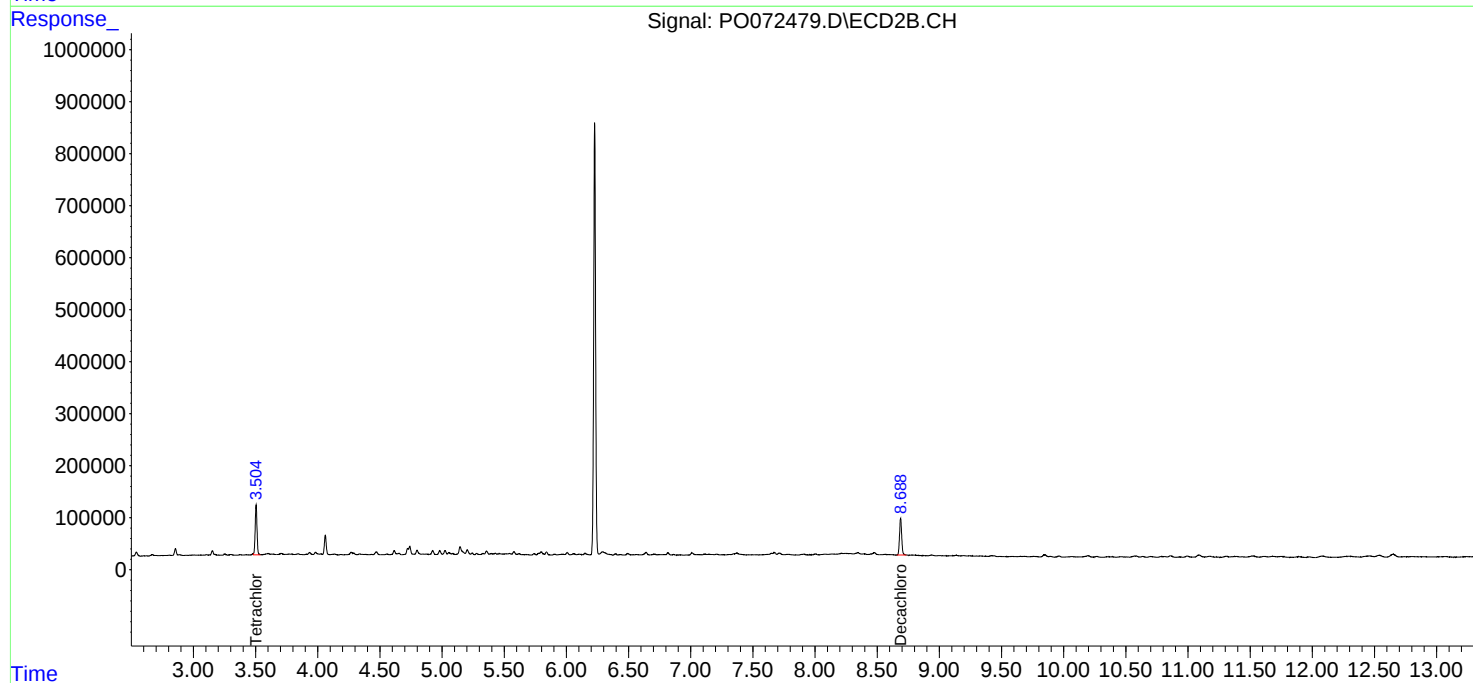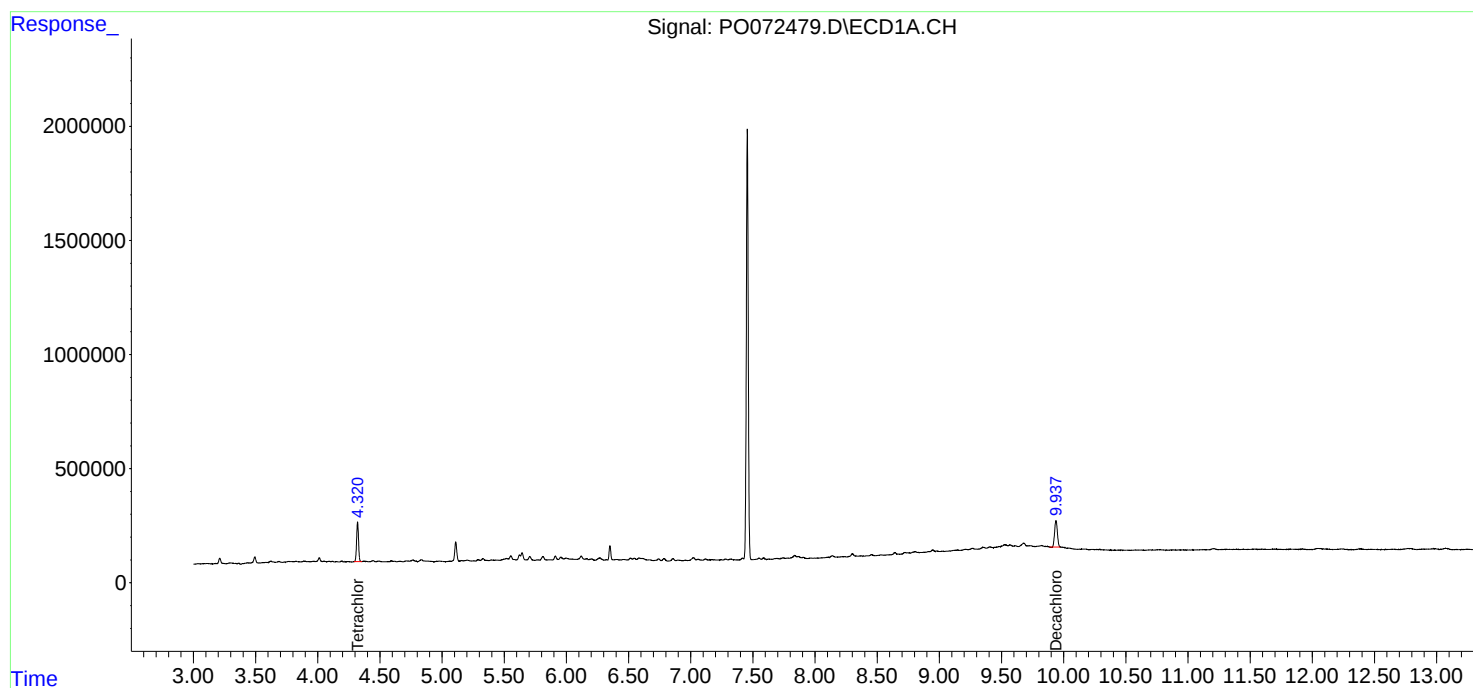

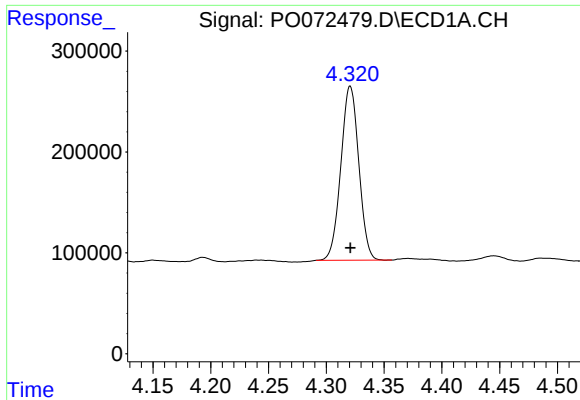


#1 Tetrachloro-m-xylene

R.T.: 4.321 min
Delta R.T.: 0.000 min
Response: 1857937
Conc: 21.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
30688


Manual Integrations
APPROVED

Ankita
10/20/2020 1:05:44 PM

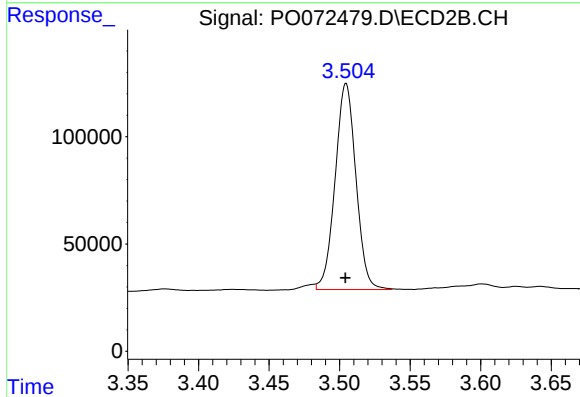


#1 Tetrachloro-m-xylene

R.T.: 3.504 min
Delta R.T.: 0.000 min
Response: 983144
Conc: 23.34 ng/ml m

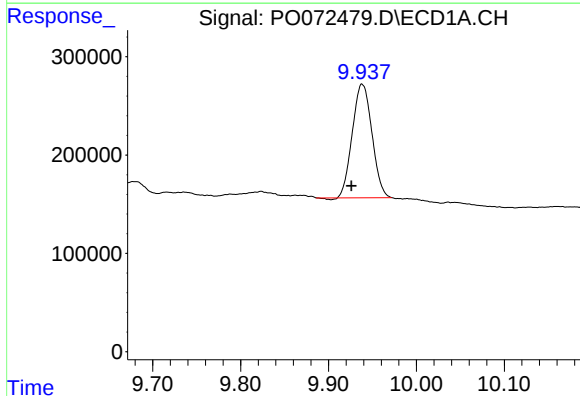

#2 Decachlorobiphenyl

R.T.: 9.938 min
Delta R.T.: 0.012 min
Response: 1791094
Conc: 16.24 ng/ml

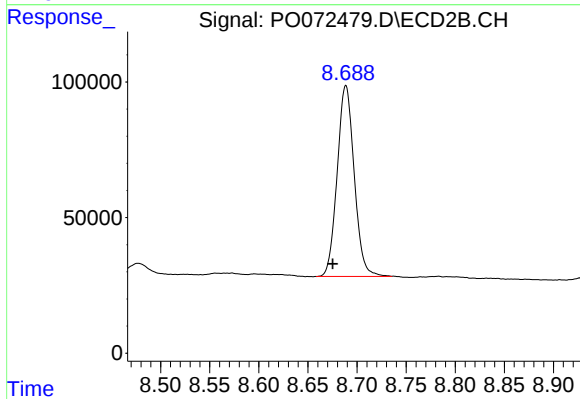

#2 Decachlorobiphenyl

R.T.: 8.688 min
Delta R.T.: 0.013 min
Response: 850334
Conc: 16.45 ng/ml m