

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101920\
 Data File : PO072487.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Oct 2020 12:10
 Operator : DD\AJ
 Sample : L4442-12DL 2X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 C0AL3DL

Manual Integrations
 APPROVED

Ankita
 10/20/2020 1:05:46 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 17:17:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 14 17:47:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.319	3.503	971849	486790	11.458	11.557
2) SA Decachlor...	9.920	8.668	1156098	566356	10.481	10.956
Target Compounds						
31) L7 AR-1260-1	7.276	6.278	650153	331517	133.414	129.589m
32) L7 AR-1260-2	7.542	6.479	1161826	504221	151.422	156.370
33) L7 AR-1260-3	7.900	6.624	633732	339913	98.886	113.256
34) L7 AR-1260-4	8.127	7.100	632374	247437	103.905	93.850
35) L7 AR-1260-5	8.442	7.353	1610247	657300	110.843	100.607

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101920\
Data File : PO072487.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Oct 2020 12:10
Operator : DD\AJ
Sample : L4442-12DL 2X
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
COAL3DL


Manual Integrations
APPROVED

Ankita
10/20/2020 1:05:46 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 17:17:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 14 17:47:24 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

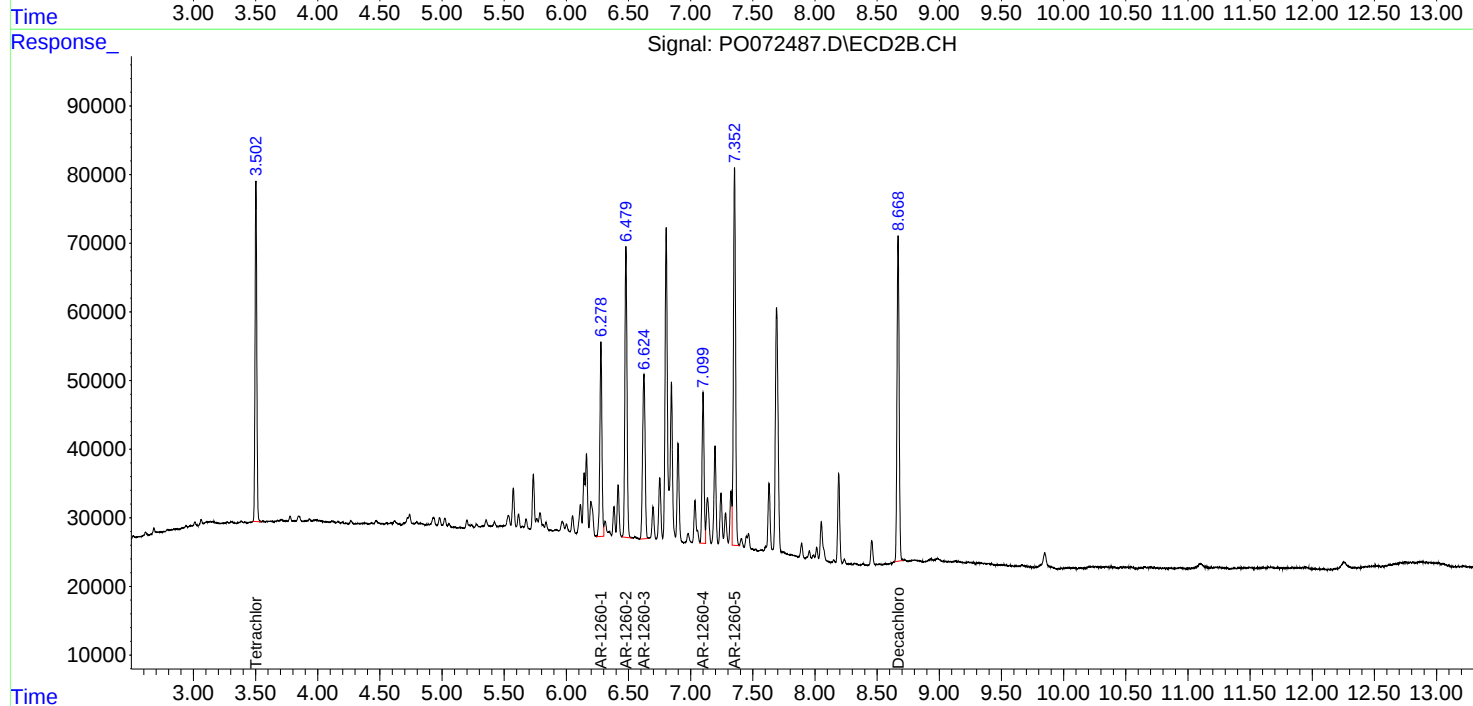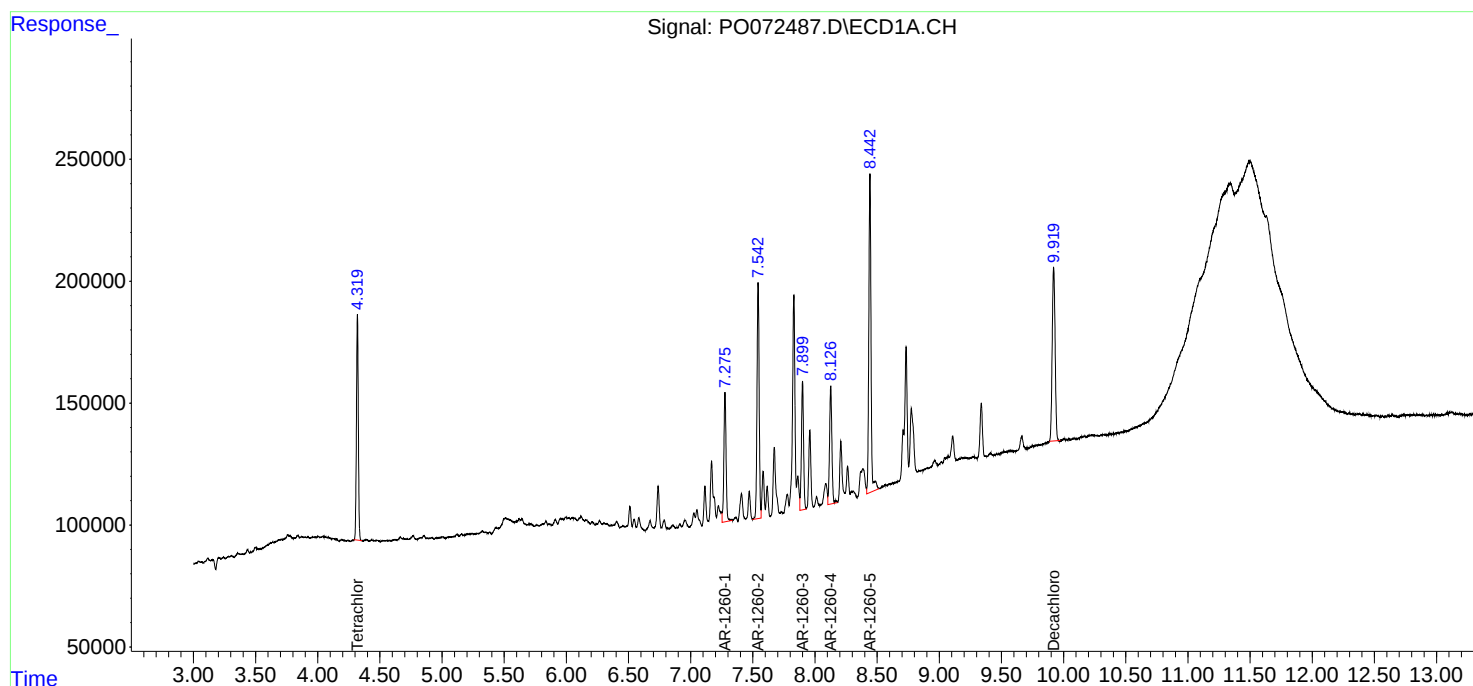

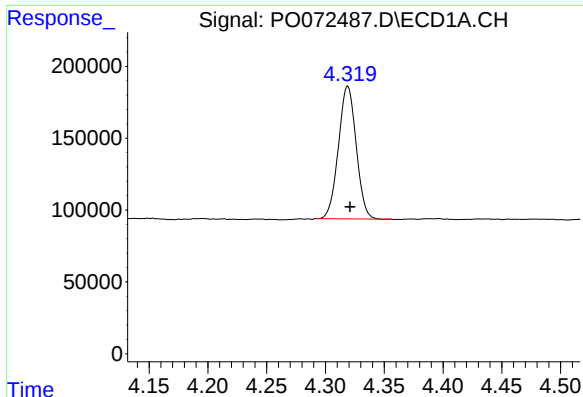


#1 Tetrachloro-m-xylene

R.T.: 4.319 min
Delta R.T.: -0.002 min
Response: 971849
Conc: 11.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
C0AL3DL


Manual Integrations
APPROVED

Ankita
10/20/2020 1:05:46 PM

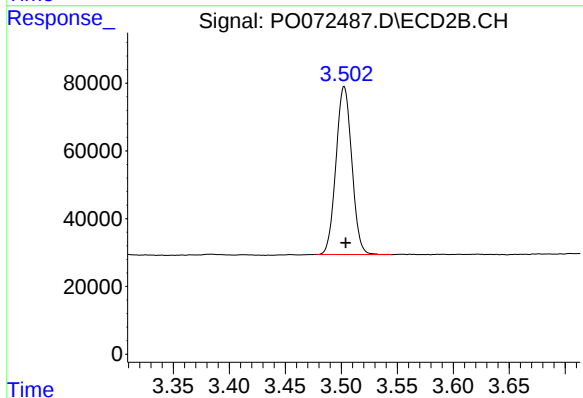


#1 Tetrachloro-m-xylene

R.T.: 3.503 min
Delta R.T.: -0.002 min
Response: 486790
Conc: 11.56 ng/ml

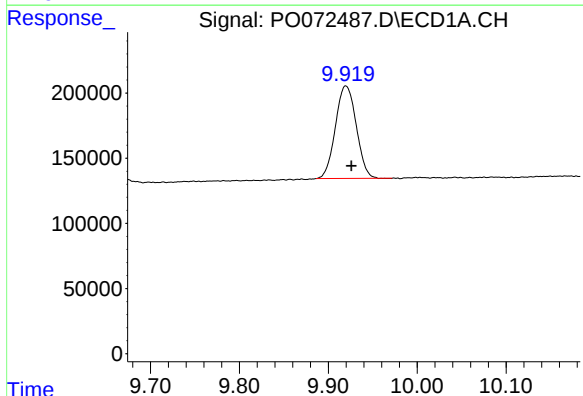


#2 Decachlorobiphenyl

R.T.: 9.920 min
Delta R.T.: -0.006 min
Response: 1156098
Conc: 10.48 ng/ml

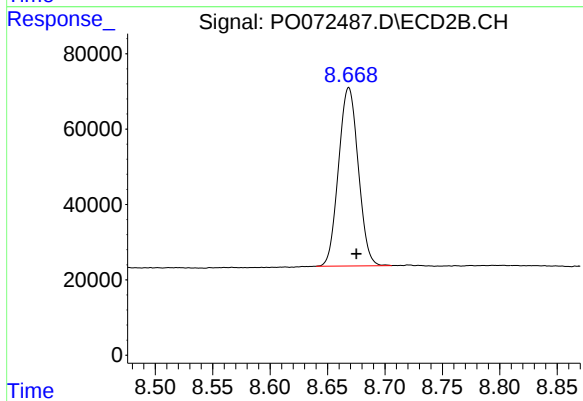

#2 Decachlorobiphenyl

R.T.: 8.668 min
Delta R.T.: -0.007 min
Response: 566356
Conc: 10.96 ng/ml

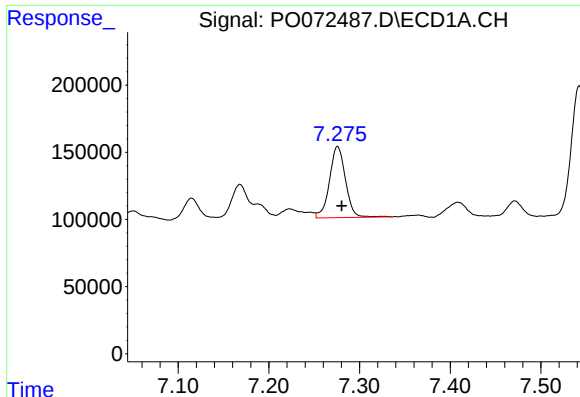


#31 AR-1260-1

R.T.: 7.276 min
Delta R.T.: -0.004 min
Response: 650153
Conc: 133.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
C0AL3DL


Manual Integrations
APPROVED

Ankita
10/20/2020 1:05:46 PM

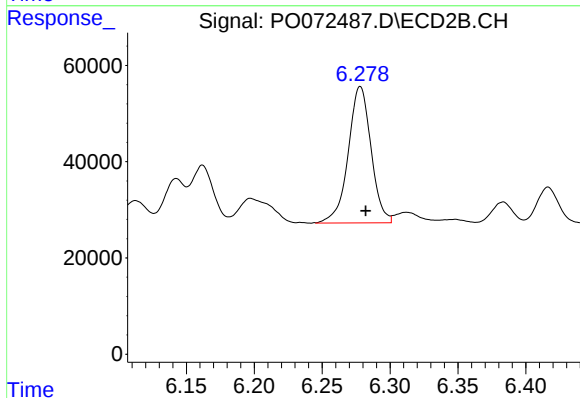


#31 AR-1260-1

R.T.: 6.278 min
Delta R.T.: -0.005 min
Response: 331517
Conc: 129.59 ng/ml m

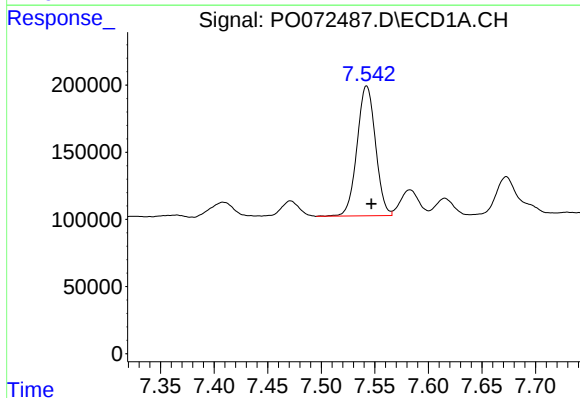


#32 AR-1260-2

R.T.: 7.542 min
Delta R.T.: -0.004 min
Response: 1161826
Conc: 151.42 ng/ml

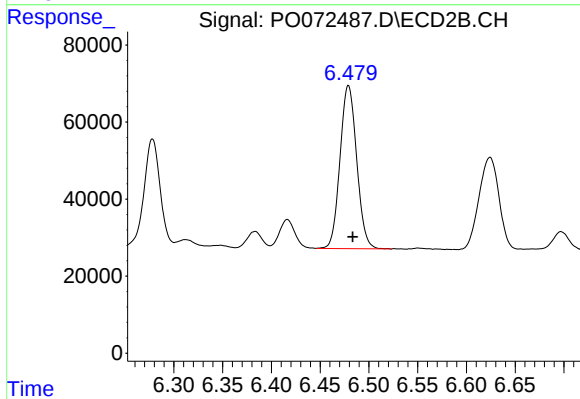

#32 AR-1260-2

R.T.: 6.479 min
Delta R.T.: -0.004 min
Response: 504221
Conc: 156.37 ng/ml

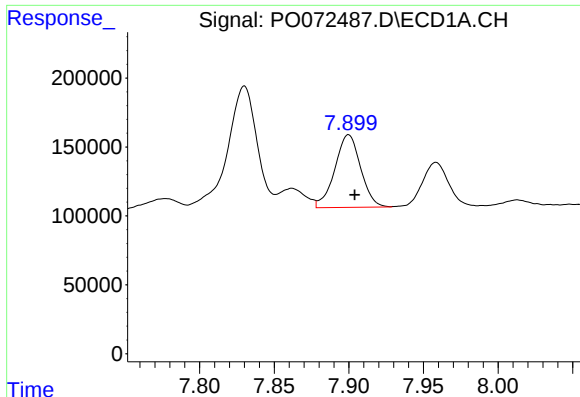


#33 AR-1260-3

R.T.: 7.900 min
Delta R.T.: -0.004 min
Response: 633732
Conc: 98.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
C0AL3DL


Manual Integrations
APPROVED

Ankita
10/20/2020 1:05:46 PM

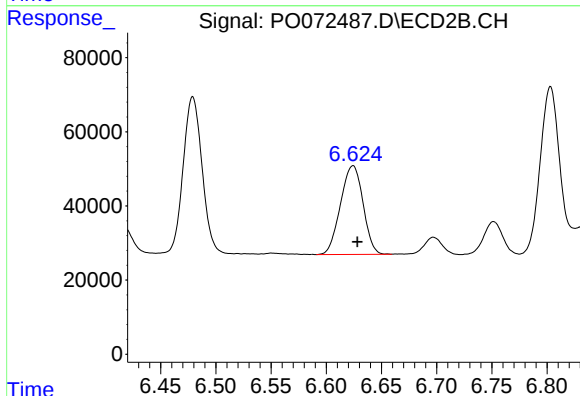


#33 AR-1260-3

R.T.: 6.624 min
Delta R.T.: -0.004 min
Response: 339913
Conc: 113.26 ng/ml

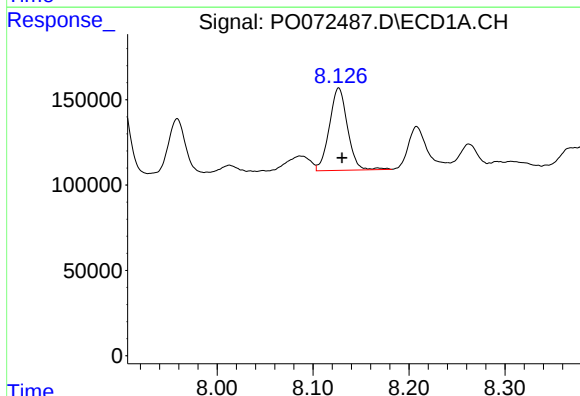


#34 AR-1260-4

R.T.: 8.127 min
Delta R.T.: -0.004 min
Response: 632374
Conc: 103.91 ng/ml

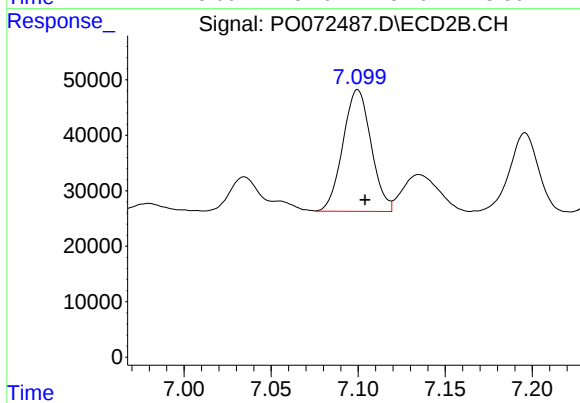

#34 AR-1260-4

R.T.: 7.100 min
Delta R.T.: -0.004 min
Response: 247437
Conc: 93.85 ng/ml

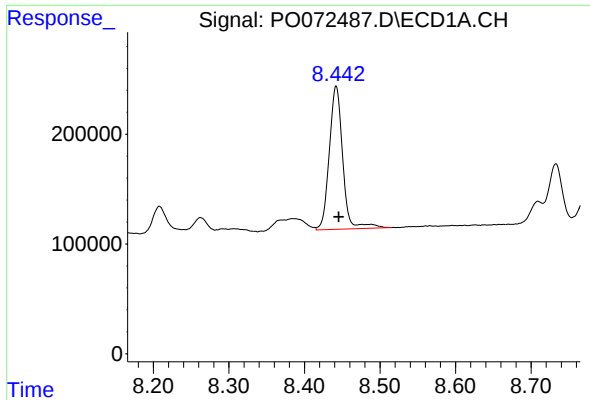


#35 AR-1260-5

R.T.: 8.442 min
Delta R.T.: -0.004 min
Response: 1610247
Conc: 110.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
C0AL3DL

Manual Integrations
APPROVED

Ankita
10/20/2020 1:05:46 PM

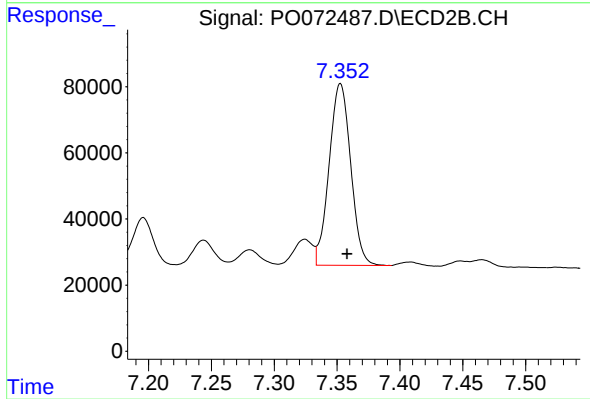

#35 AR-1260-5

R.T.: 7.353 min
Delta R.T.: -0.005 min
Response: 657300
Conc: 100.61 ng/ml