

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101920\
 Data File : PO072512.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Oct 2020 19:41
 Operator : DD\AJ
 Sample : L4454-01
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TEST-PIT

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 02:05:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 14 17:47:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.318	3.501	1962609	965187	23.139	22.914
2) SA Decachlor...	9.919	8.668	2235547	1054016	20.267	20.389

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101920\
Data File : PO072512.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Oct 2020 19:41
Operator : DD\AJ
Sample : L4454-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TEST-PIT

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 02:05:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 14 17:47:24 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

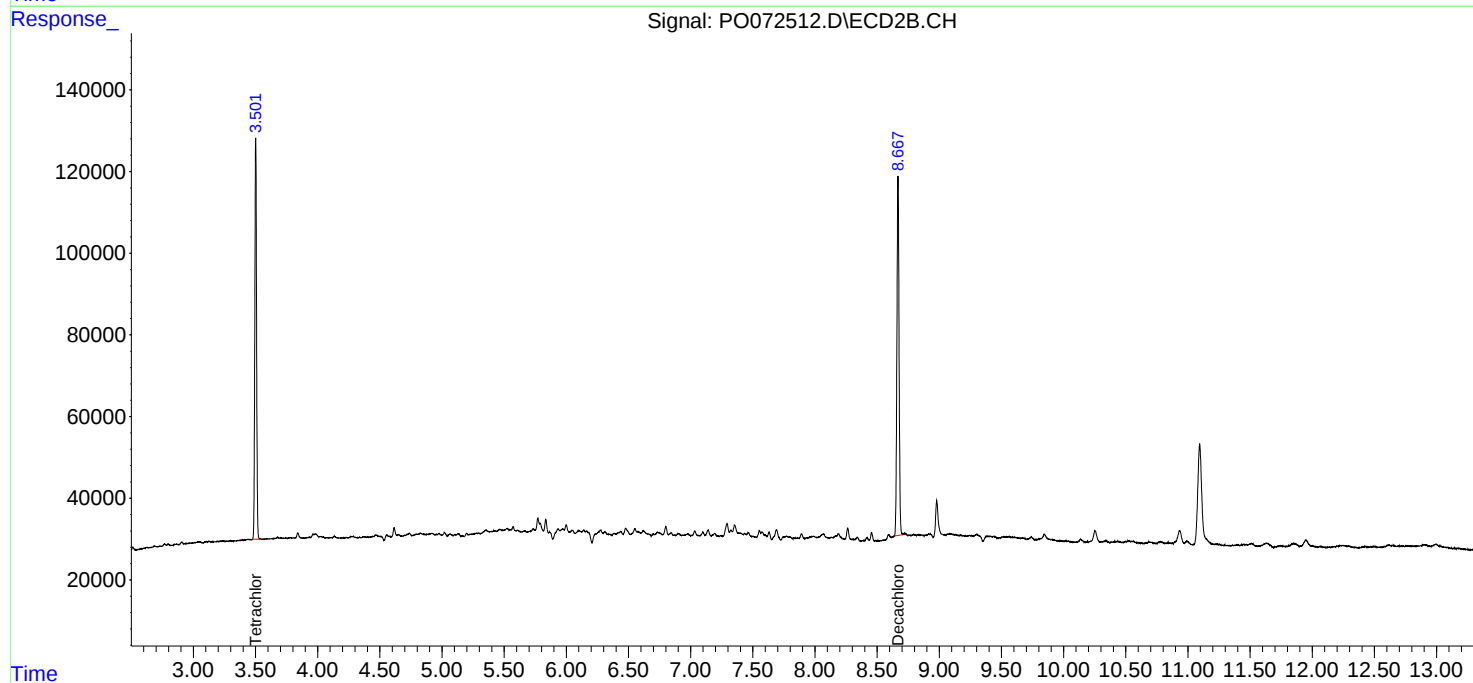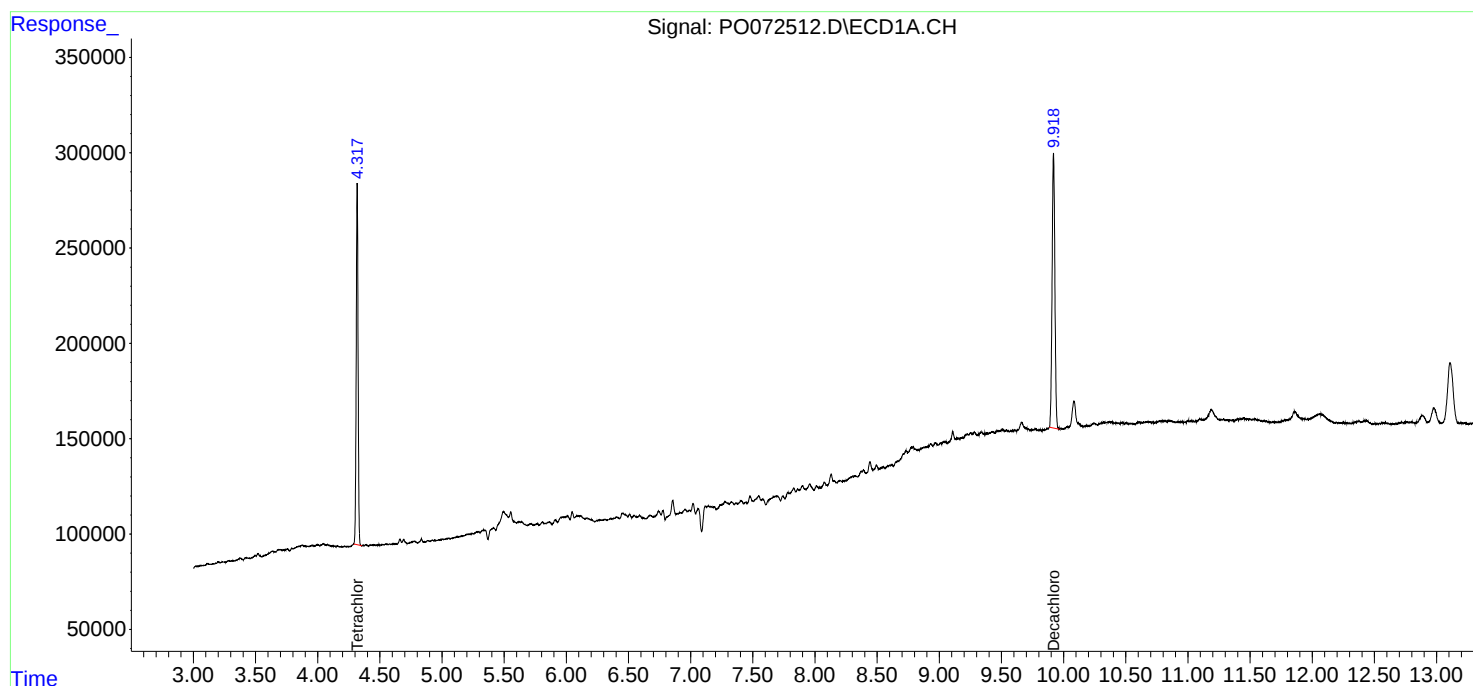


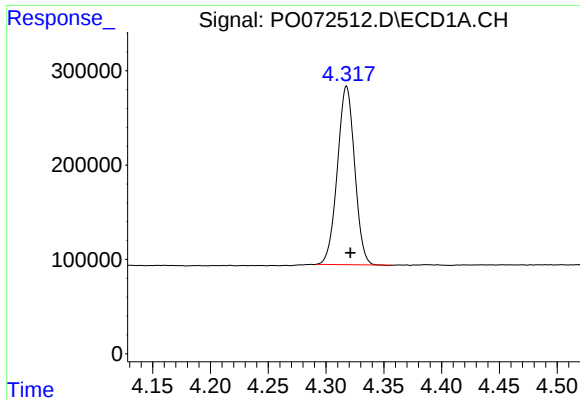

#1 Tetrachloro-m-xylene


R.T.: 4.318 min
Delta R.T.: -0.003 min
Response: 1962609
Conc: 23.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
TEST-PIT

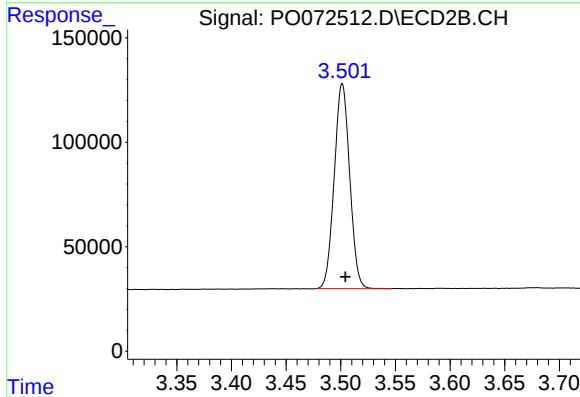


#1 Tetrachloro-m-xylene

R.T.: 3.501 min
Delta R.T.: -0.003 min
Response: 965187
Conc: 22.91 ng/ml

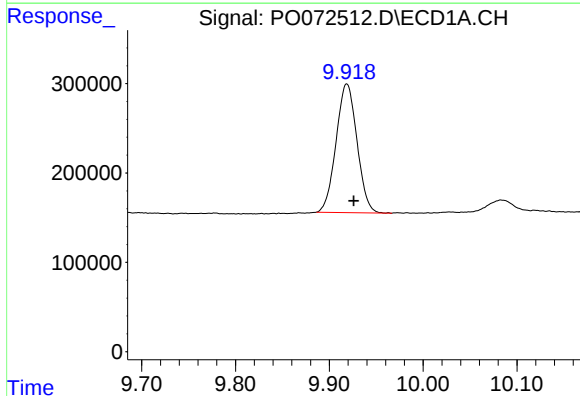

#2 Decachlorobiphenyl

R.T.: 9.919 min
Delta R.T.: -0.007 min
Response: 2235547
Conc: 20.27 ng/ml

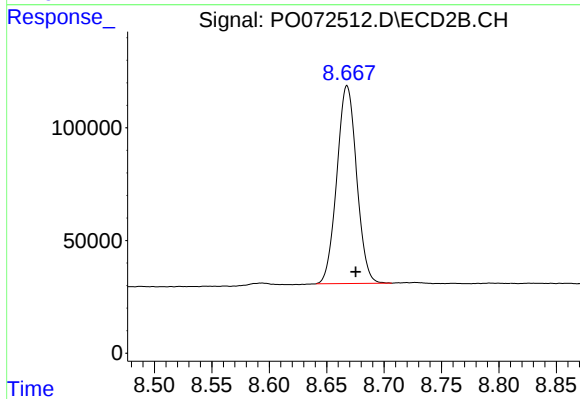

#2 Decachlorobiphenyl

R.T.: 8.668 min
Delta R.T.: -0.007 min
Response: 1054016
Conc: 20.39 ng/ml