

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102020\
 Data File : PO072540.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Oct 2020 15:33
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 16:14:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 14 17:47:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.319	3.502	2034978	969156	23.992	23.008
2) SA Decachlor...	9.919	8.667	2473878	1137596	22.428	22.006
Target Compounds						
20) L4 AR-1242-5	0.000	5.592	0	36515	N.D.	26.597 #
24) L5 AR-1248-4	6.525f	0.000	182705	0	41.316	N.D. #
25) L5 AR-1248-5	0.000	5.592f	0	36515	N.D.	19.770 #
26) L6 AR-1254-1	6.525	5.592	182705	36515	43.250	13.210 #
30) L6 AR-1254-5	7.819f	0.000	68853	0	10.749	N.D. #
39) L8 AR-1262-4	8.791	0.000	45261	0	11.326	N.D. #
42) L9 AR-1268-2	8.791	0.000	45261	0	2.742	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102020\
Data File : PO072540.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Oct 2020 15:33
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 16:14:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 14 17:47:24 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

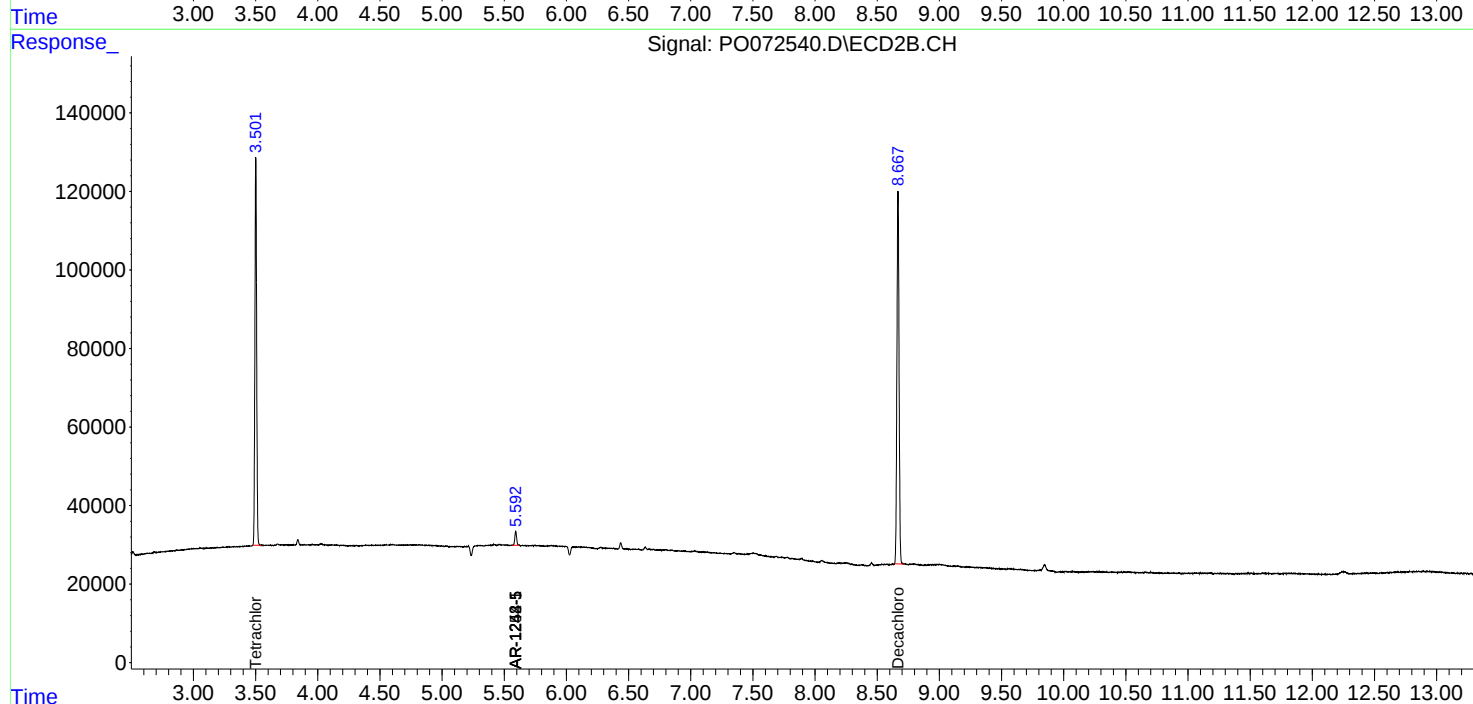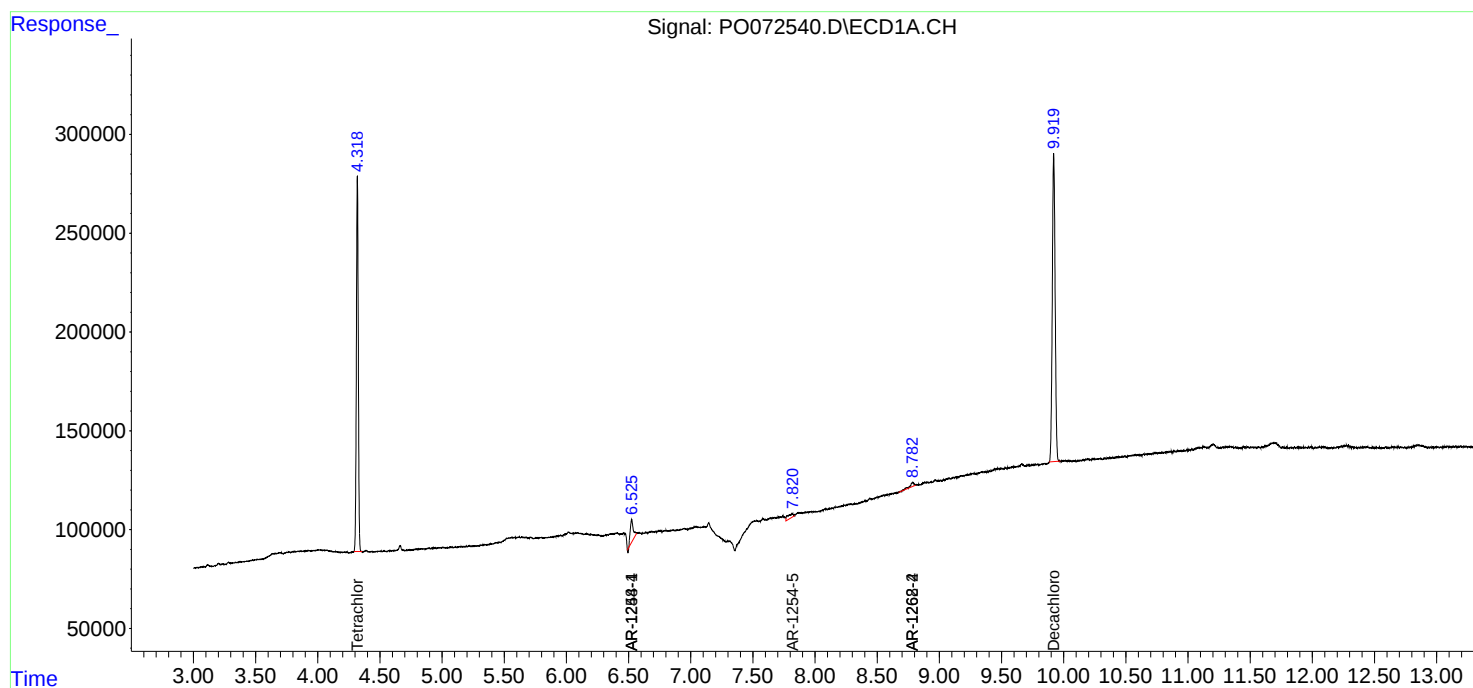


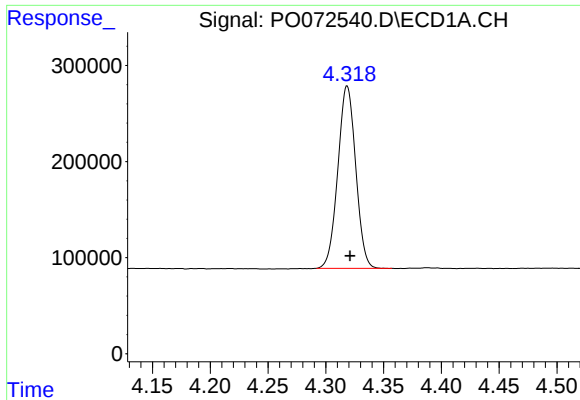

#1 Tetrachloro-m-xylene


R.T.: 4.319 min
Delta R.T.: -0.002 min
Response: 2034978
Conc: 23.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

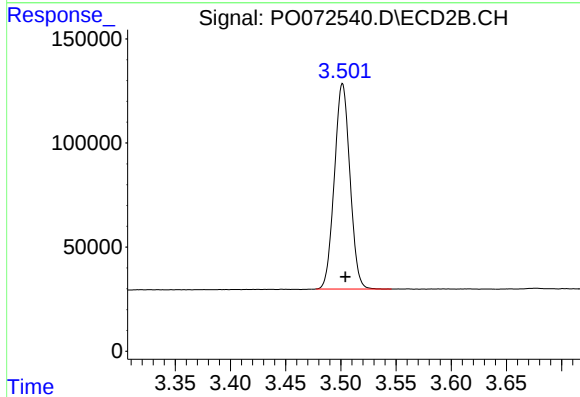


#1 Tetrachloro-m-xylene

R.T.: 3.502 min
Delta R.T.: -0.003 min
Response: 969156
Conc: 23.01 ng/ml

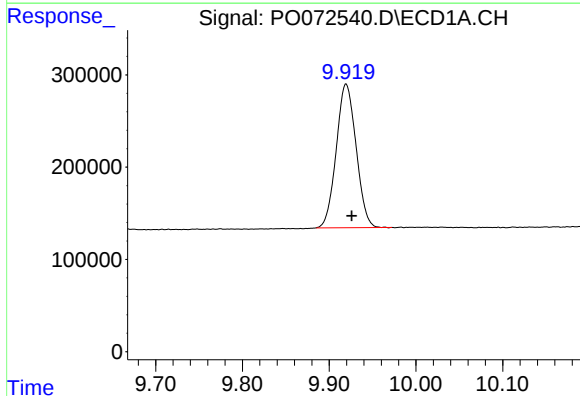


#2 Decachlorobiphenyl

R.T.: 9.919 min
Delta R.T.: -0.006 min
Response: 2473878
Conc: 22.43 ng/ml

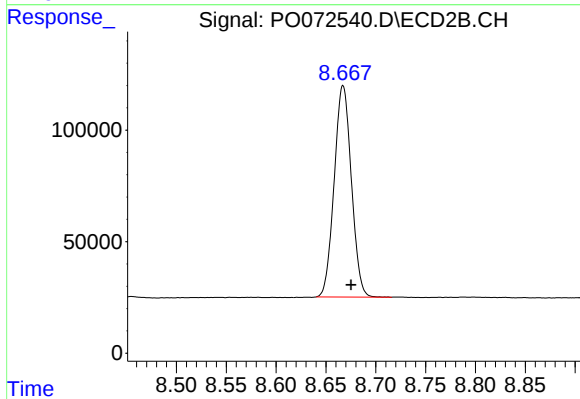

#2 Decachlorobiphenyl


R.T.: 8.667 min
Delta R.T.: -0.008 min
Response: 1137596
Conc: 22.01 ng/ml

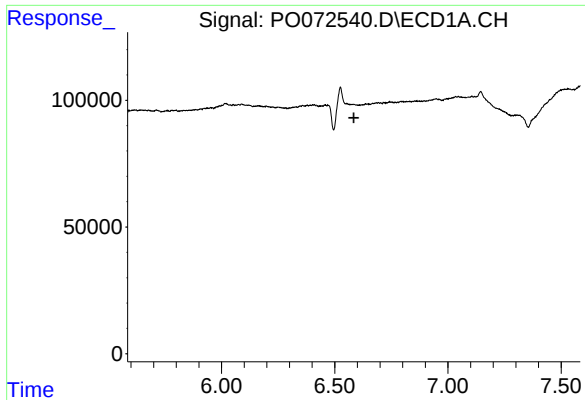

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 6.585 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

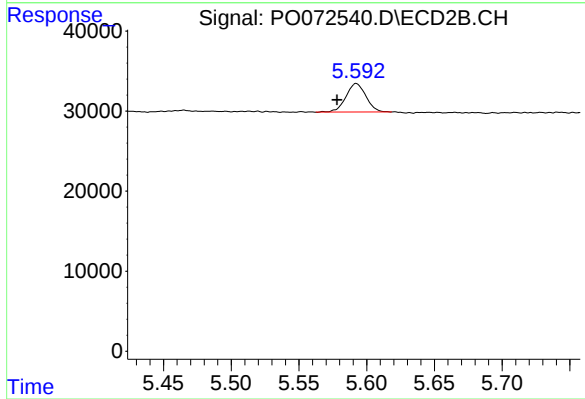


#20 AR-1242-5

R.T.: 5.592 min
Delta R.T.: 0.014 min
Response: 36515
Conc: 26.60 ng/ml

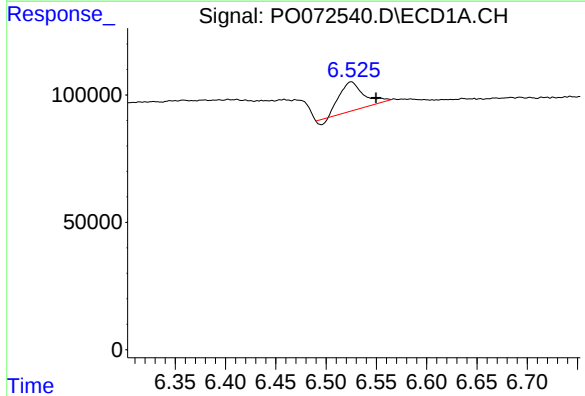


#24 AR-1248-4

R.T.: 6.525 min
Delta R.T.: -0.025 min
Response: 182705
Conc: 41.32 ng/ml

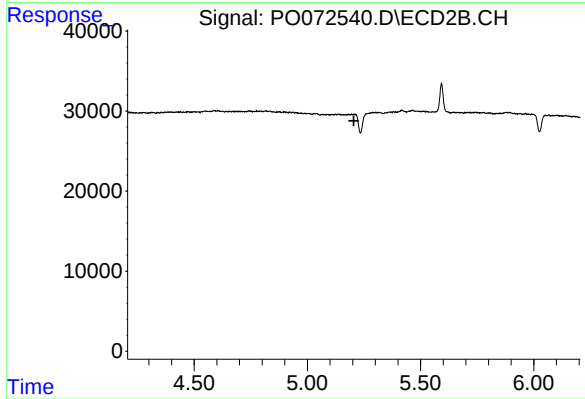

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.205 min
Response: 0
Conc: N.D.

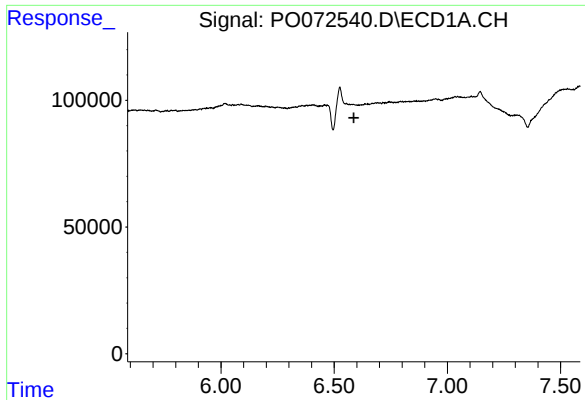

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 6.587 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

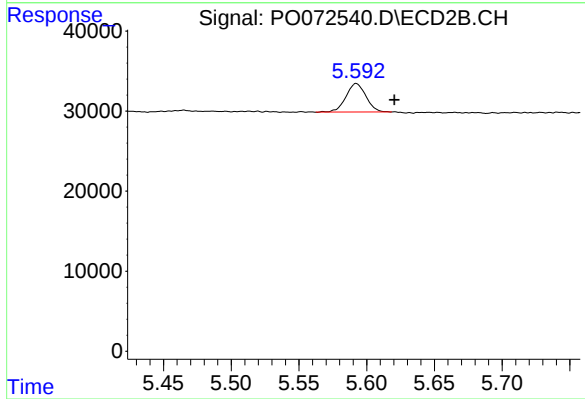


#25 AR-1248-5

R.T.: 5.592 min
Delta R.T.: -0.028 min
Response: 36515
Conc: 19.77 ng/ml

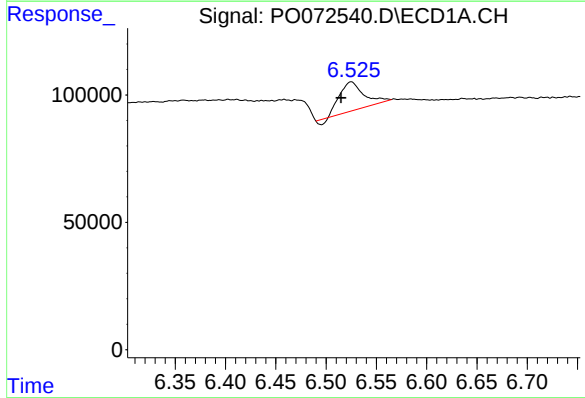


#26 AR-1254-1

R.T.: 6.525 min
Delta R.T.: 0.010 min
Response: 182705
Conc: 43.25 ng/ml

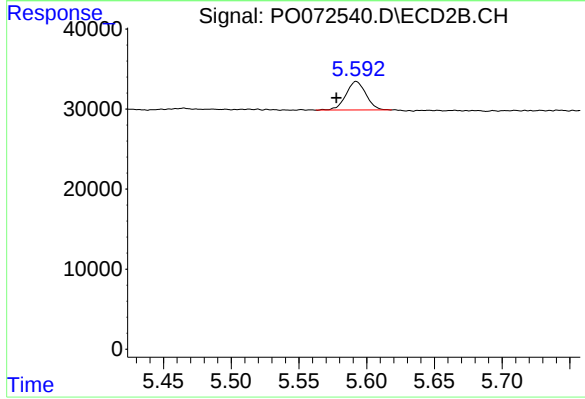

#26 AR-1254-1


R.T.: 5.592 min
Delta R.T.: 0.015 min
Response: 36515
Conc: 13.21 ng/ml

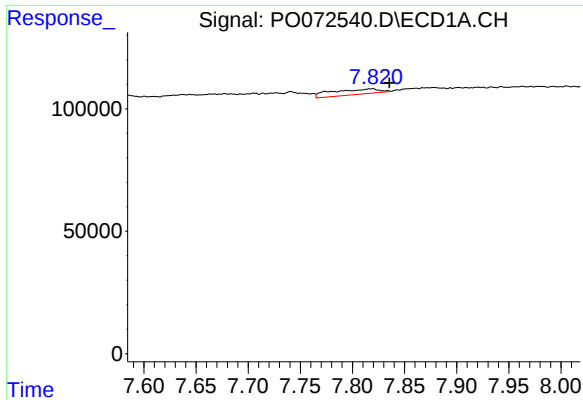

#30 AR-1254-5


R.T.: 7.819 min
Delta R.T.: -0.017 min
Response: 68853
Conc: 10.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

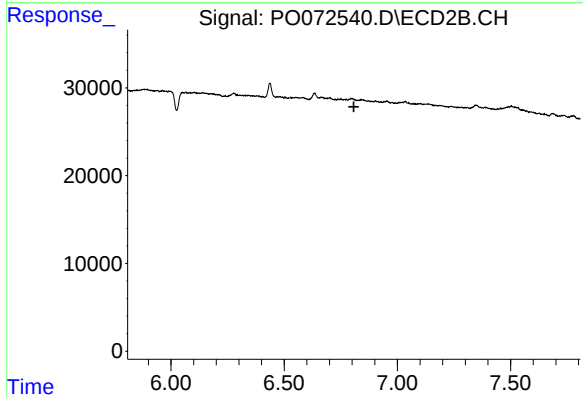


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 6.808 min
Response: 0
Conc: N.D.

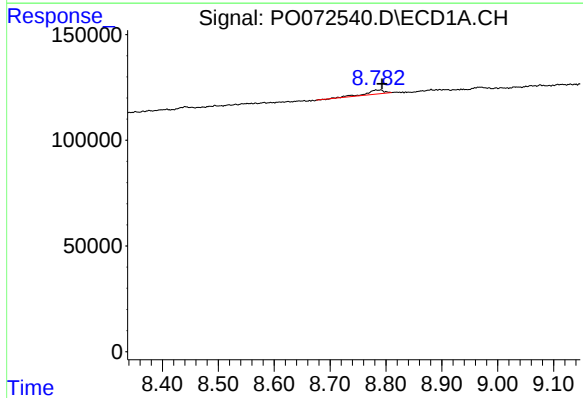


#39 AR-1262-4

R.T.: 8.791 min
Delta R.T.: -0.002 min
Response: 45261
Conc: 11.33 ng/ml

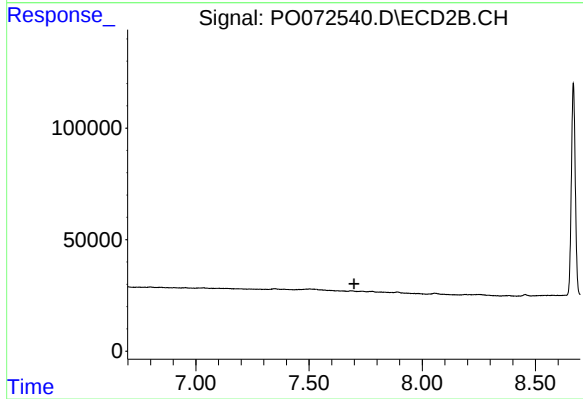

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 7.698 min
Response: 0
Conc: N.D.

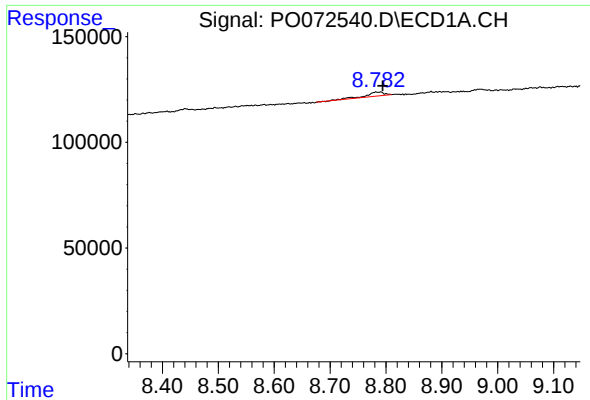

#42 AR-1268-2

R.T.: 8.791 min
Delta R.T.: -0.003 min
Response: 45261
Conc: 2.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

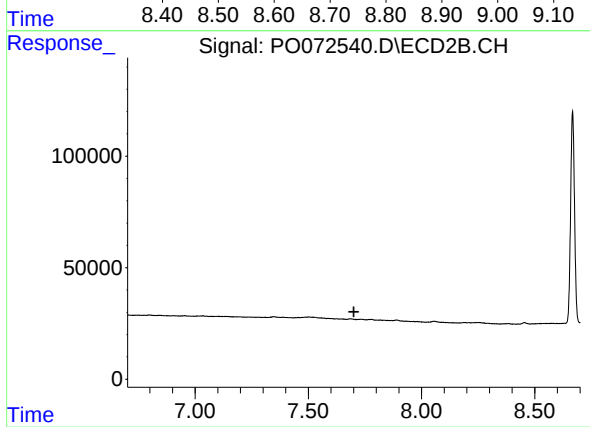

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 7.701 min
Response: 0
Conc: N.D.