

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102020\
 Data File : PO072545.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Oct 2020 17:24
 Operator : DD\AJ
 Sample : L4442-20
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 04:40:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 14 17:47:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.320	3.503	1726328	836026	20.353	19.848
2)	SA Decachlor...	9.921	8.668	1563695	749831	14.176	14.505
Target Compounds							
12)	L3 AR-1232-2	5.333	0.000	54027	0	56.738	N.D. #
25)	L5 AR-1248-5	0.000	5.643f	0	179175	N.D.	97.007 #
28)	L6 AR-1254-3	0.000	6.149	0	84566	N.D.	21.976 #
29)	L6 AR-1254-4	7.407	0.000	36119	0	5.449	N.D. #
35)	L7 AR-1260-5	8.448	0.000	22103	0	1.521	N.D. #
37)	L8 AR-1262-2	8.448	0.000	22103	0	1.383	N.D. #
39)	L8 AR-1262-4	8.786	0.000	47380	0	11.856	N.D. #
42)	L9 AR-1268-2	8.786	0.000	47380	0	2.870	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102020\
Data File : PO072545.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Oct 2020 17:24
Operator : DD\AJ
Sample : L4442-20
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 04:40:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 14 17:47:24 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

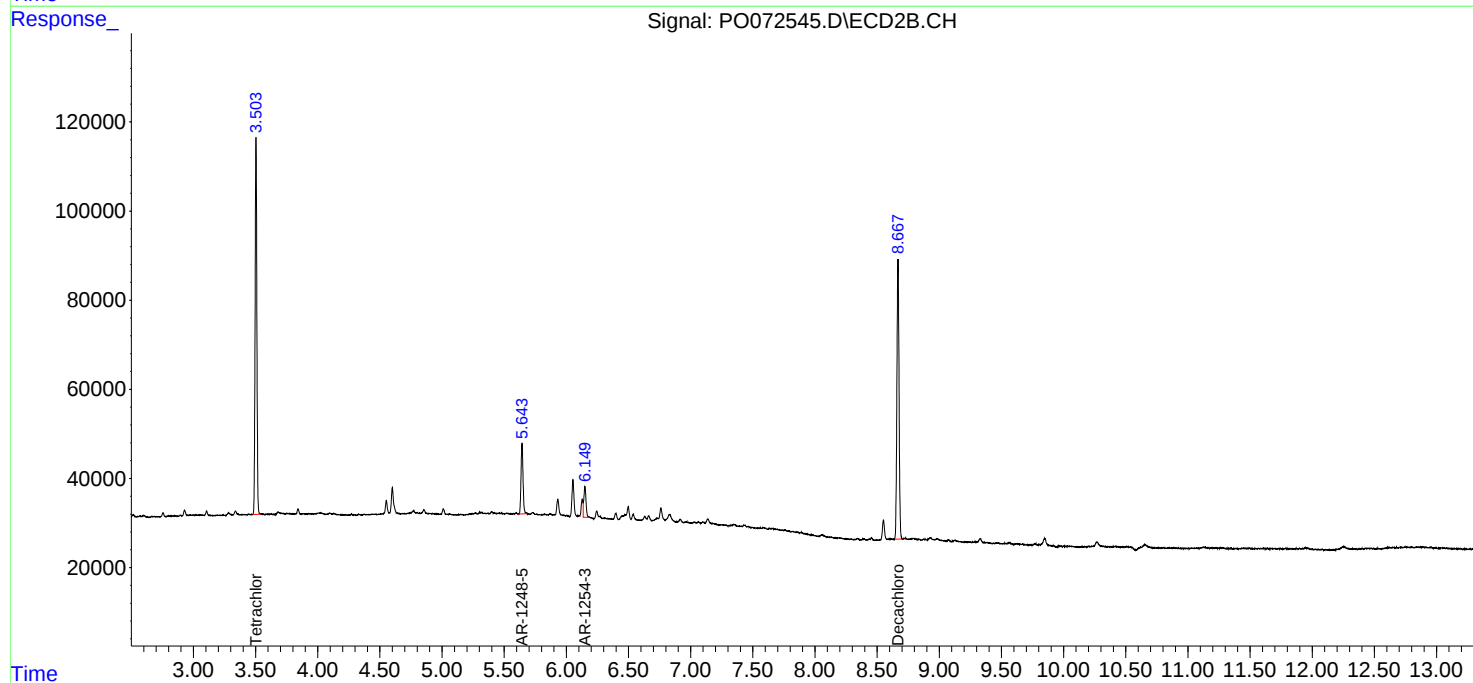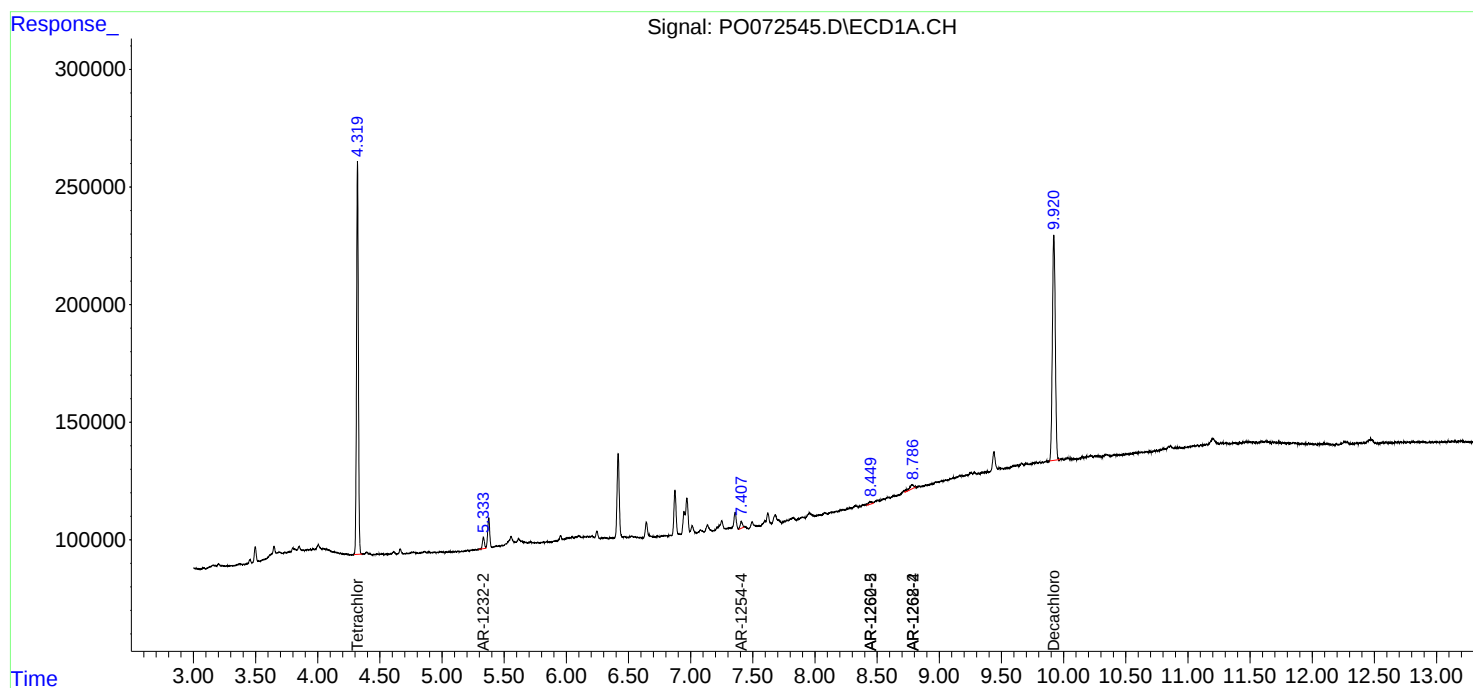


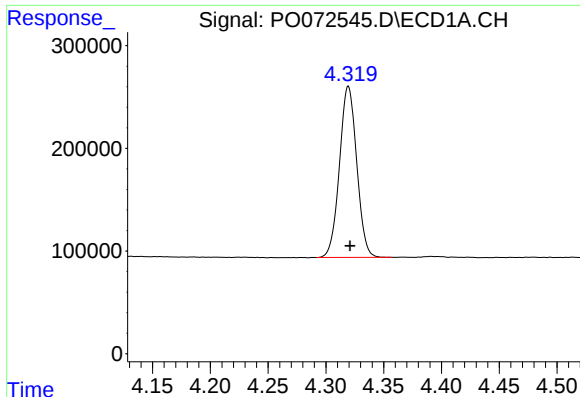

#1 Tetrachloro-m-xylene


R.T.: 4.320 min
Delta R.T.: -0.001 min
Response: 1726328
Conc: 20.35 ng/ml

Instrument :
ECD_O
ClientSampleId :

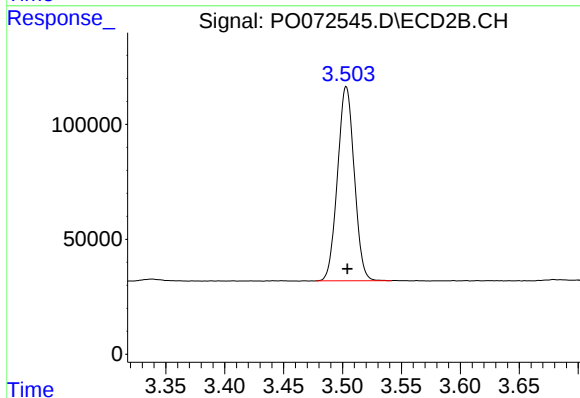


#1 Tetrachloro-m-xylene

R.T.: 3.503 min
Delta R.T.: -0.001 min
Response: 836026
Conc: 19.85 ng/ml

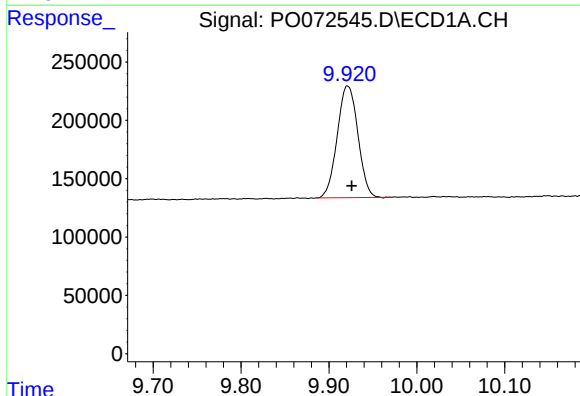


#2 Decachlorobiphenyl

R.T.: 9.921 min
Delta R.T.: -0.005 min
Response: 1563695
Conc: 14.18 ng/ml

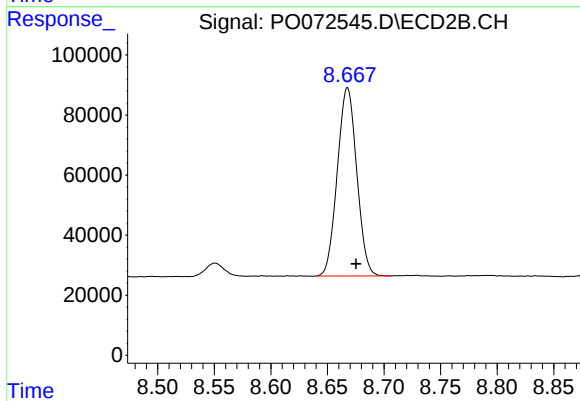

#2 Decachlorobiphenyl


R.T.: 8.668 min
Delta R.T.: -0.007 min
Response: 749831
Conc: 14.50 ng/ml

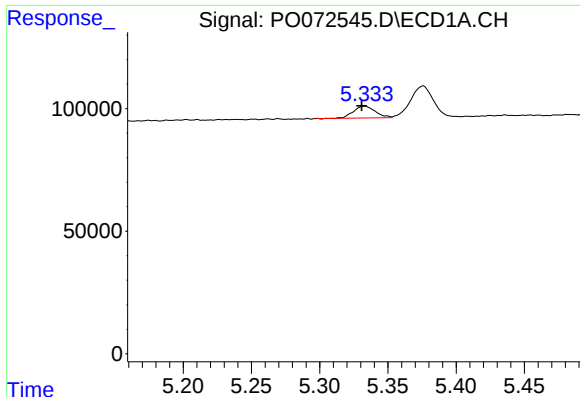

#12 AR-1232-2


R.T.: 5.333 min
Delta R.T.: 0.002 min
Response: 54027
Conc: 56.74 ng/ml

Instrument :
ECD_O
ClientSampleId :

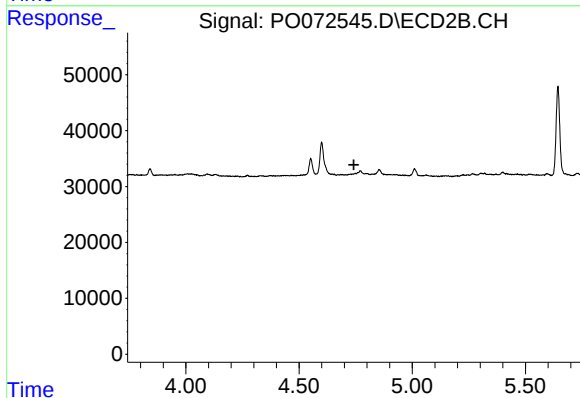


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 4.742 min
Response: 0
Conc: N.D.

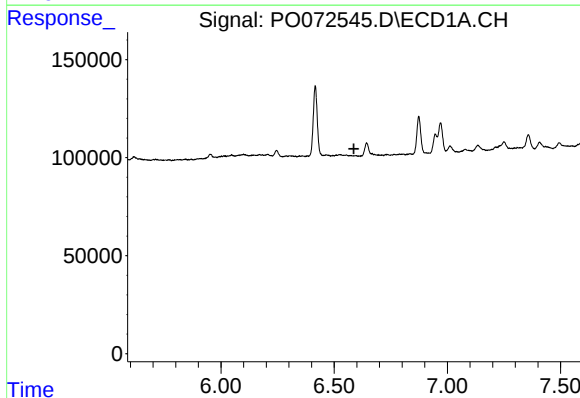


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 6.587 min
Response: 0
Conc: N.D.

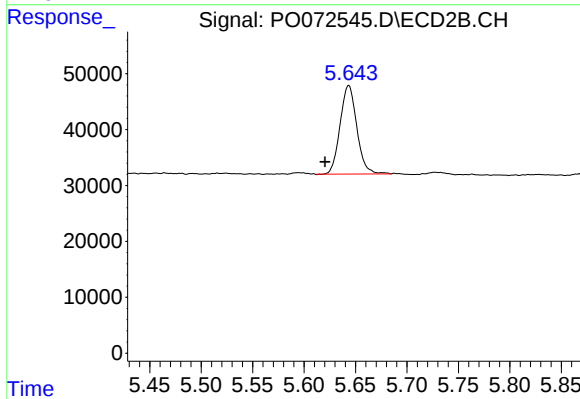

#25 AR-1248-5


R.T.: 5.643 min
Delta R.T.: 0.023 min
Response: 179175
Conc: 97.01 ng/ml

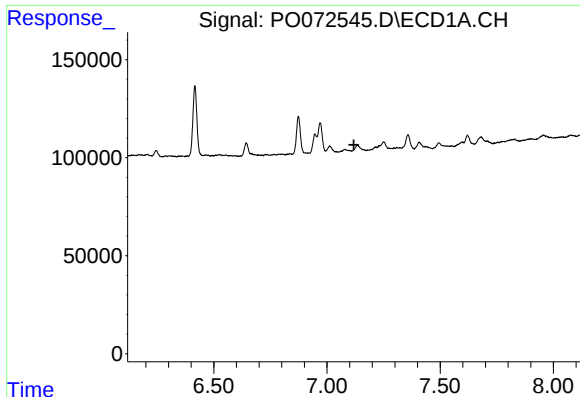

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T.: 7.119 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

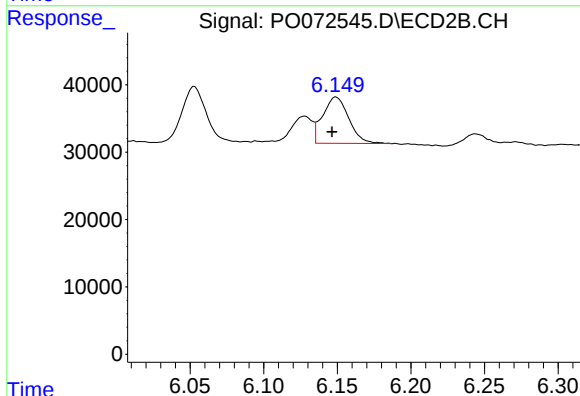


#28 AR-1254-3

R.T.: 6.149 min
Delta R.T.: 0.003 min
Response: 84566
Conc: 21.98 ng/ml

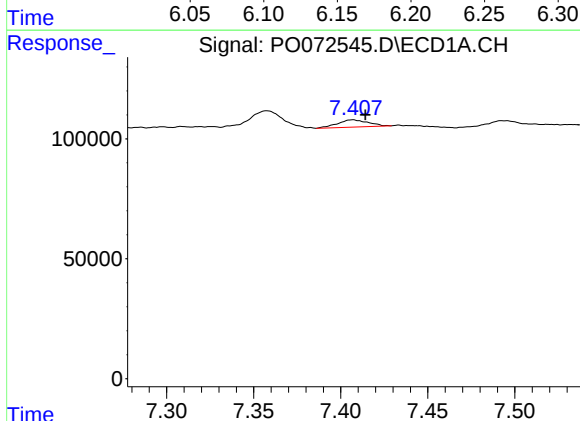


#29 AR-1254-4

R.T.: 7.407 min
Delta R.T.: -0.007 min
Response: 36119
Conc: 5.45 ng/ml

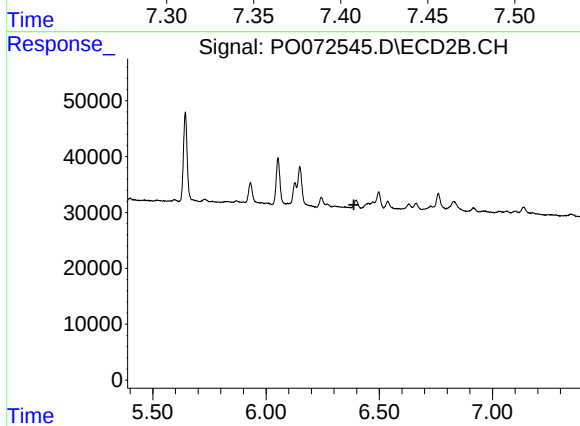

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T.: 6.388 min
Response: 0
Conc: N.D.

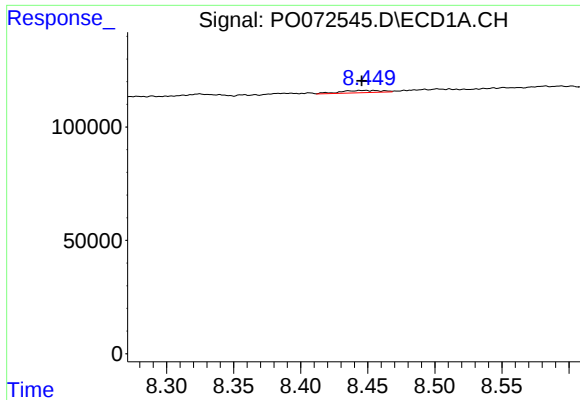

#35 AR-1260-5


R.T.: 8.448 min
Delta R.T.: 0.003 min
Response: 22103
Conc: 1.52 ng/ml

Instrument :
ECD_O
ClientSampleId :

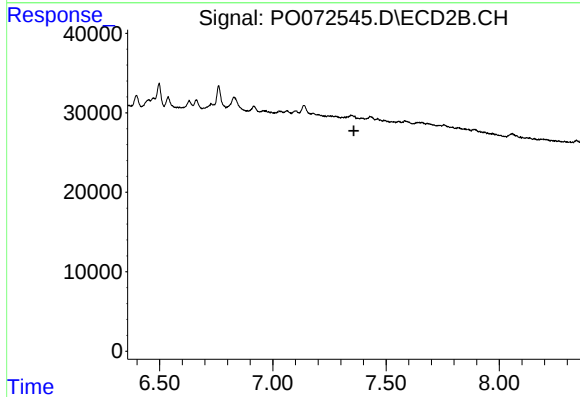


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.358 min
Response: 0
Conc: N.D.

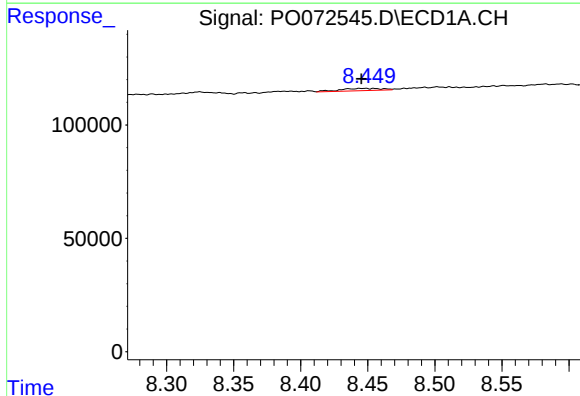


#37 AR-1262-2

R.T.: 8.448 min
Delta R.T.: 0.003 min
Response: 22103
Conc: 1.38 ng/ml

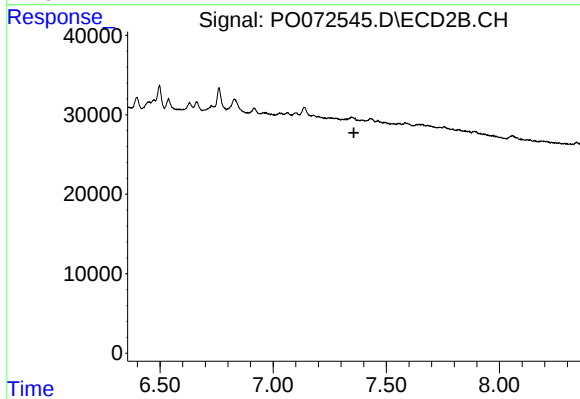

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 7.357 min
Response: 0
Conc: N.D.

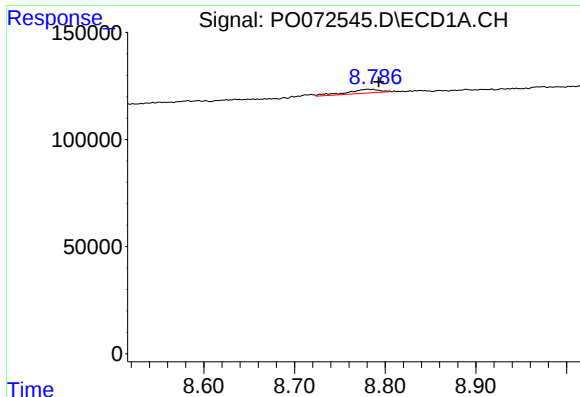

#39 AR-1262-4


R.T.: 8.786 min
Delta R.T.: -0.007 min
Response: 47380
Conc: 11.86 ng/ml

Instrument :
ECD_O
ClientSampleId :

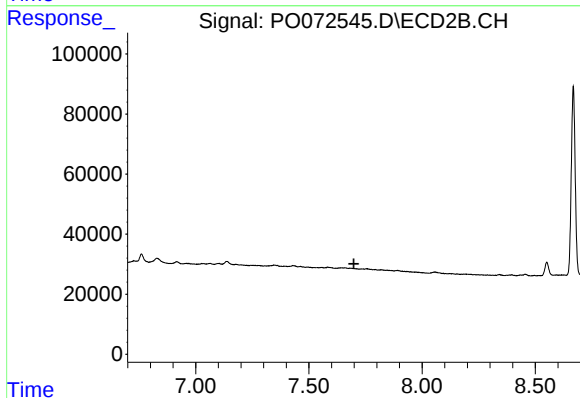


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 7.698 min
Response: 0
Conc: N.D.

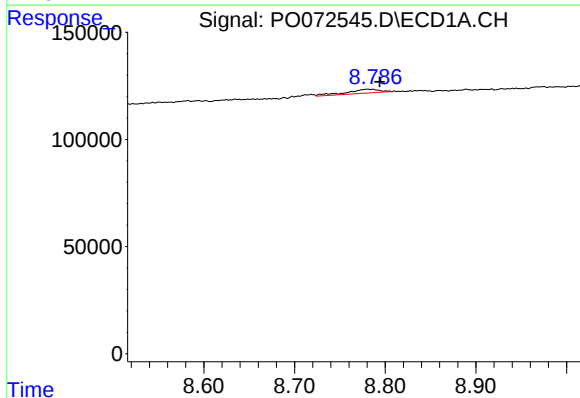

#42 AR-1268-2

R.T.: 8.786 min
Delta R.T.: -0.008 min
Response: 47380
Conc: 2.87 ng/ml

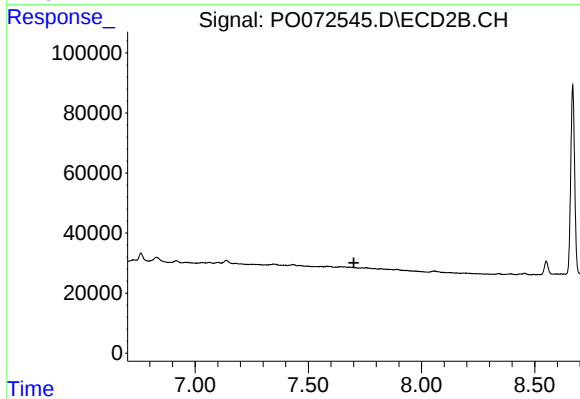

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 7.701 min
Response: 0
Conc: N.D.