

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102020\
 Data File : PO072552.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Oct 2020 19:24
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 04:43:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 14 17:47:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.319	3.503	1933556	941019	22.796	22.340
2)	SA Decachlor...	9.921	8.668	2473466	1148993	22.424	22.226
Target Compounds							
20)	L4 AR-1242-5	0.000	5.594	0	41182	N.D.	29.996 #
24)	L5 AR-1248-4	6.526f	0.000	169772	0	38.391	N.D. #
25)	L5 AR-1248-5	0.000	5.594f	0	41182	N.D.	22.297 #
26)	L6 AR-1254-1	6.526	5.594f	169772	41182	40.188	14.899 #
29)	L6 AR-1254-4	7.418	0.000	204116	0	30.795	N.D. #
30)	L6 AR-1254-5	7.823	0.000	42900	0	6.697	N.D. #
39)	L8 AR-1262-4	8.783	0.000	88440	0	22.131	N.D. #
42)	L9 AR-1268-2	8.783	0.000	88440	0	5.357	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102020\
Data File : PO072552.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Oct 2020 19:24
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 04:43:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 14 17:47:24 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

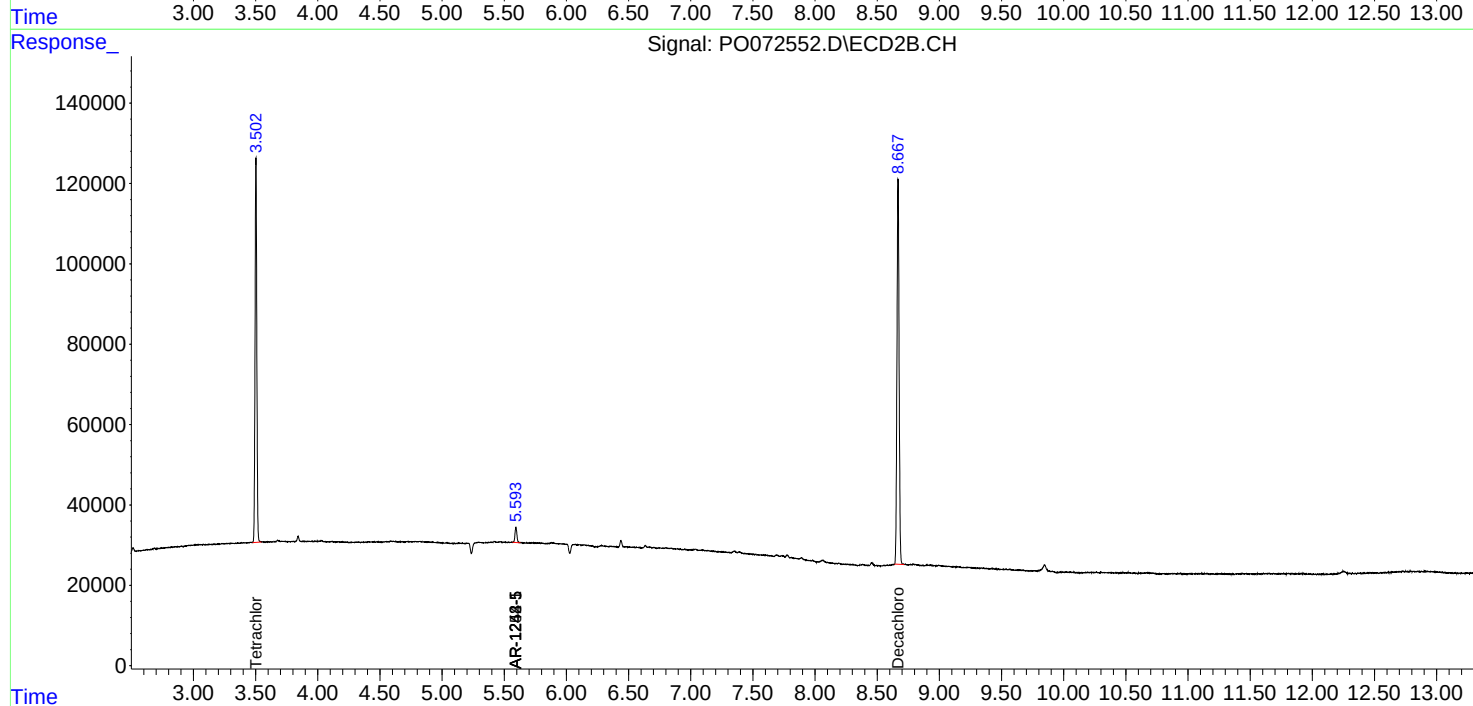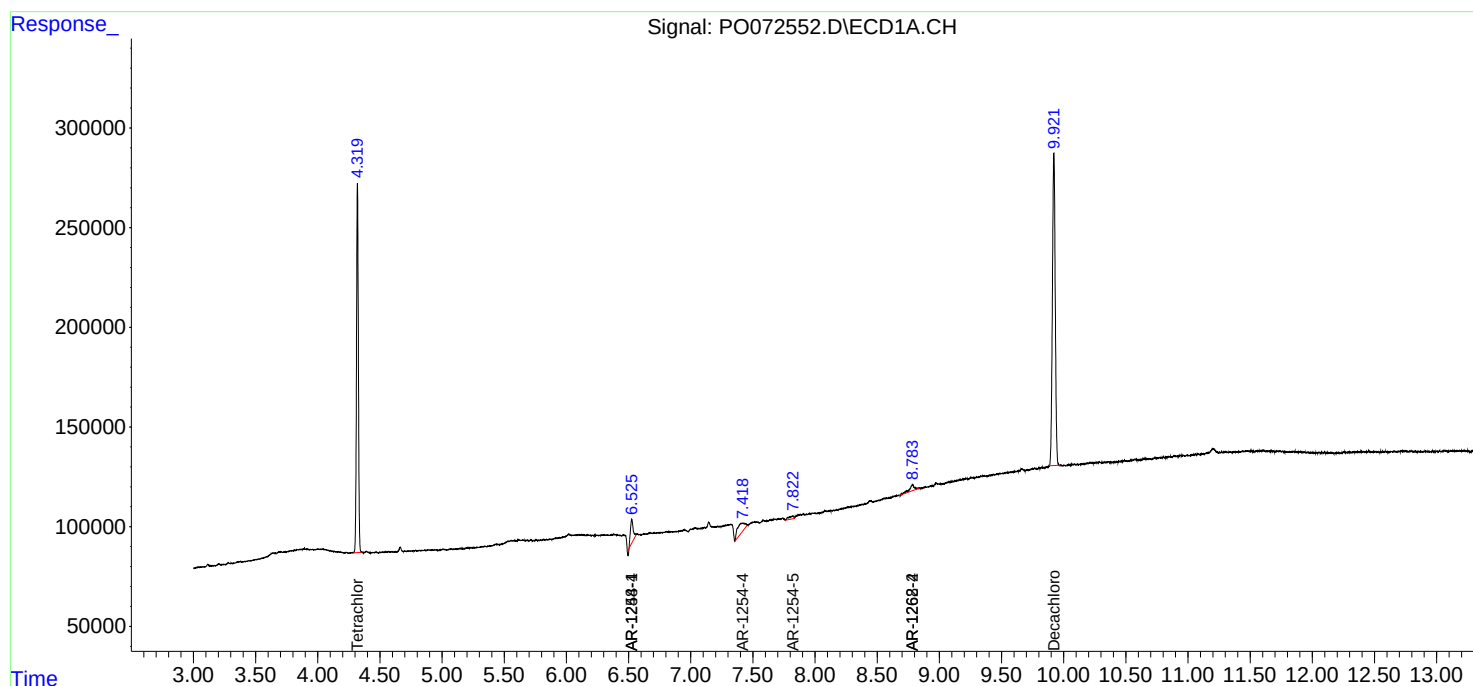


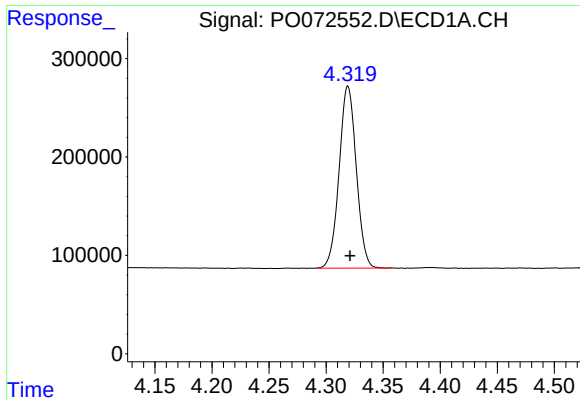

#1 Tetrachloro-m-xylene


R.T.: 4.319 min
Delta R.T.: -0.002 min
Response: 1933556
Conc: 22.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

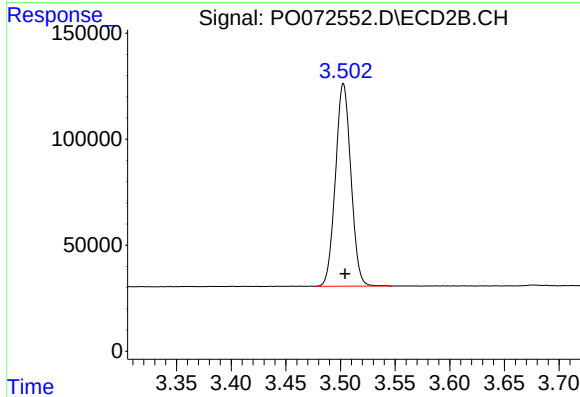


#1 Tetrachloro-m-xylene

R.T.: 3.503 min
Delta R.T.: -0.001 min
Response: 941019
Conc: 22.34 ng/ml

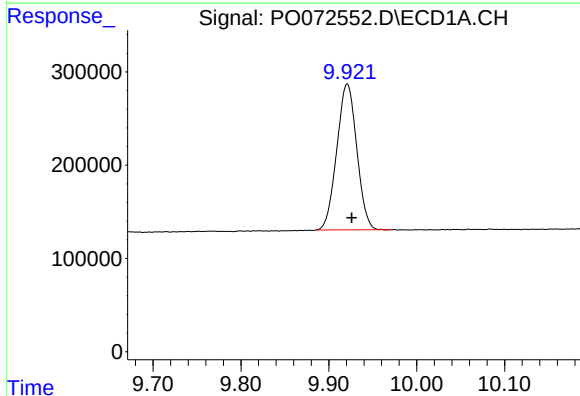


#2 Decachlorobiphenyl

R.T.: 9.921 min
Delta R.T.: -0.005 min
Response: 2473466
Conc: 22.42 ng/ml

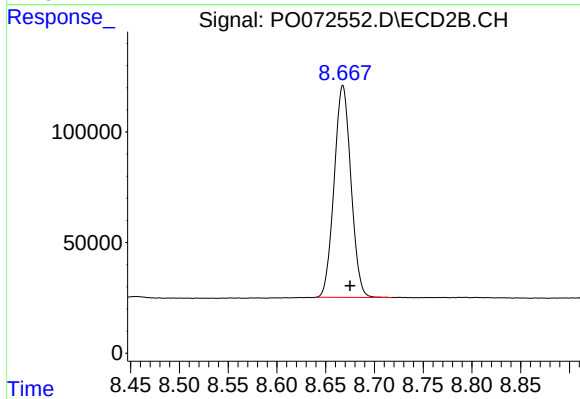

#2 Decachlorobiphenyl


R.T.: 8.668 min
Delta R.T.: -0.008 min
Response: 1148993
Conc: 22.23 ng/ml

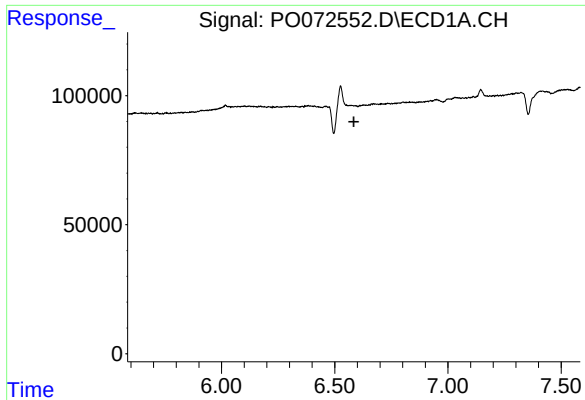

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 6.585 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

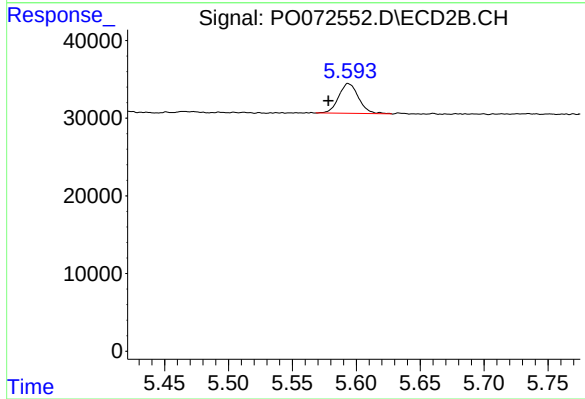


#20 AR-1242-5

R.T.: 5.594 min
Delta R.T.: 0.015 min
Response: 41182
Conc: 30.00 ng/ml

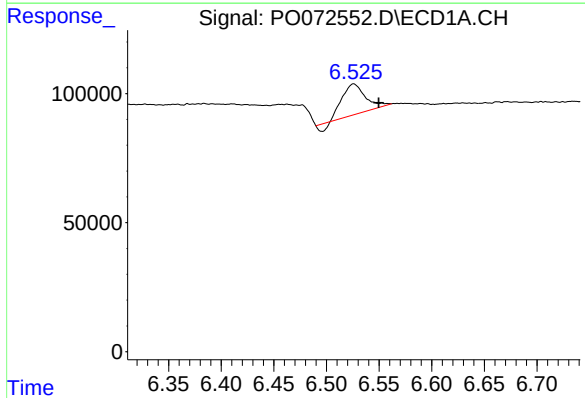


#24 AR-1248-4

R.T.: 6.526 min
Delta R.T.: -0.024 min
Response: 169772
Conc: 38.39 ng/ml

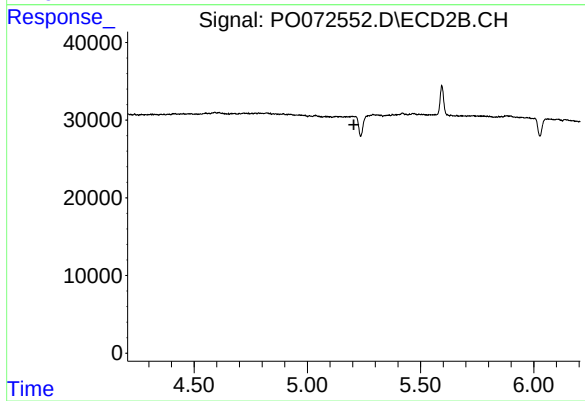

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.205 min
Response: 0
Conc: N.D.

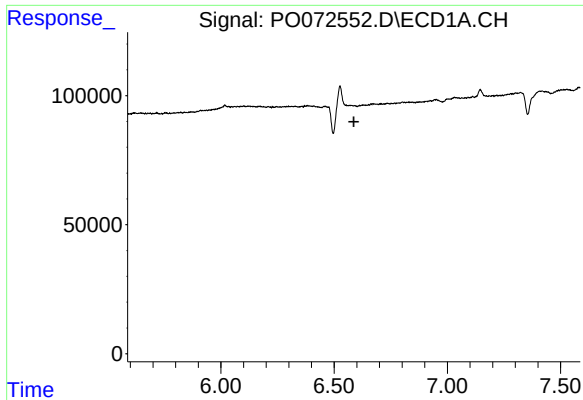

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 6.587 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

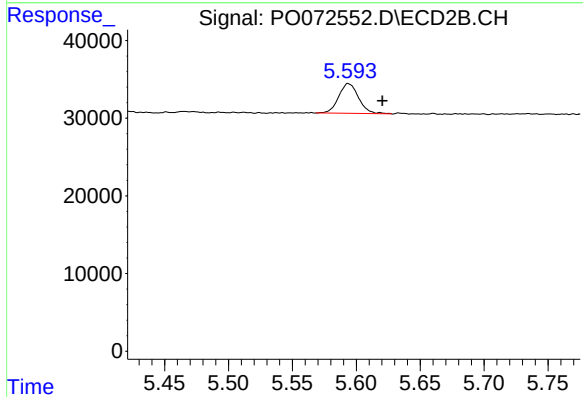


#25 AR-1248-5

R.T.: 5.594 min
Delta R.T.: -0.027 min
Response: 41182
Conc: 22.30 ng/ml

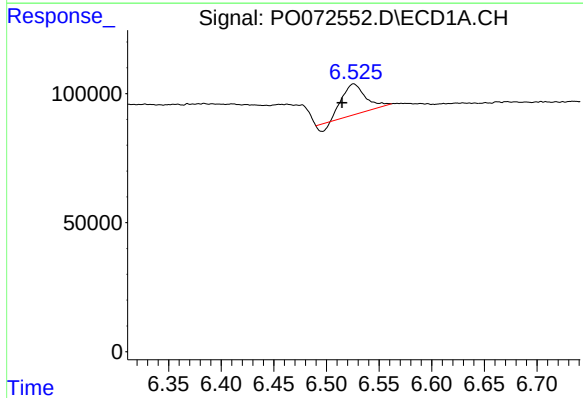


#26 AR-1254-1

R.T.: 6.526 min
Delta R.T.: 0.011 min
Response: 169772
Conc: 40.19 ng/ml

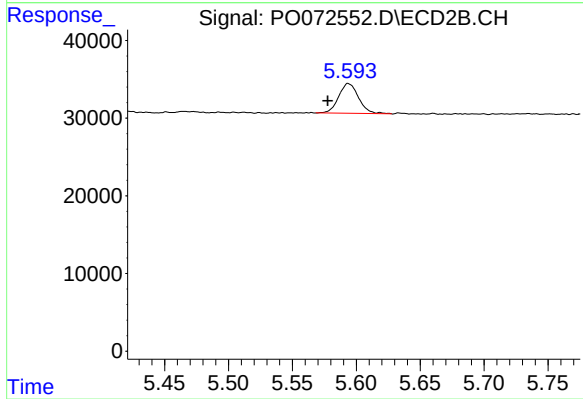

#26 AR-1254-1


R.T.: 5.594 min
Delta R.T.: 0.016 min
Response: 41182
Conc: 14.90 ng/ml

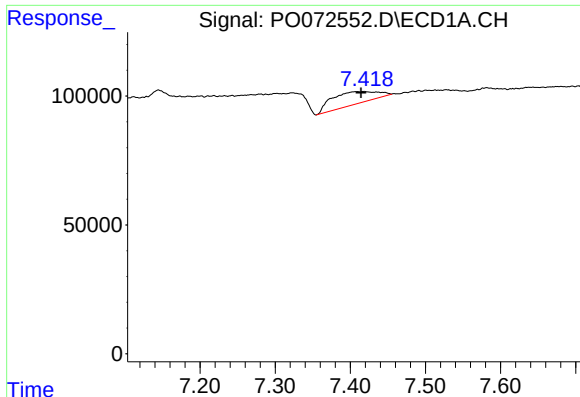

#29 AR-1254-4


R.T.: 7.418 min
Delta R.T.: 0.004 min
Response: 204116
Conc: 30.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

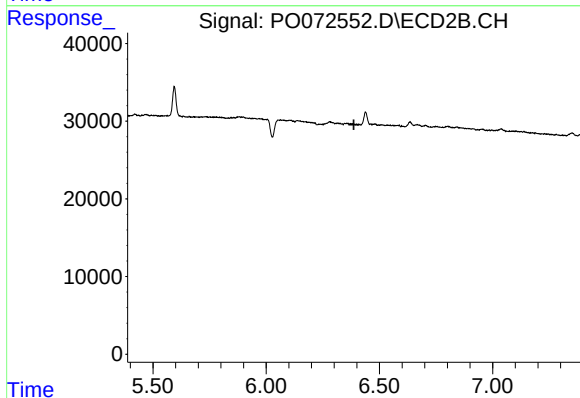


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.388 min
Response: 0
Conc: N.D.

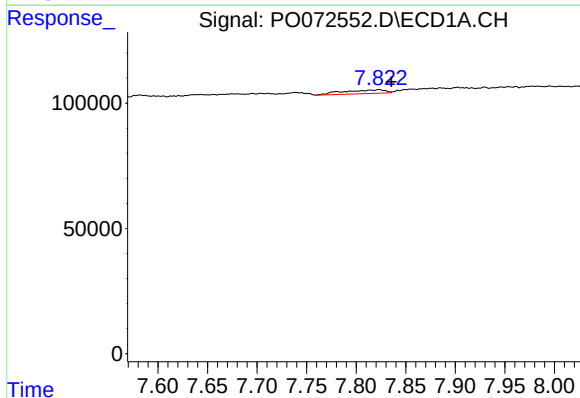


#30 AR-1254-5

R.T.: 7.823 min
Delta R.T.: -0.013 min
Response: 42900
Conc: 6.70 ng/ml

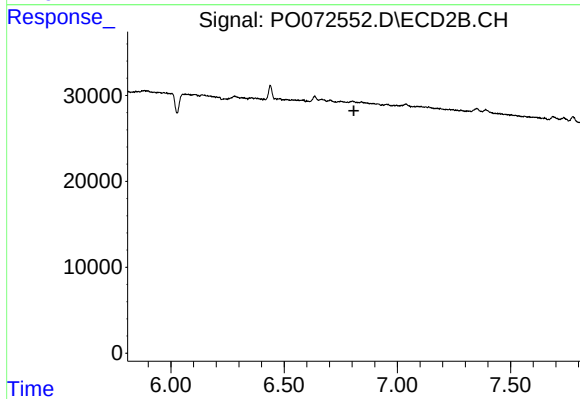

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 6.808 min
Response: 0
Conc: N.D.

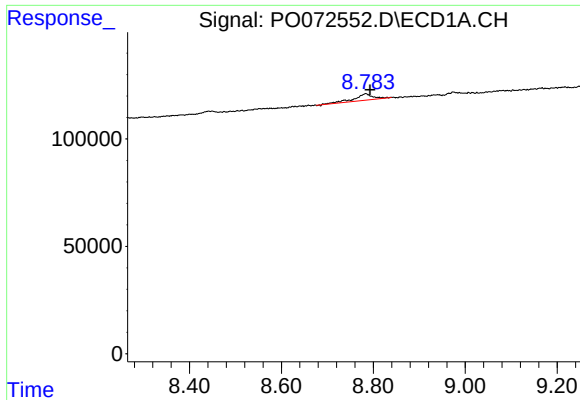

#39 AR-1262-4


R.T.: 8.783 min
Delta R.T.: -0.010 min
Response: 88440
Conc: 22.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

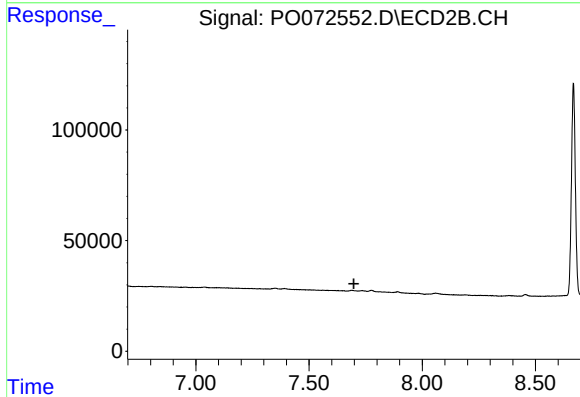


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 7.698 min
Response: 0
Conc: N.D.

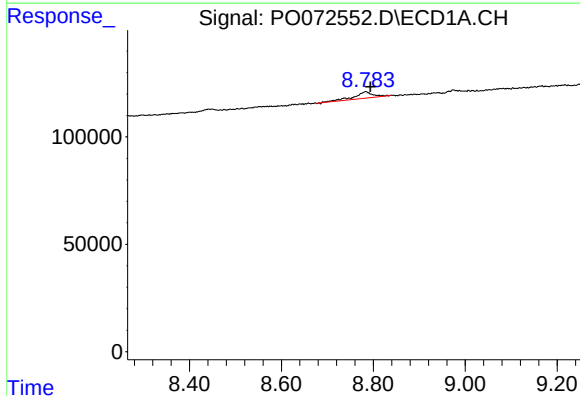

#42 AR-1268-2

R.T.: 8.783 min
Delta R.T.: -0.011 min
Response: 88440
Conc: 5.36 ng/ml

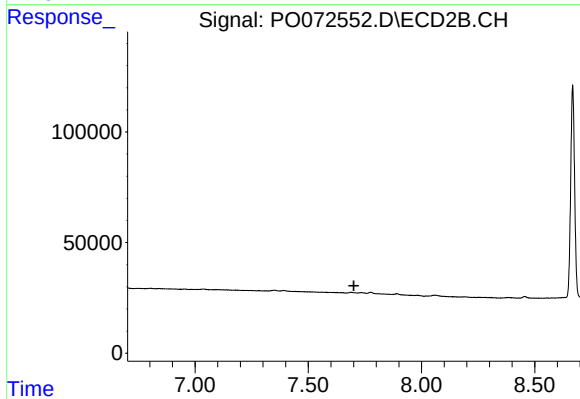

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 7.701 min
Response: 0
Conc: N.D.