

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102020\
 Data File : PO072588.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Oct 2020 6:32
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 06:58:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 14 17:47:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.319	3.503	1862583	1025153	21.960	24.338
2) SA Decachlor...	9.919	8.667	1895350	901460	17.183	17.438
Target Compounds						
20) L4 AR-1242-5	0.000	5.592	0	43506	N.D.	31.689 #
24) L5 AR-1248-4	6.524f	0.000	87171	0	19.712	N.D. #
25) L5 AR-1248-5	0.000	5.592f	0	43506	N.D.	23.555 #
26) L6 AR-1254-1	6.524	5.592	87171	43506	20.635	15.739
39) L8 AR-1262-4	8.779	0.000	45150	0	11.298	N.D. #
40) L8 AR-1262-5	9.342	0.000	185952	0	34.954	N.D. #
42) L9 AR-1268-2	8.779f	0.000	45150	0	2.735	N.D. #
44) L9 AR-1268-4	9.342	0.000	185952	0	31.165	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102020\
Data File : PO072588.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Oct 2020 6:32
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 06:58:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 14 17:47:24 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

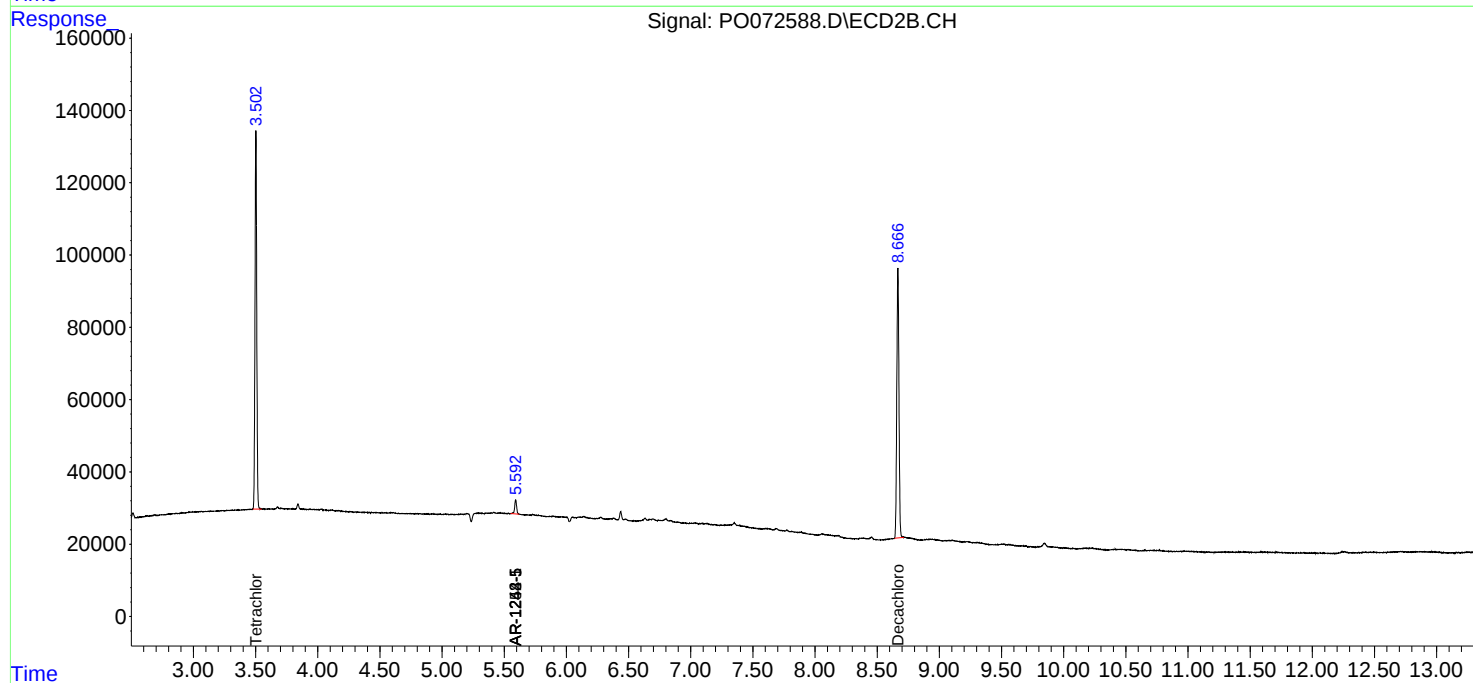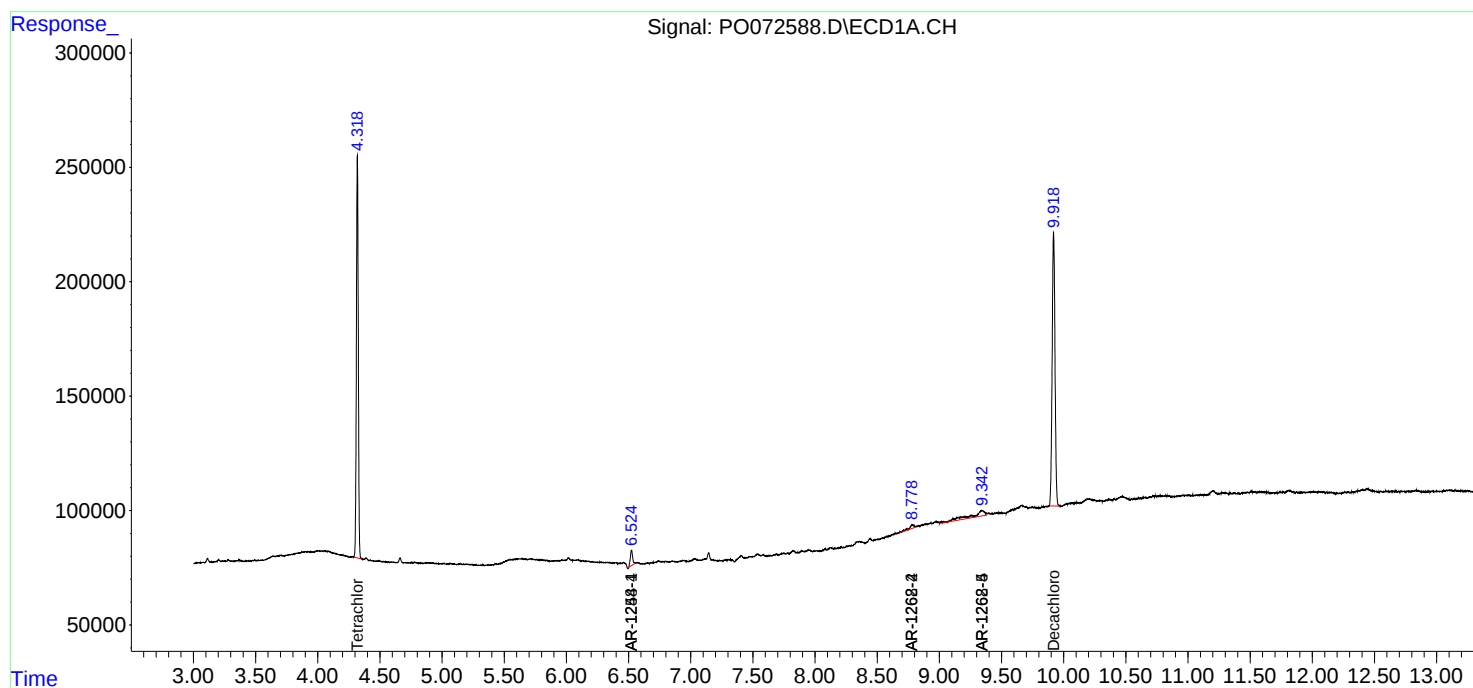


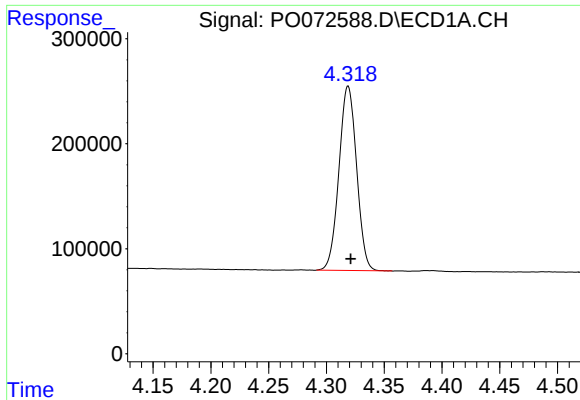

#1 Tetrachloro-m-xylene


R.T.: 4.319 min
Delta R.T.: -0.002 min
Response: 1862583
Conc: 21.96 ng/ml

Instrument :
ECD_O
ClientSampleId :

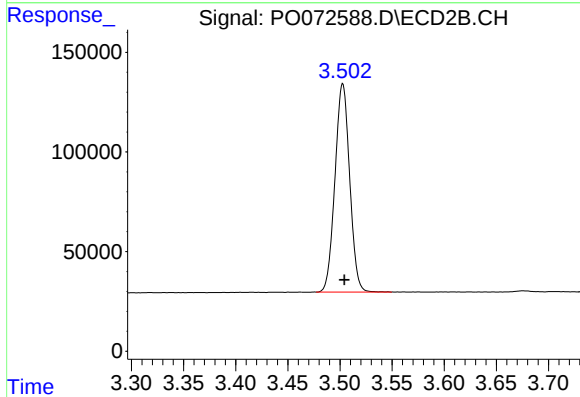


#1 Tetrachloro-m-xylene

R.T.: 3.503 min
Delta R.T.: -0.002 min
Response: 1025153
Conc: 24.34 ng/ml

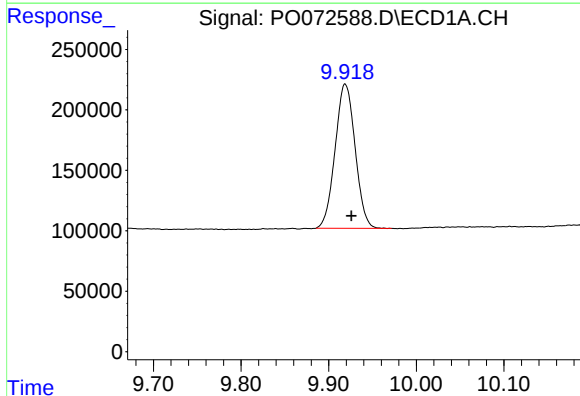


#2 Decachlorobiphenyl

R.T.: 9.919 min
Delta R.T.: -0.007 min
Response: 1895350
Conc: 17.18 ng/ml

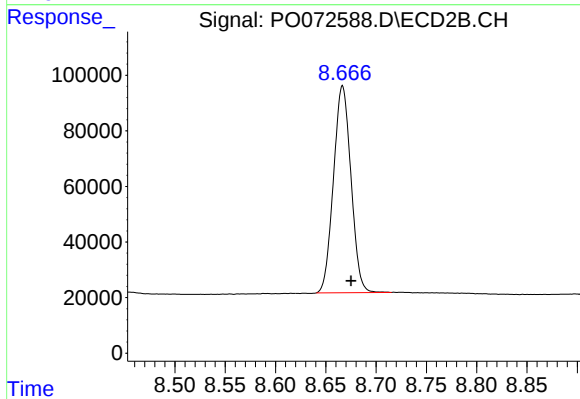

#2 Decachlorobiphenyl


R.T.: 8.667 min
Delta R.T.: -0.009 min
Response: 901460
Conc: 17.44 ng/ml

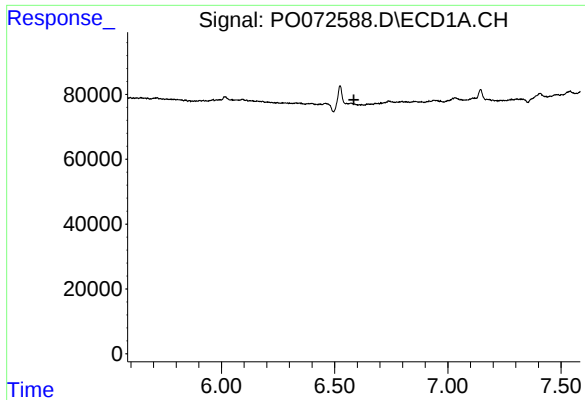

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 6.585 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

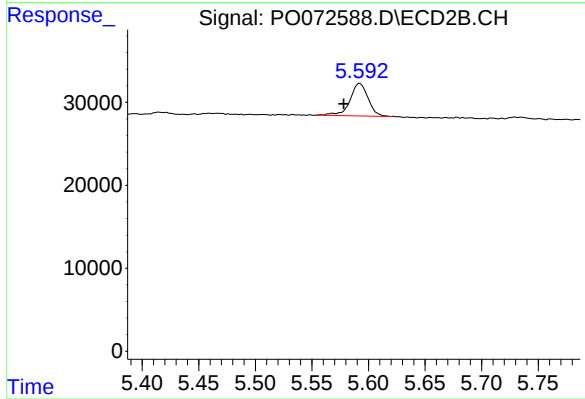


#20 AR-1242-5

R.T.: 5.592 min
Delta R.T.: 0.014 min
Response: 43506
Conc: 31.69 ng/ml

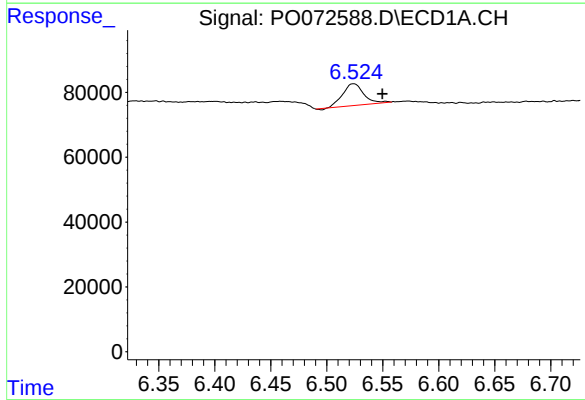


#24 AR-1248-4

R.T.: 6.524 min
Delta R.T.: -0.026 min
Response: 87171
Conc: 19.71 ng/ml

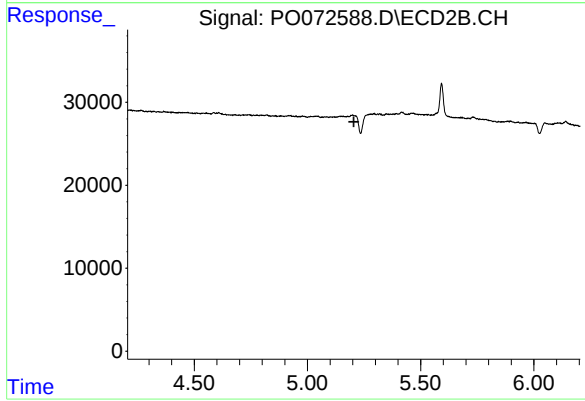

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.205 min
Response: 0
Conc: N.D.

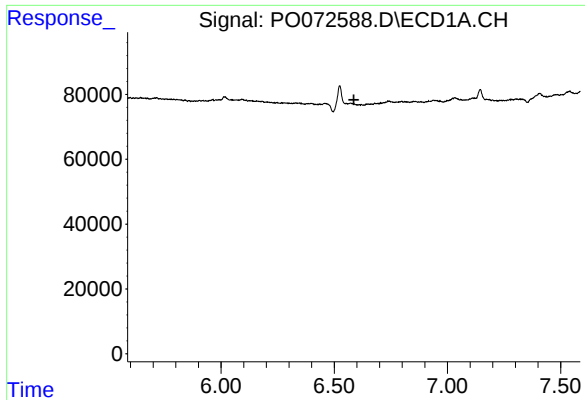

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 6.587 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

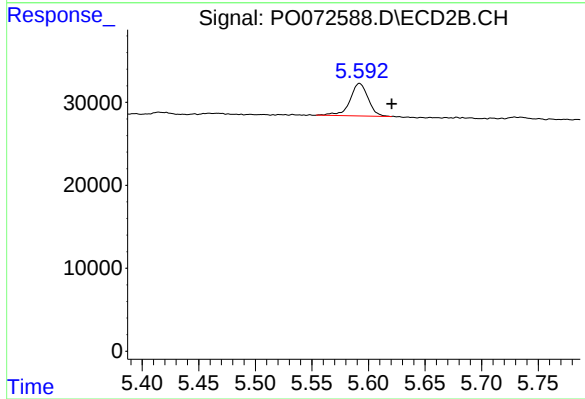


#25 AR-1248-5

R.T.: 5.592 min
Delta R.T.: -0.028 min
Response: 43506
Conc: 23.55 ng/ml

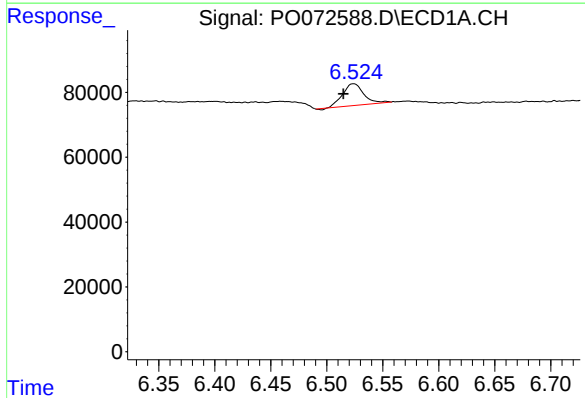


#26 AR-1254-1

R.T.: 6.524 min
Delta R.T.: 0.009 min
Response: 87171
Conc: 20.64 ng/ml

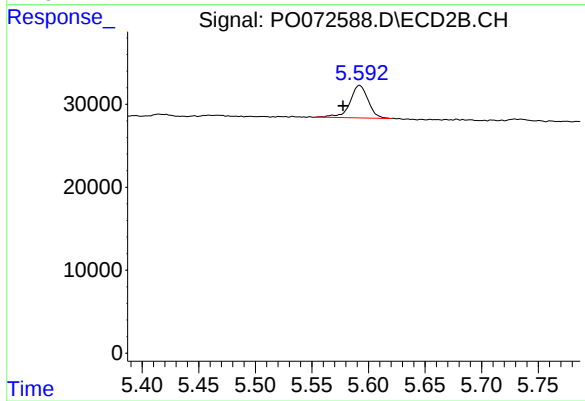

#26 AR-1254-1


R.T.: 5.592 min
Delta R.T.: 0.014 min
Response: 43506
Conc: 15.74 ng/ml

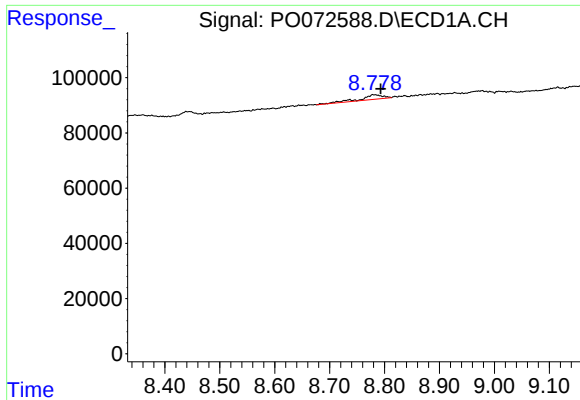

#39 AR-1262-4


R.T.: 8.779 min
Delta R.T.: -0.014 min
Response: 45150
Conc: 11.30 ng/ml

Instrument :
ECD_O
ClientSampleId :

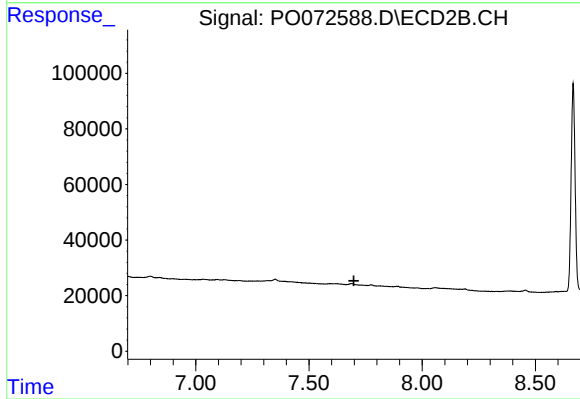


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 7.698 min
Response: 0
Conc: N.D.

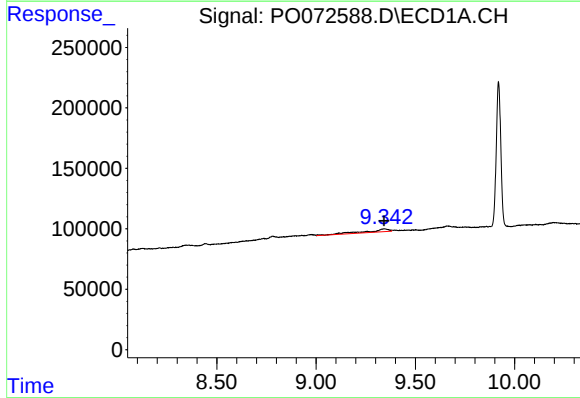


#40 AR-1262-5

R.T.: 9.342 min
Delta R.T.: 0.000 min
Response: 185952
Conc: 34.95 ng/ml

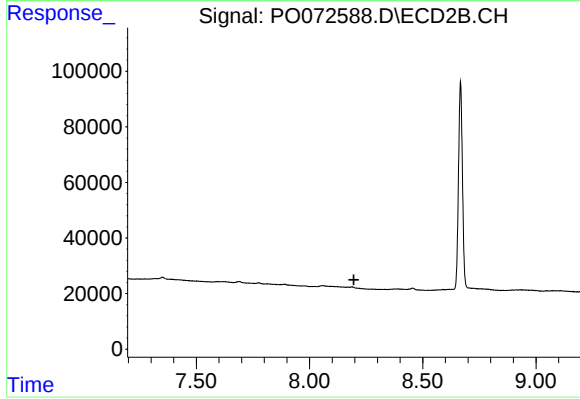

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 8.195 min
Response: 0
Conc: N.D.

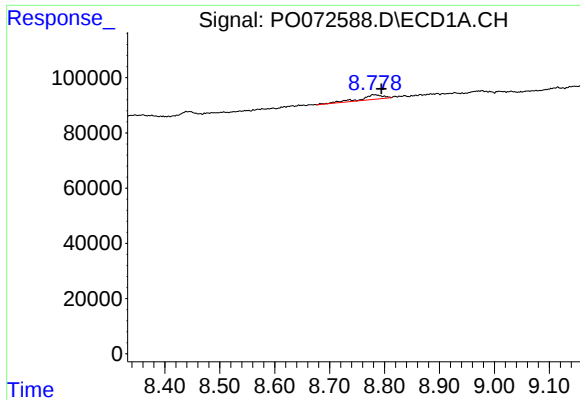

#42 AR-1268-2


R.T.: 8.779 min
Delta R.T.: -0.015 min
Response: 45150
Conc: 2.73 ng/ml

Instrument :
ECD_O
ClientSampleId :

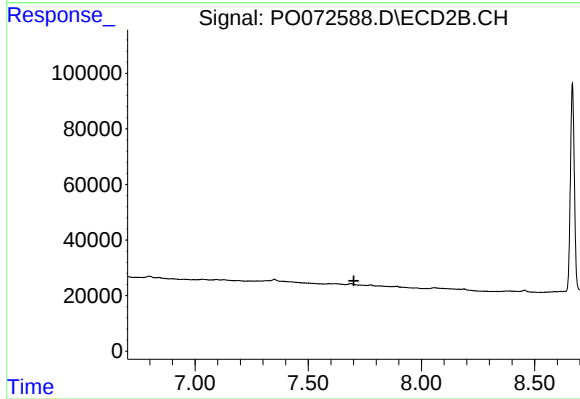


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 7.701 min
Response: 0
Conc: N.D.

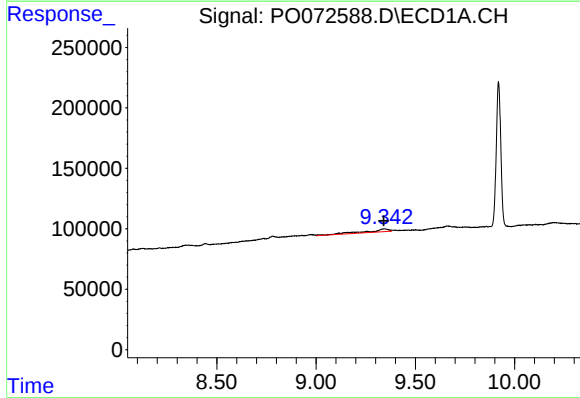

#44 AR-1268-4

R.T.: 9.342 min
Delta R.T.: 0.000 min
Response: 185952
Conc: 31.17 ng/ml

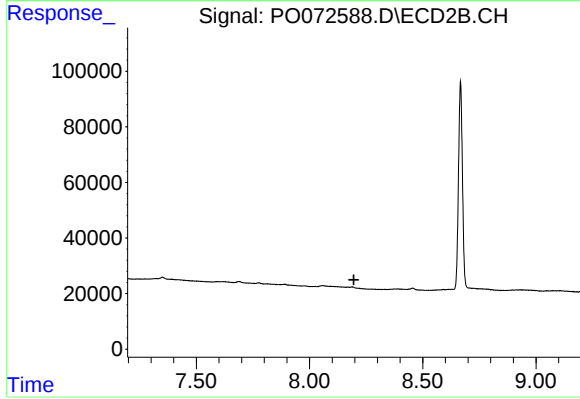

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 8.195 min
Response: 0
Conc: N.D.