

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102020\
 Data File : PO072563.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Oct 2020 22:49
 Operator : DD\AJ
 Sample : L4436-08
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 36A

Manual Integrations
 APPROVED

Ankita
 10/21/2020 5:15:18 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 04:49:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 14 17:47:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.319	3.502	1992353	975876	23.490	23.168
2) SA Decachlor...	9.922	8.668	2461000	1128109	22.311	21.822
Target Compounds						
26) L6 AR-1254-1	6.512	5.572	215790	72162	51.081	26.106 #
27) L6 AR-1254-2	6.740	5.734	240029	76781	37.036	31.581
28) L6 AR-1254-3	7.115	6.142	225826	132998	33.225m	34.562
29) L6 AR-1254-4	7.410	6.382	211388	69569	31.892	25.908
30) L6 AR-1254-5	7.830	6.804	438895	442294	68.516	120.690 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102020\
Data File : PO072563.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Oct 2020 22:49
Operator : DD\AJ
Sample : L4436-08
Misc :
ALS Vial : 40 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
36A


Manual Integrations
APPROVED

Ankita
10/21/2020 5:15:18 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 04:49:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 14 17:47:24 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

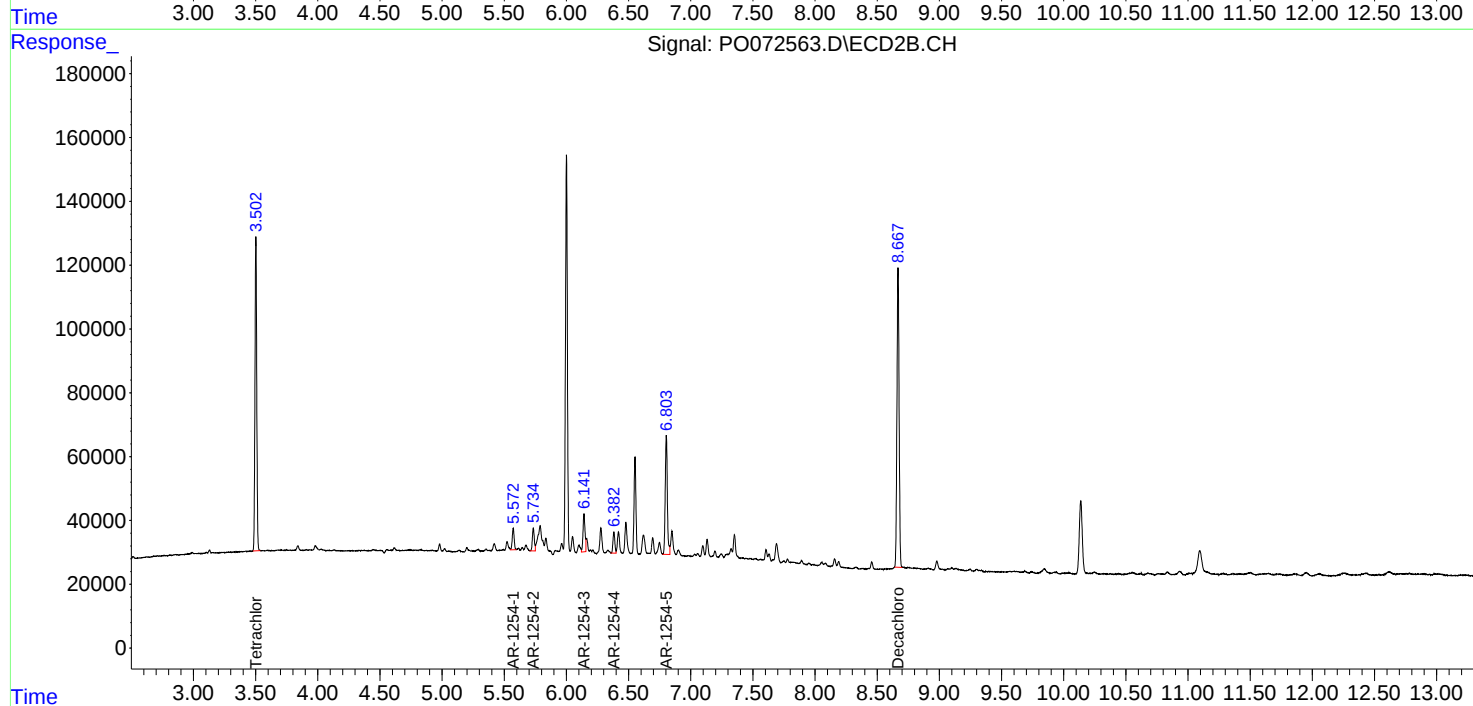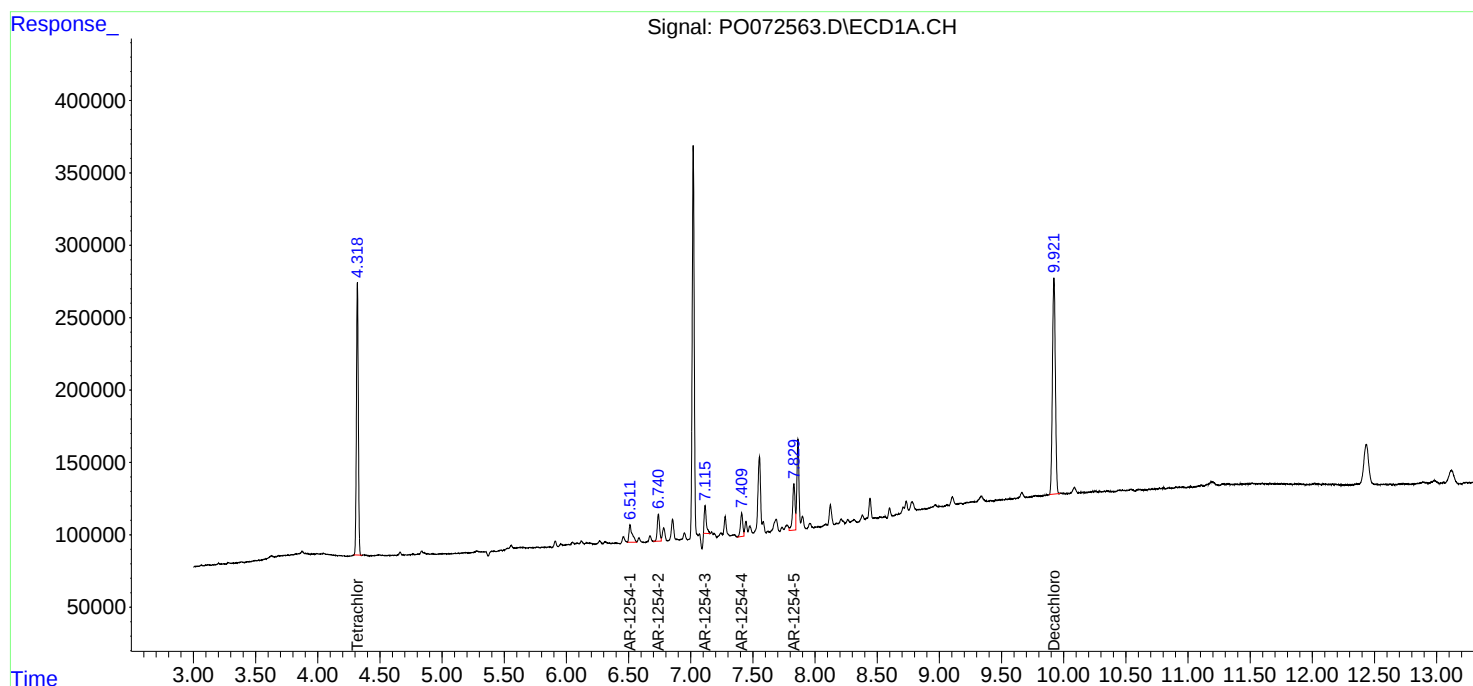

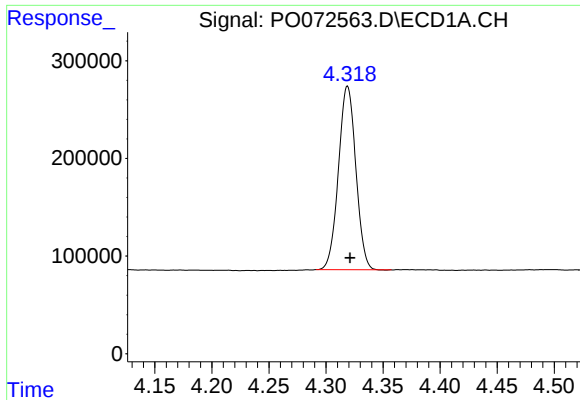


#1 Tetrachloro-m-xylene

R.T.: 4.319 min
Delta R.T.: -0.002 min
Response: 1992353
Conc: 23.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
36A


Manual Integrations
APPROVED

Ankita
10/21/2020 5:15:18 PM

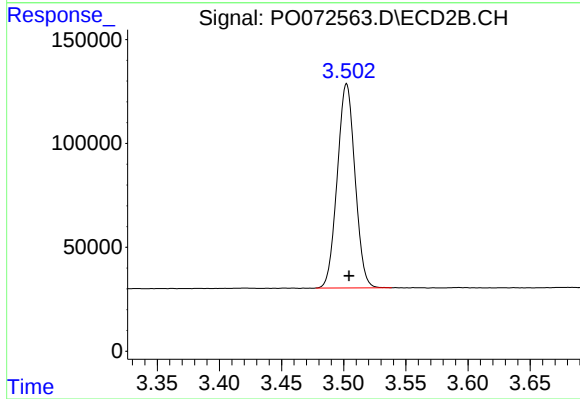


#1 Tetrachloro-m-xylene

R.T.: 3.502 min
Delta R.T.: -0.002 min
Response: 975876
Conc: 23.17 ng/ml

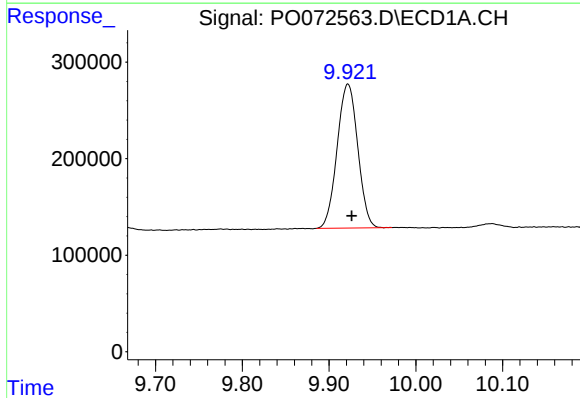


#2 Decachlorobiphenyl

R.T.: 9.922 min
Delta R.T.: -0.004 min
Response: 2461000
Conc: 22.31 ng/ml

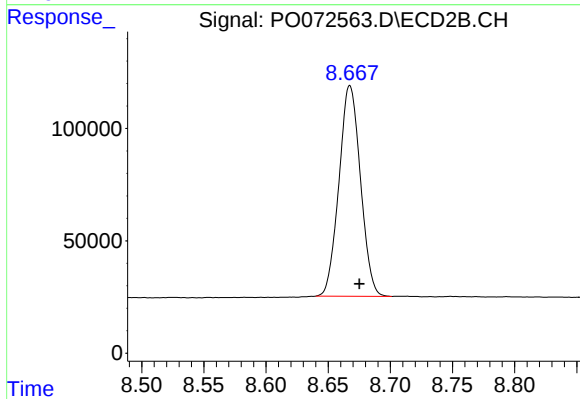

#2 Decachlorobiphenyl

R.T.: 8.668 min
Delta R.T.: -0.008 min
Response: 1128109
Conc: 21.82 ng/ml

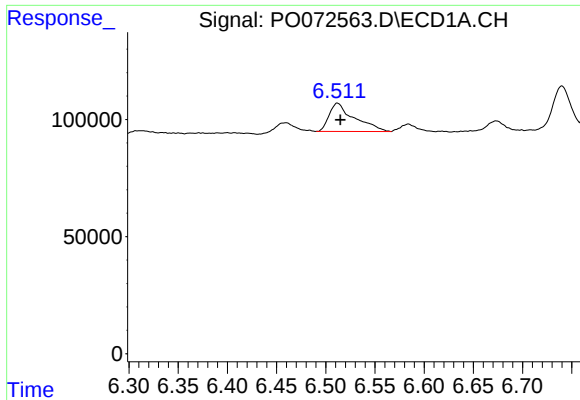


#26 AR-1254-1

R.T.: 6.512 min
Delta R.T.: -0.003 min
Response: 215790
Conc: 51.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
36A


Manual Integrations
APPROVED

Ankita
10/21/2020 5:15:18 PM

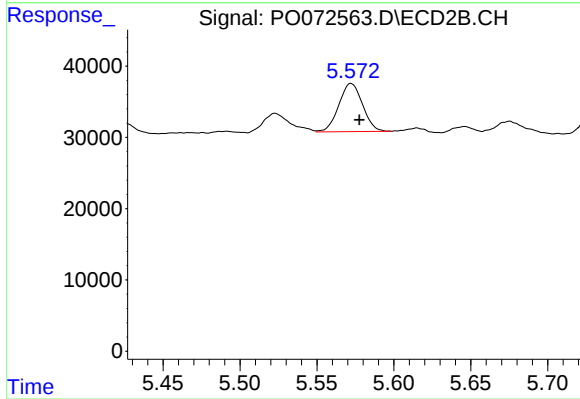


#26 AR-1254-1

R.T.: 5.572 min
Delta R.T.: -0.005 min
Response: 72162
Conc: 26.11 ng/ml

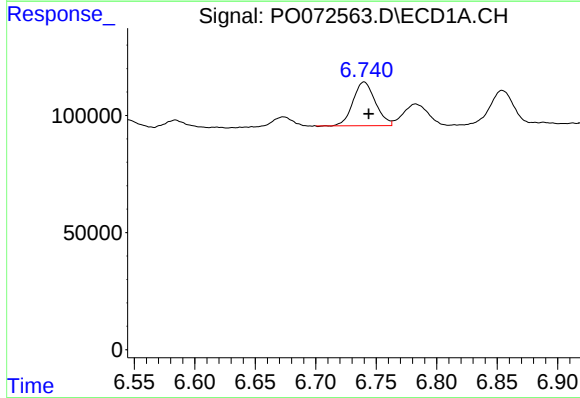


#27 AR-1254-2

R.T.: 6.740 min
Delta R.T.: -0.004 min
Response: 240029
Conc: 37.04 ng/ml

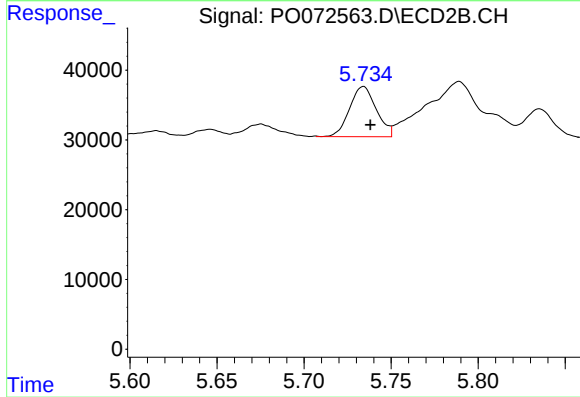

#27 AR-1254-2

R.T.: 5.734 min
Delta R.T.: -0.004 min
Response: 76781
Conc: 31.58 ng/ml

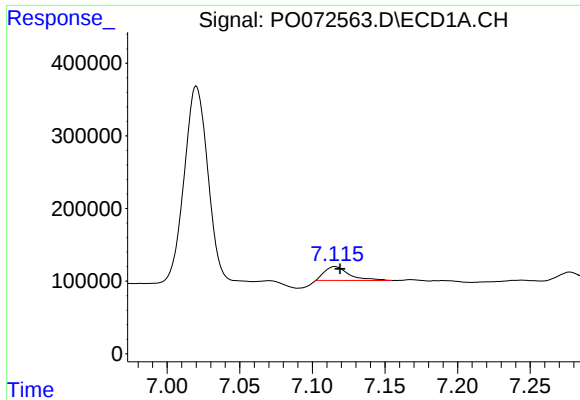


#28 AR-1254-3

R.T.: 7.115 min
Delta R.T.: -0.004 min
Response: 225826
Conc: 33.23 ng/ml m

Instrument :
ECD_O
ClientSampleId :
36A


Manual Integrations
APPROVED

Ankita
10/21/2020 5:15:18 PM

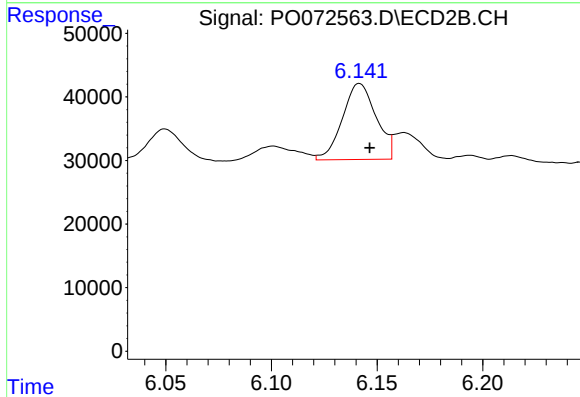


#28 AR-1254-3

R.T.: 6.142 min
Delta R.T.: -0.005 min
Response: 132998
Conc: 34.56 ng/ml

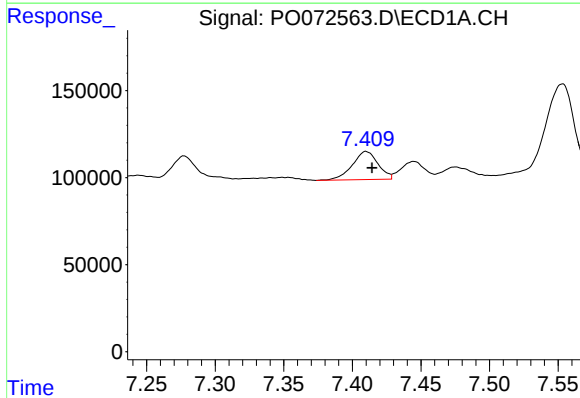


#29 AR-1254-4

R.T.: 7.410 min
Delta R.T.: -0.004 min
Response: 211388
Conc: 31.89 ng/ml

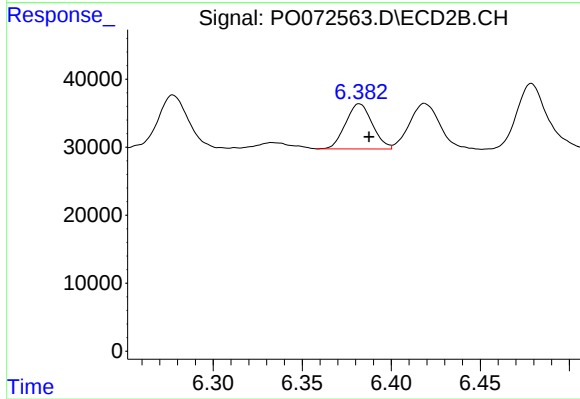

#29 AR-1254-4

R.T.: 6.382 min
Delta R.T.: -0.005 min
Response: 69569
Conc: 25.91 ng/ml

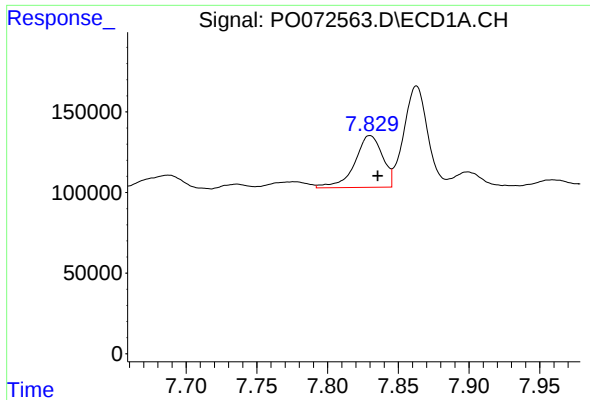


#30 AR-1254-5

R.T.: 7.830 min
Delta R.T.: -0.005 min
Response: 438895
Conc: 68.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
36A

Manual Integrations
APPROVED

Ankita
10/21/2020 5:15:18 PM

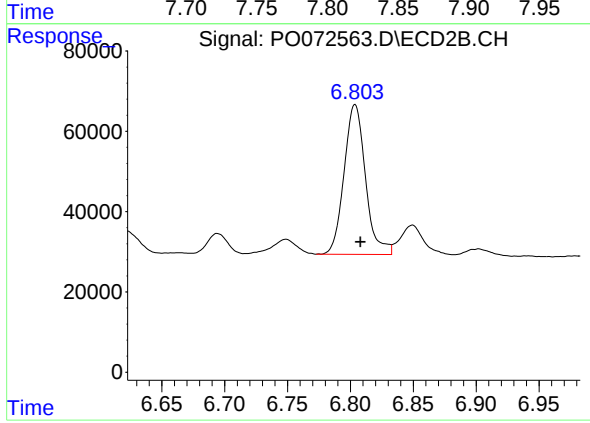

#30 AR-1254-5

R.T.: 6.804 min
Delta R.T.: -0.004 min
Response: 442294
Conc: 120.69 ng/ml