

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102020\
 Data File : PO072572.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Oct 2020 1:41
 Operator : DD\AJ
 Sample : L4473-04
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TT-021-IDW/GW-20201019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 04:56:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 14 17:47:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.320	3.504	1636916	801966	19.299	19.039
2) SA Decachlor...	9.920	8.667	1336718	632562	12.118	12.236

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102020\
Data File : P0072572.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Oct 2020 1:41
Operator : DD\AJ
Sample : L4473-04
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TT-021-IDWGW-20201019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 04:56:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 14 17:47:24 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

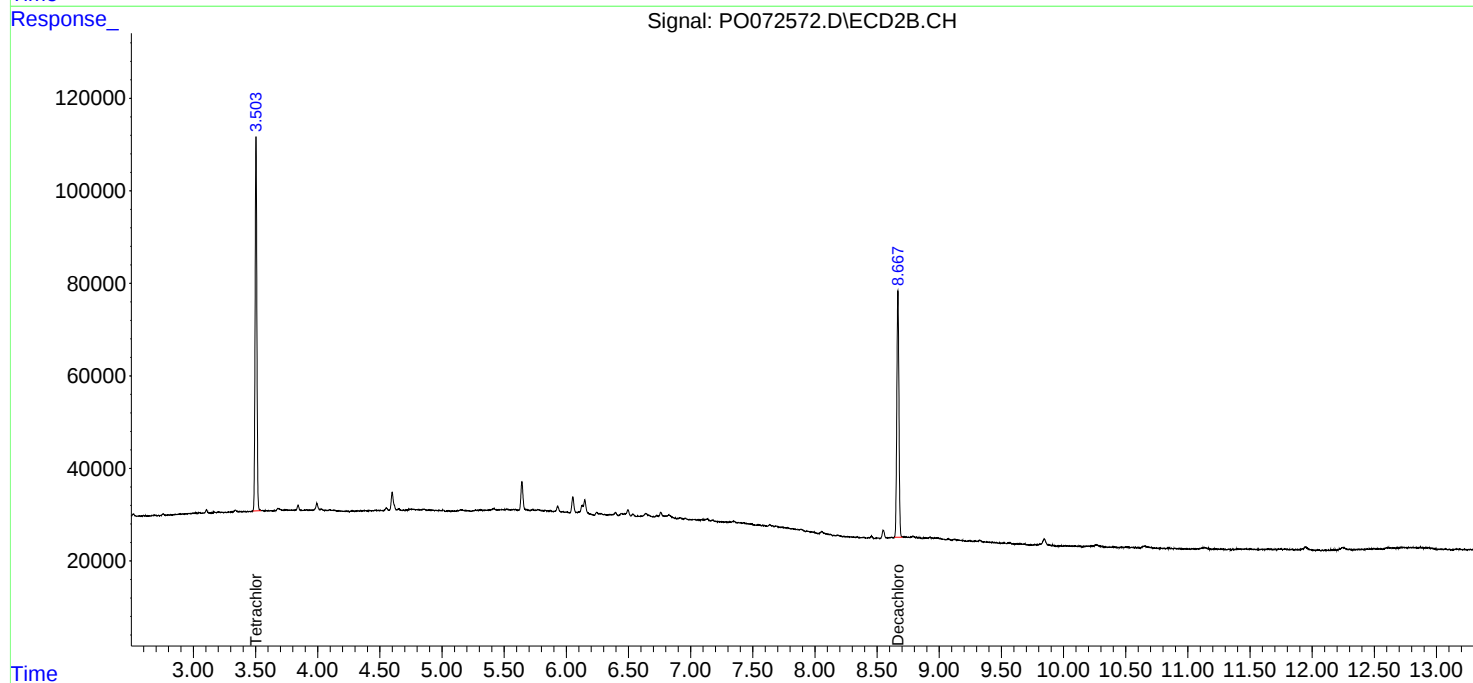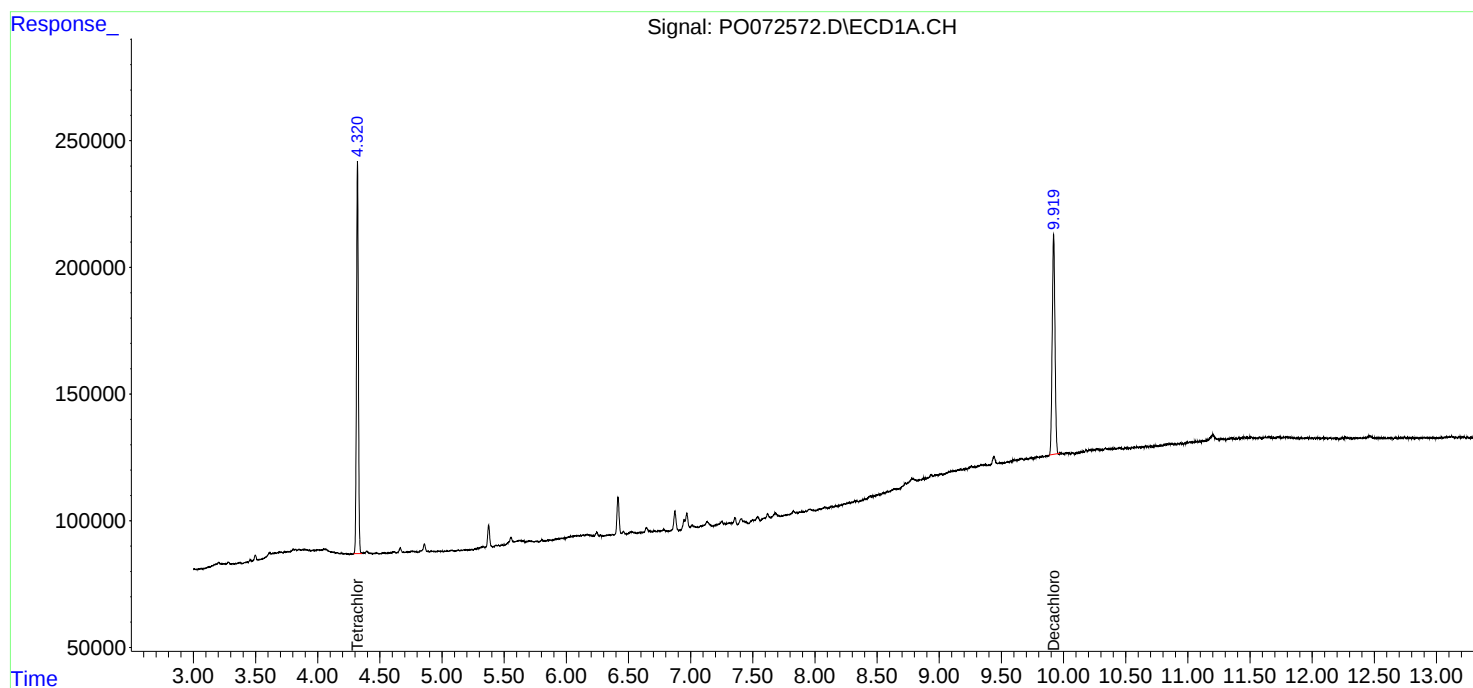


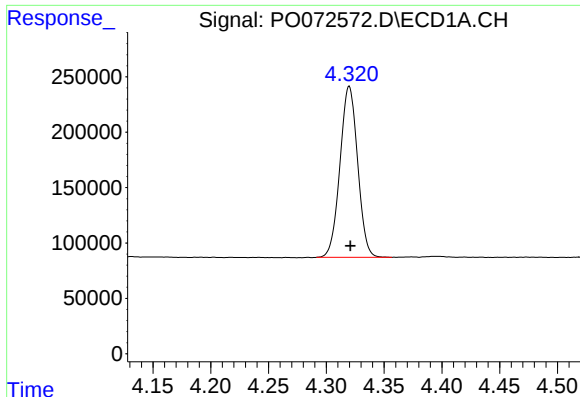

#1 Tetrachloro-m-xylene


R.T.: 4.320 min
Delta R.T.: -0.001 min
Response: 1636916
Conc: 19.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
TT-021-IDWGW-20201019

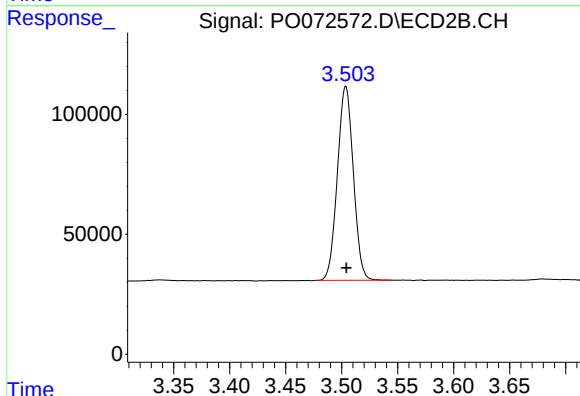


#1 Tetrachloro-m-xylene

R.T.: 3.504 min
Delta R.T.: 0.000 min
Response: 801966
Conc: 19.04 ng/ml

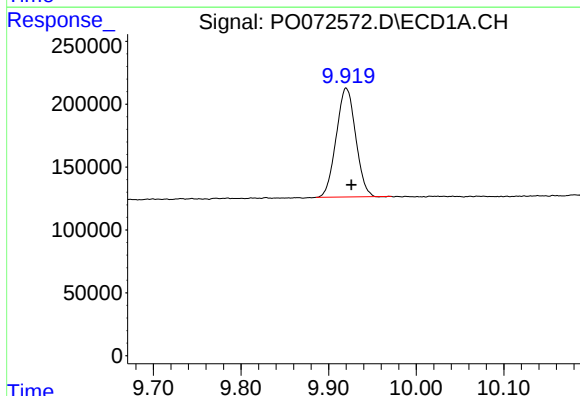

#2 Decachlorobiphenyl

R.T.: 9.920 min
Delta R.T.: -0.006 min
Response: 1336718
Conc: 12.12 ng/ml

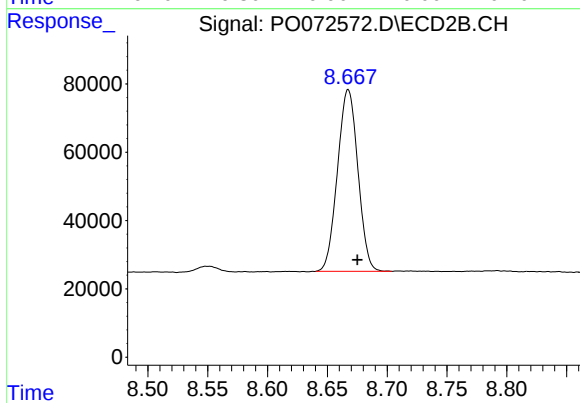

#2 Decachlorobiphenyl

R.T.: 8.667 min
Delta R.T.: -0.008 min
Response: 632562
Conc: 12.24 ng/ml