

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102020\
 Data File : PO072585.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Oct 2020 5:40
 Operator : DD\AJ
 Sample : L4222-01
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 EO-03-101920

Manual Integrations
 APPROVED

Ankita
 10/22/2020 5:29:10 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 06:28:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 14 17:47:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.320	3.504	1701877	878852	20.065m	20.864
2) SA Decachlor...	9.921	8.668	1925224	848433	17.454	16.412

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102020\
Data File : PO072585.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Oct 2020 5:40
Operator : DD\AJ
Sample : L4222-01
Misc :
ALS Vial : 56 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
EO-03-101920


Manual Integrations
APPROVED

Ankita
10/22/2020 5:29:10 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 06:28:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 14 17:47:24 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

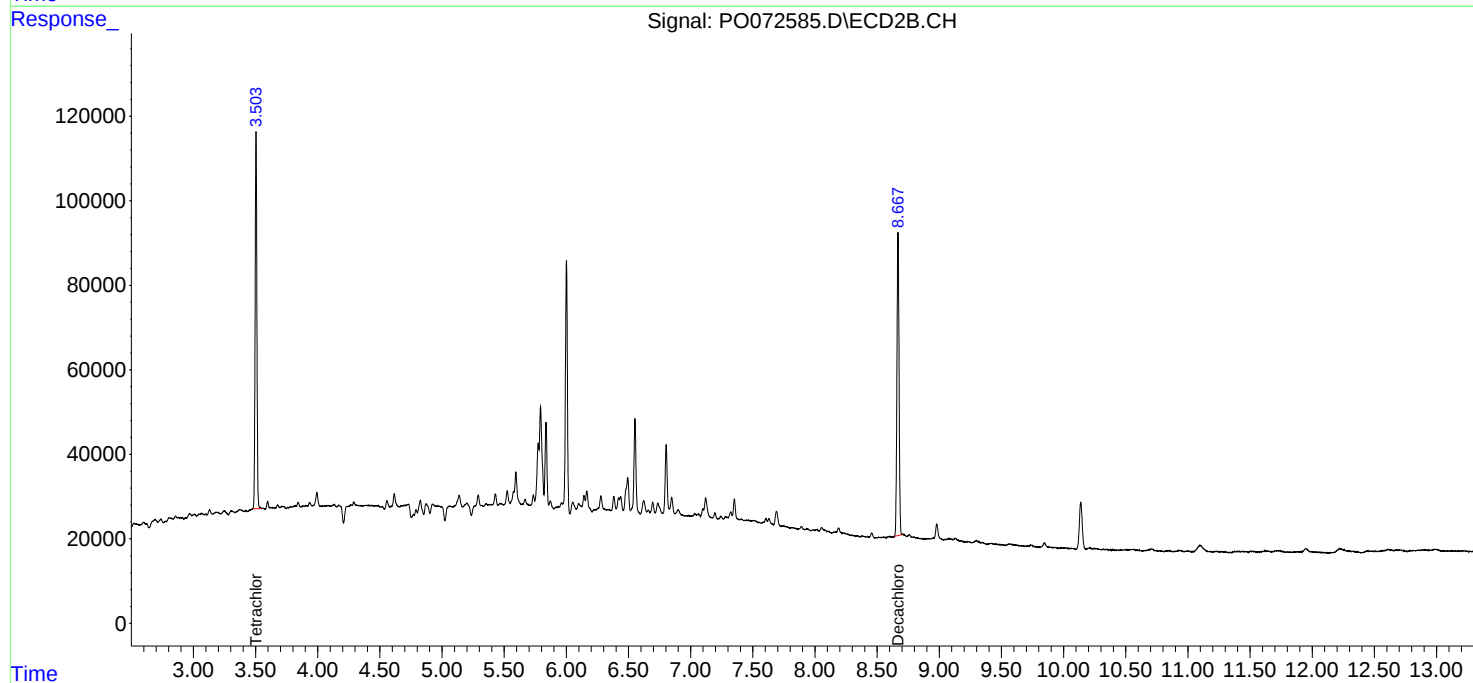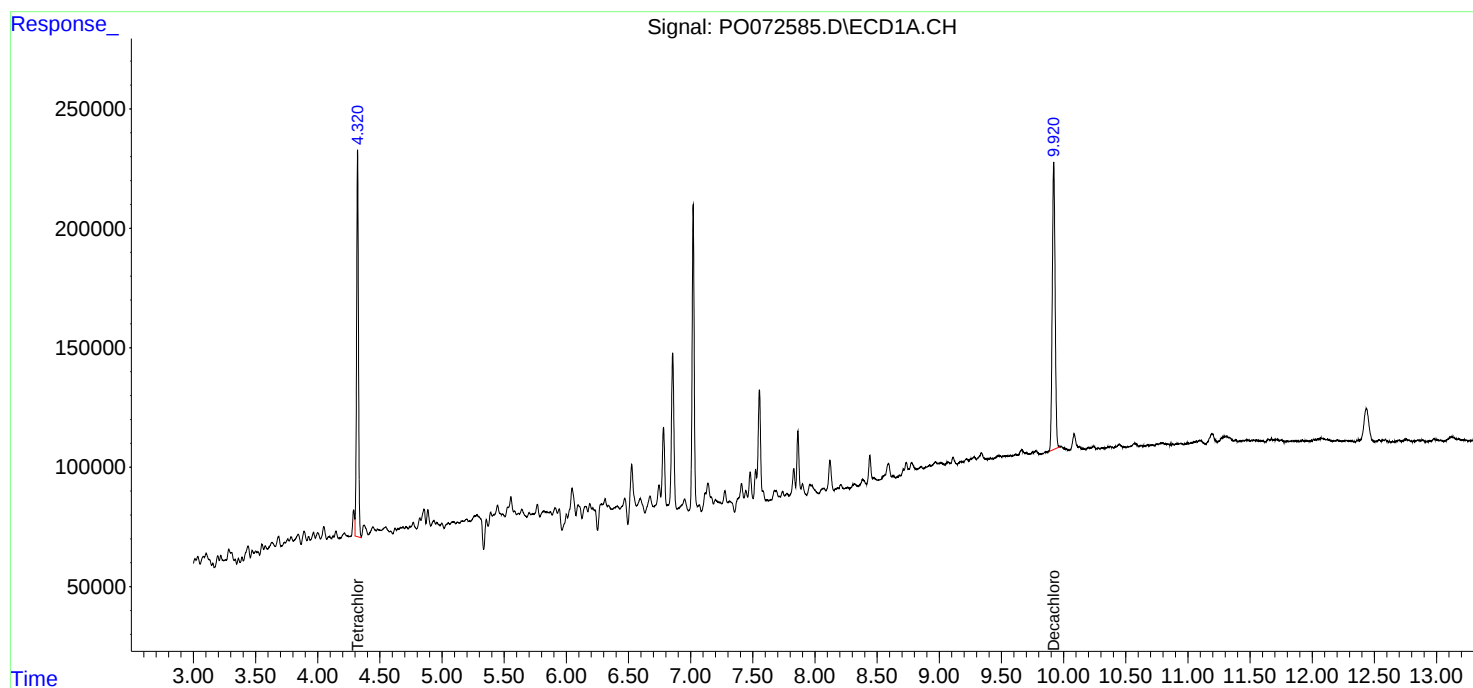

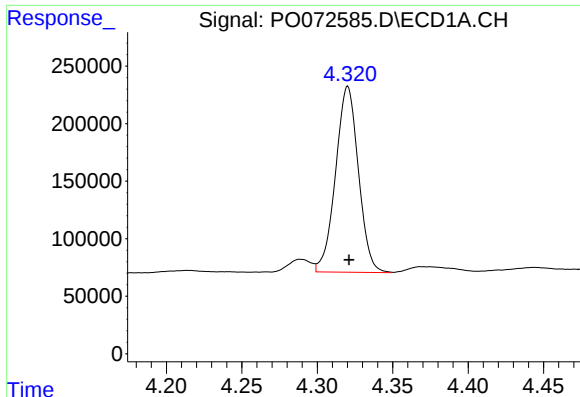


#1 Tetrachloro-m-xylene

R.T.: 4.320 min
Delta R.T.: -0.001 min
Response: 1701877
Conc: 20.06 ng/ml m

Instrument :
ECD_O
ClientSampleId :
EO-03-101920


Manual Integrations
APPROVED

Ankita
10/22/2020 5:29:10 PM

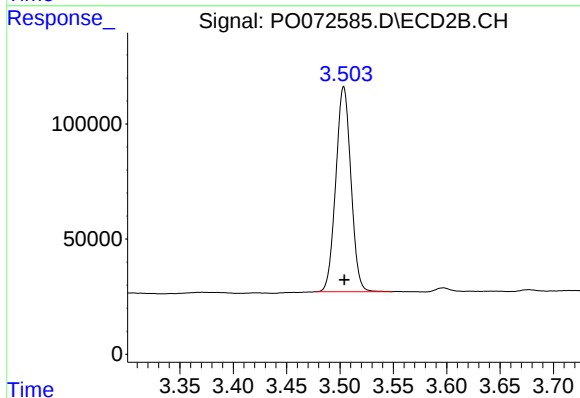


#1 Tetrachloro-m-xylene

R.T.: 3.504 min
Delta R.T.: 0.000 min
Response: 878852
Conc: 20.86 ng/ml

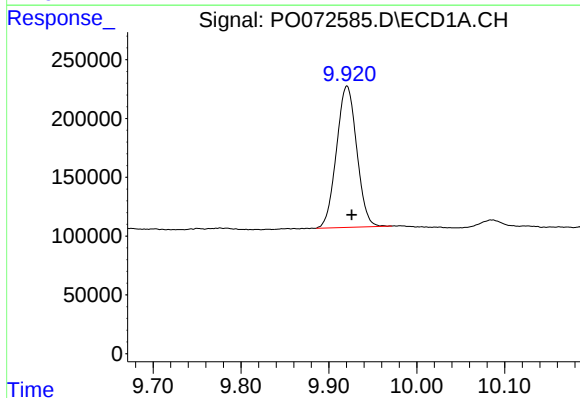

#2 Decachlorobiphenyl

R.T.: 9.921 min
Delta R.T.: -0.005 min
Response: 1925224
Conc: 17.45 ng/ml

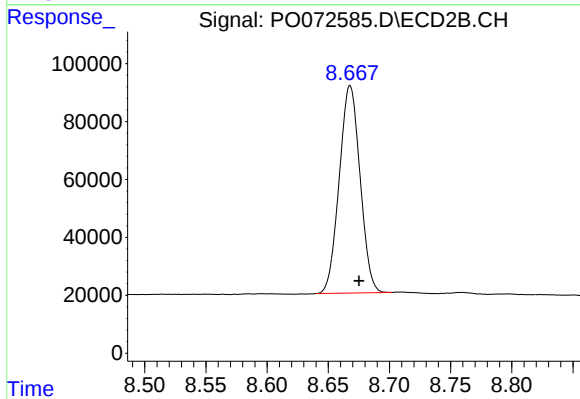

#2 Decachlorobiphenyl

R.T.: 8.668 min
Delta R.T.: -0.007 min
Response: 848433
Conc: 16.41 ng/ml