

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102119\
 Data File : P0063027.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Oct 2019 13:18
 Operator : HP/AJ
 Sample : PB124105BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB124105BL

Manual Integrations
 APPROVED

Ankita
 10/22/2019 9:23:01 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 14:25:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.327	3.477	1026661	756574	16.600	17.643
2)	SA Decachlor...	9.956	8.332	1296446	690635	23.170	23.538m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102119\
Data File : PO063027.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Oct 2019 13:18
Operator : HP/AJ
Sample : PB124105BL
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB124105BL


Manual Integrations
APPROVED

Ankita
10/22/2019 9:23:01 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 14:25:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

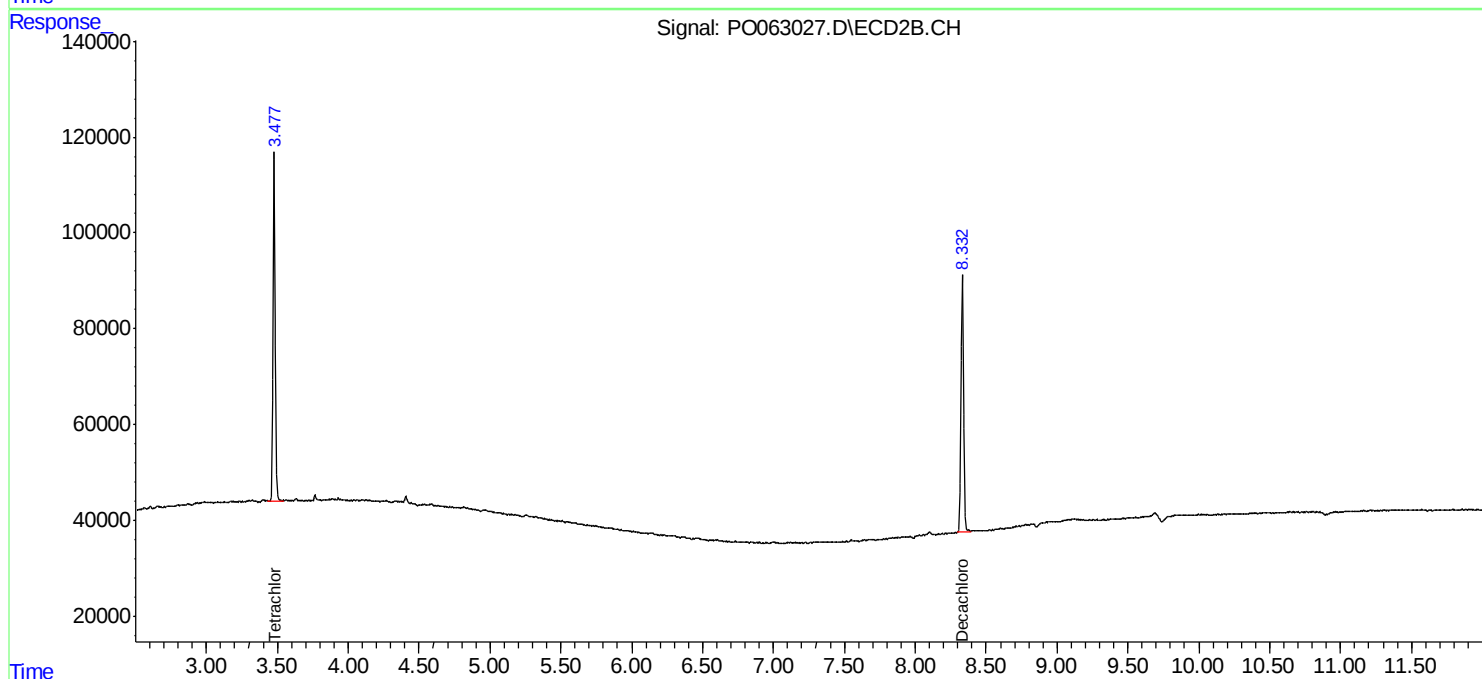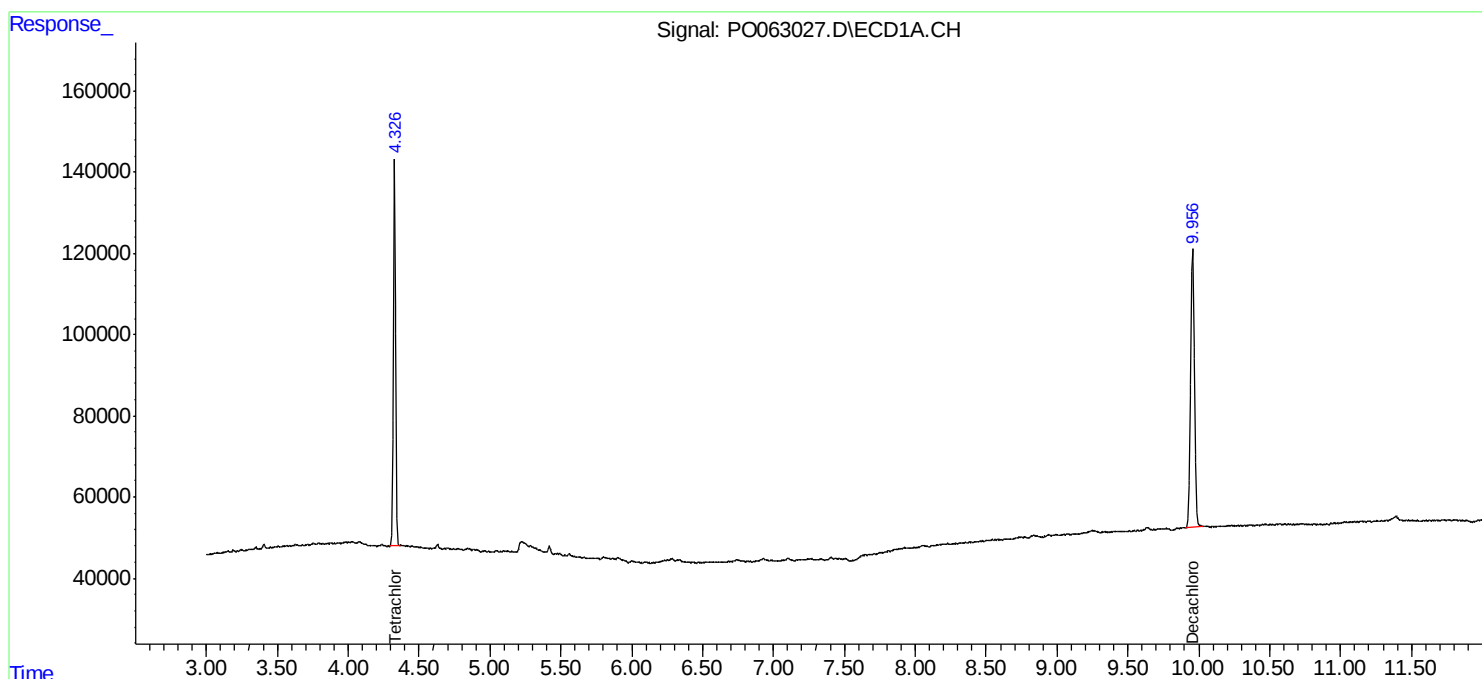

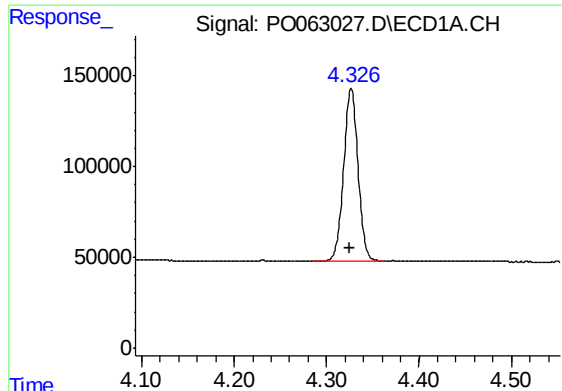


#1 Tetrachloro-m-xylene

R.T.: 4.327 min
Delta R.T.: 0.002 min
Response: 1026661
Conc: 16.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB124105BL


Manual Integrations
APPROVED

Ankita
10/22/2019 9:23:01 AM

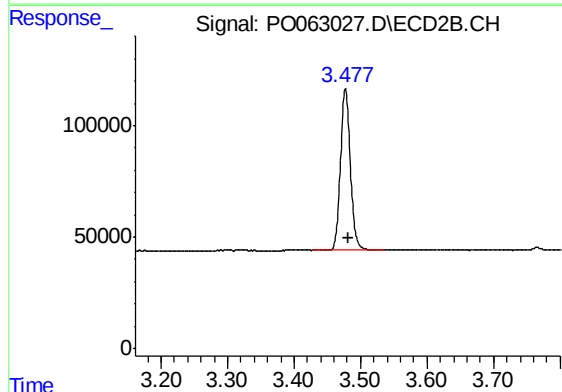


#1 Tetrachloro-m-xylene

R.T.: 3.477 min
Delta R.T.: -0.004 min
Response: 756574
Conc: 17.64 ng/ml

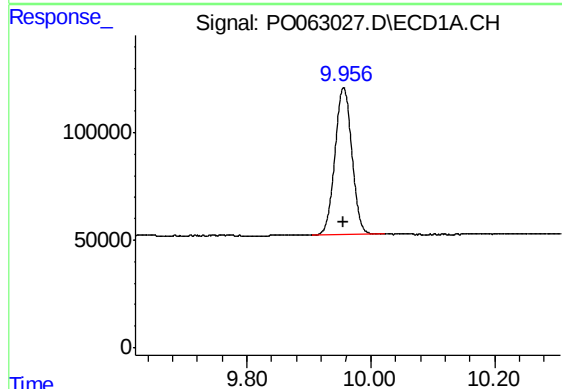

#2 Decachlorobiphenyl

R.T.: 9.956 min
Delta R.T.: 0.000 min
Response: 1296446
Conc: 23.17 ng/ml

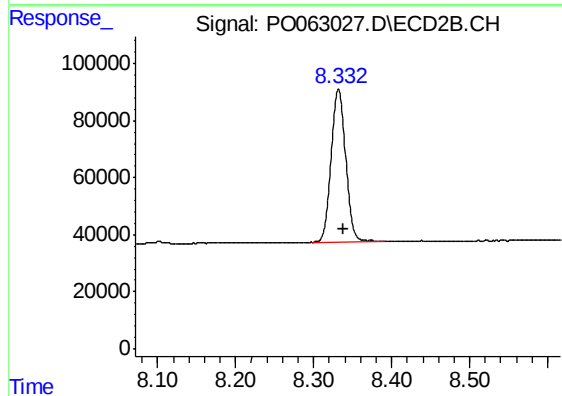

#2 Decachlorobiphenyl

R.T.: 8.332 min
Delta R.T.: -0.006 min
Response: 690635
Conc: 23.54 ng/ml m