

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102119\
 Data File : P0063033.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Oct 2019 15:29
 Operator : HP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Ankita
 10/22/2019 9:23:16 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 17:16:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.316	3.476	1244094	913270	20.116	21.297
2)	SA Decachlor...	9.939	8.326	1232621	677886	22.030m	23.103m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102119\
Data File : PO063033.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Oct 2019 15:29
Operator : HP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Ankita
10/22/2019 9:23:16 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 17:16:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

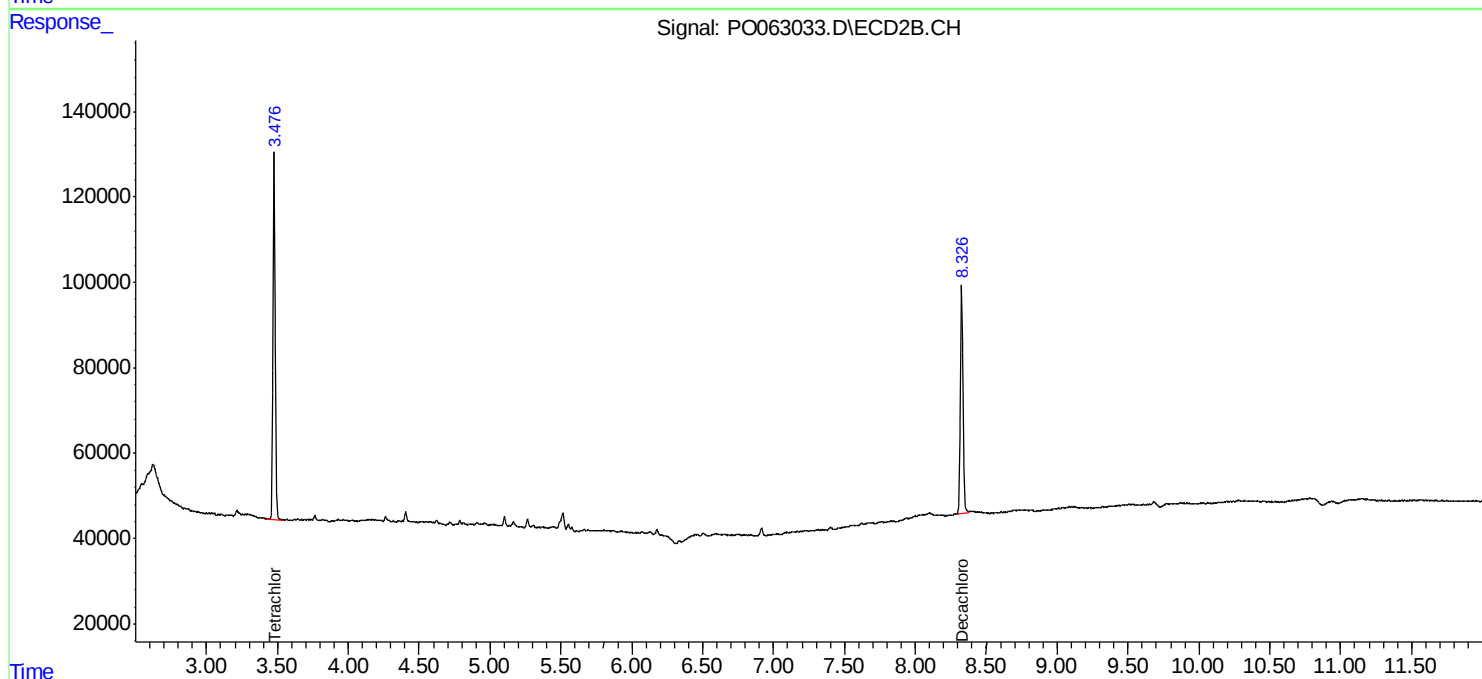

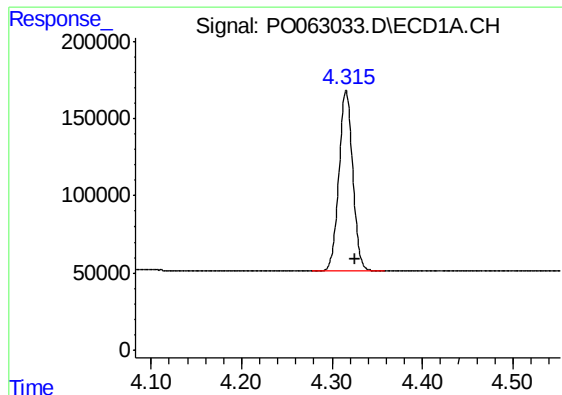


#1 Tetrachloro-m-xylene

R.T.: 4.316 min
Delta R.T.: -0.009 min
Response: 1244094
Conc: 20.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Ankita
10/22/2019 9:23:16 AM

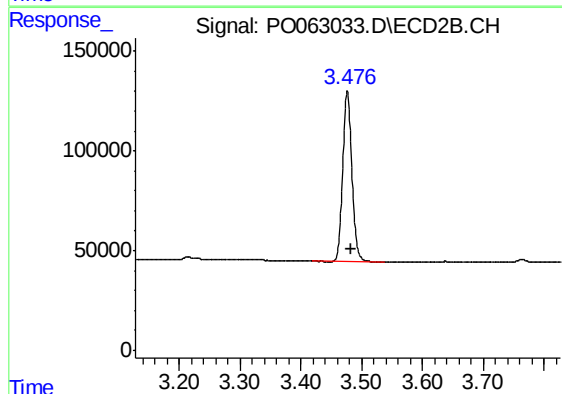


#1 Tetrachloro-m-xylene

R.T.: 3.476 min
Delta R.T.: -0.005 min
Response: 913270
Conc: 21.30 ng/ml

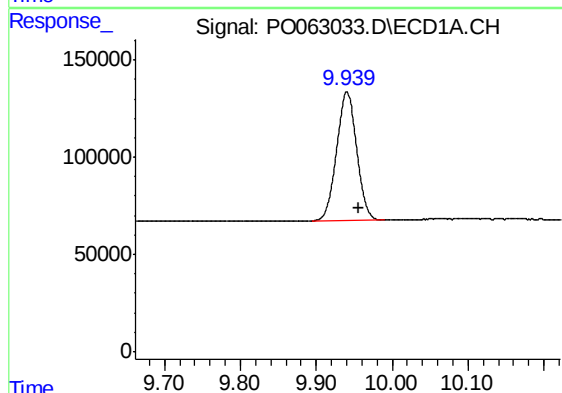

#2 Decachlorobiphenyl

R.T.: 9.939 min
Delta R.T.: -0.017 min
Response: 1232621
Conc: 22.03 ng/ml m

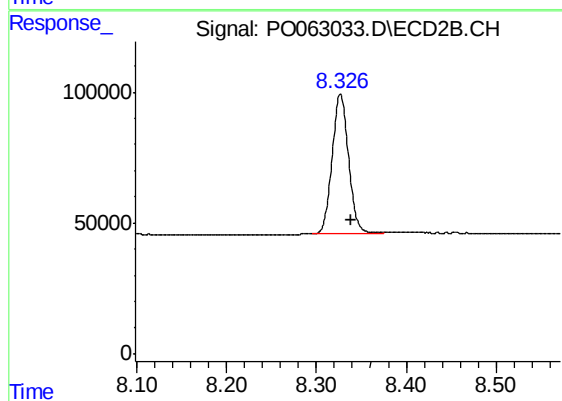

#2 Decachlorobiphenyl

R.T.: 8.326 min
Delta R.T.: -0.012 min
Response: 677886
Conc: 23.10 ng/ml m