

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102119\
 Data File : P0063037.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Oct 2019 16:35
 Operator : HP/AJ
 Sample : K5146-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CL-02-101819

Manual Integrations
 APPROVED

Ankita
 10/22/2019 9:23:35 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 00:57:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.315	3.477	1106760	833282	17.895m	19.432
2) SA Decachlor...	9.938	8.325	956979	490663	17.103m	16.723m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102119\
Data File : PO063037.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Oct 2019 16:35
Operator : HP/AJ
Sample : K5146-08
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CL-02-101819


Manual Integrations
APPROVED

Ankita
10/22/2019 9:23:35 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 00:57:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

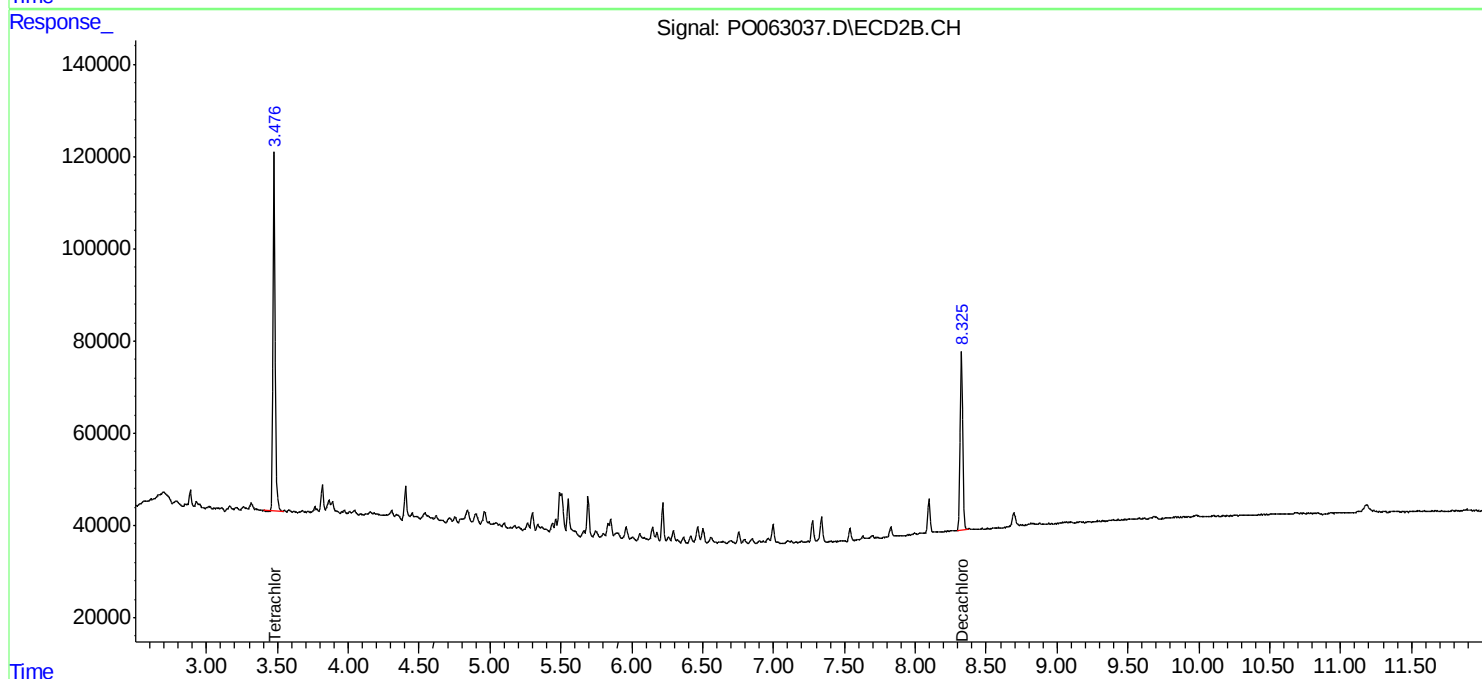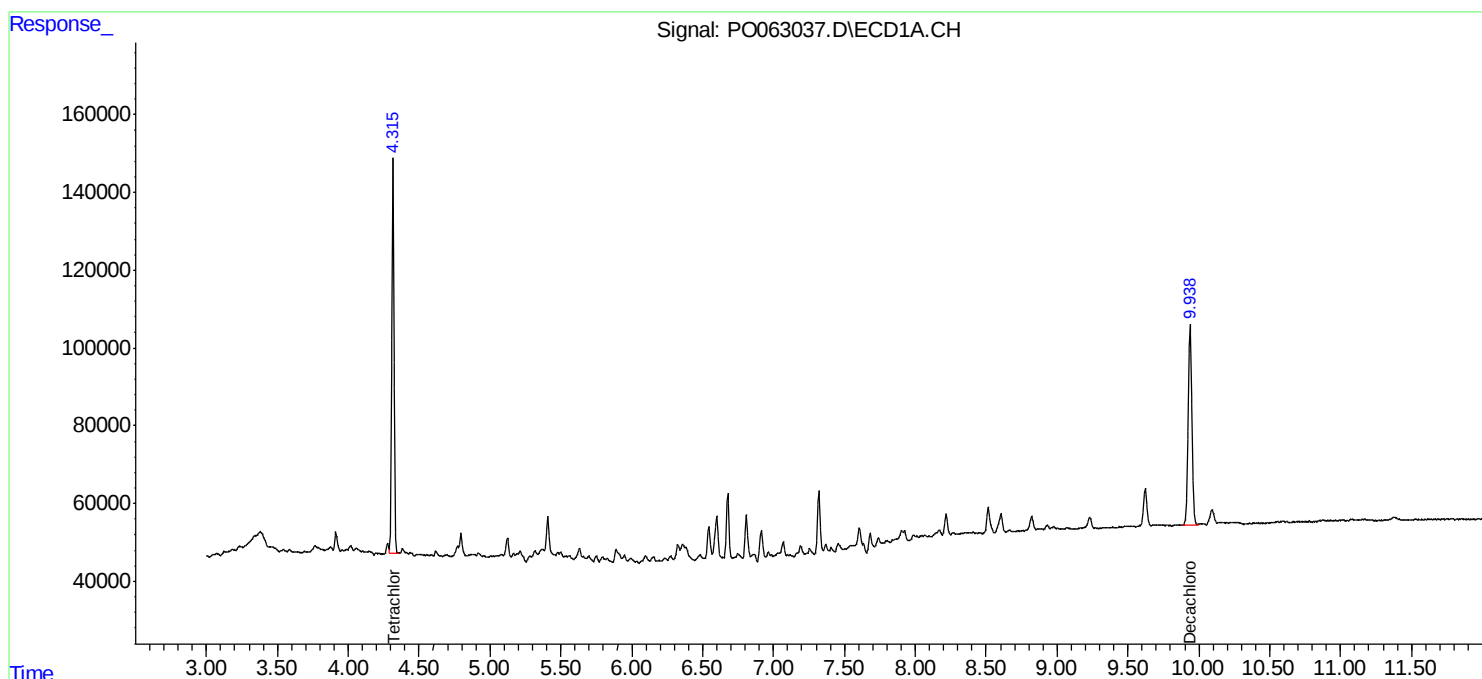

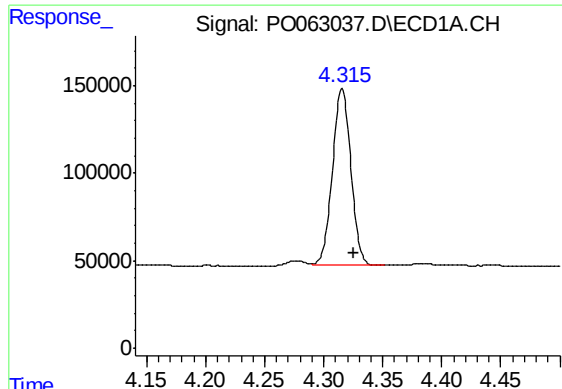


#1 Tetrachloro-m-xylene

R.T.: 4.315 min
Delta R.T.: -0.010 min
Response: 1106760
Conc: 17.90 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CL-02-101819


Manual Integrations
APPROVED

Ankita
10/22/2019 9:23:35 AM

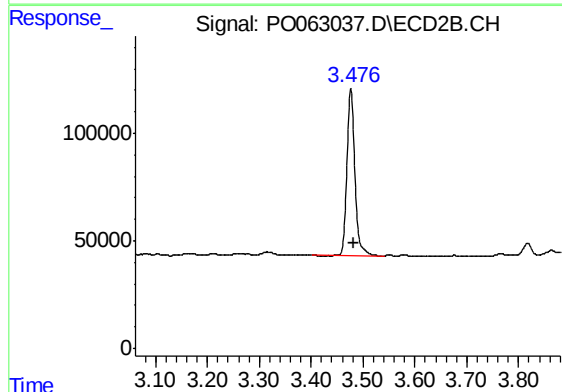


#1 Tetrachloro-m-xylene

R.T.: 3.477 min
Delta R.T.: -0.005 min
Response: 833282
Conc: 19.43 ng/ml

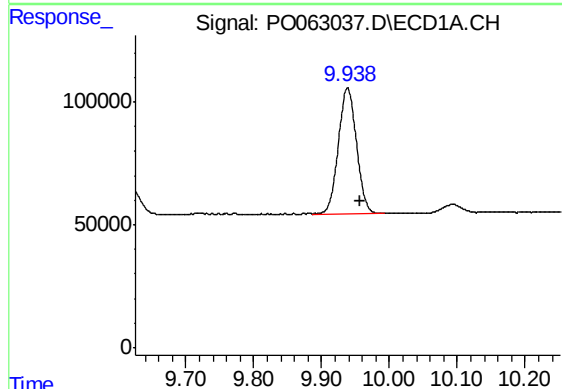

#2 Decachlorobiphenyl

R.T.: 9.938 min
Delta R.T.: -0.019 min
Response: 956979
Conc: 17.10 ng/ml m

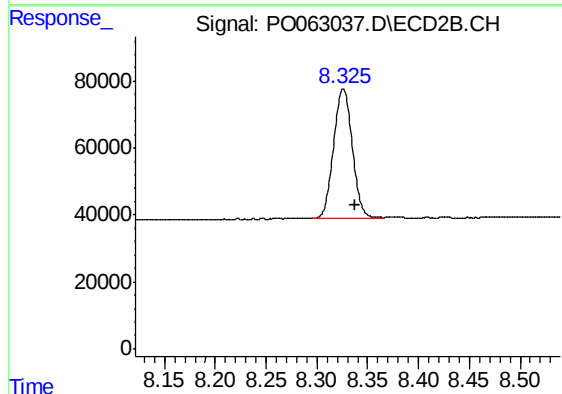

#2 Decachlorobiphenyl

R.T.: 8.325 min
Delta R.T.: -0.013 min
Response: 490663
Conc: 16.72 ng/ml m