

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102120\
 Data File : PO072602.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Oct 2020 12:20
 Operator : DD\AJ
 Sample : L4460-01 10X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CAPEMAY-ST-DRUM

Manual Integrations
 APPROVED

Ankita
 10/22/2020 12:12:11 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 14:11:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 14 17:47:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.318	3.503	210753	93180	2.485m	2.212
2) SA Decachlor...	9.928	8.677	157173	71954	1.425m	1.392

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102120\
Data File : PO072602.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Oct 2020 12:20
Operator : DD\AJ
Sample : L4460-01 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CAPEMAY-ST-DRUM


Manual Integrations
APPROVED

Ankita
10/22/2020 12:12:11 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 14:11:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 14 17:47:24 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

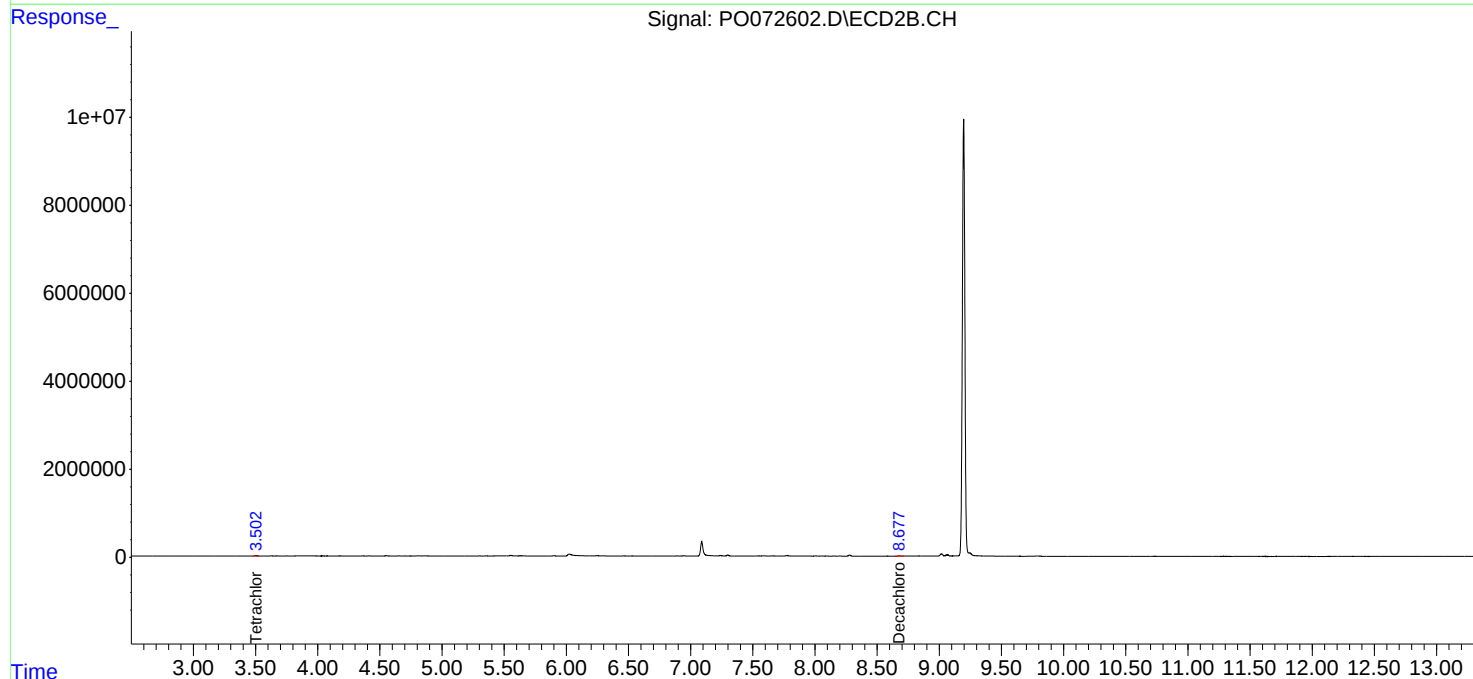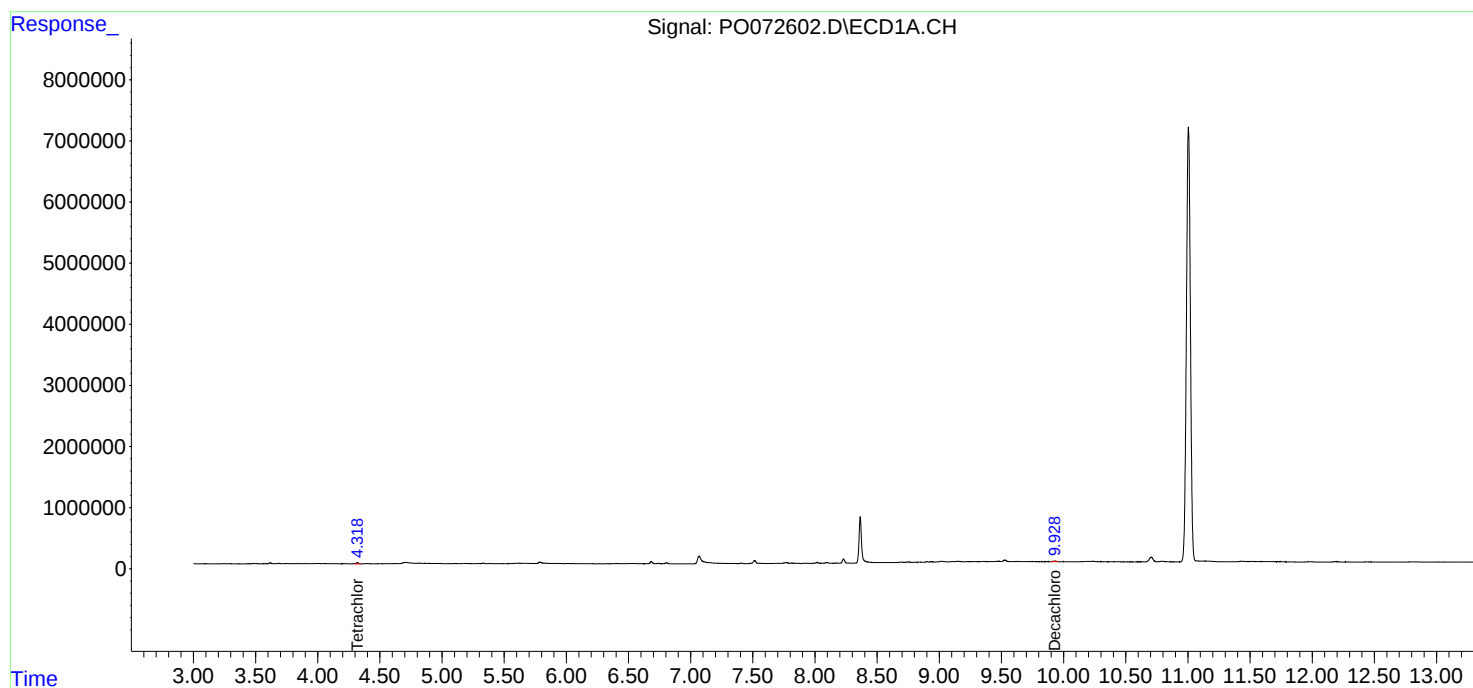

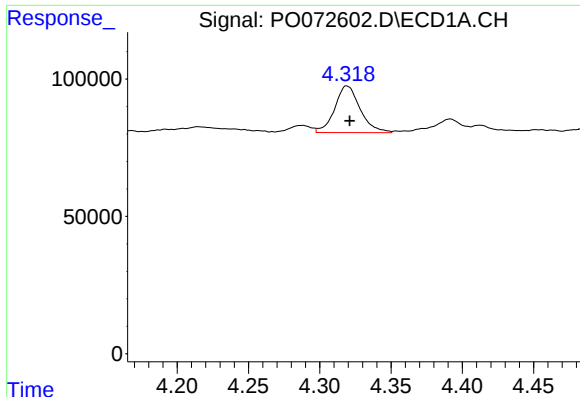


#1 Tetrachloro-m-xylene

R.T.: 4.318 min
Delta R.T.: -0.003 min
Response: 210753
Conc: 2.48 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CAPEMAY-ST-DRUM


Manual Integrations
APPROVED

Ankita
10/22/2020 12:12:11 PM

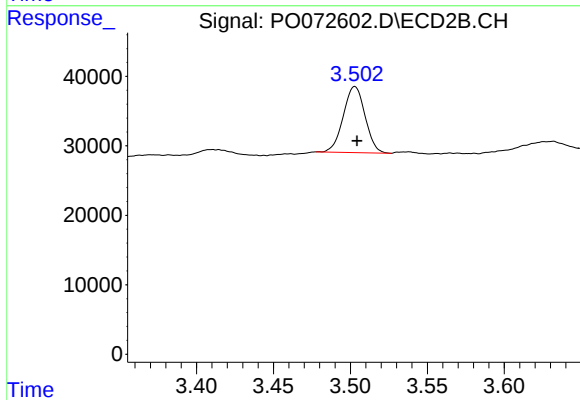


#1 Tetrachloro-m-xylene

R.T.: 3.503 min
Delta R.T.: -0.001 min
Response: 93180
Conc: 2.21 ng/ml

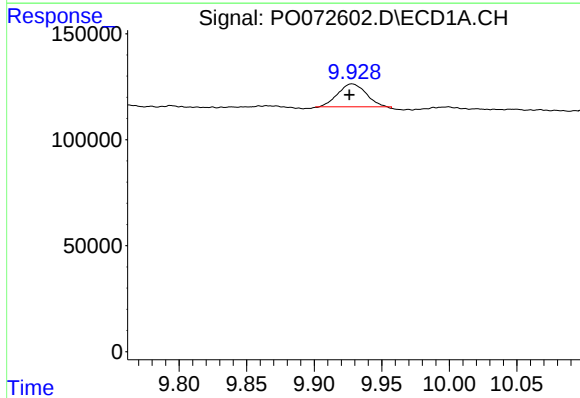

#2 Decachlorobiphenyl

R.T.: 9.928 min
Delta R.T.: 0.002 min
Response: 157173
Conc: 1.42 ng/ml m

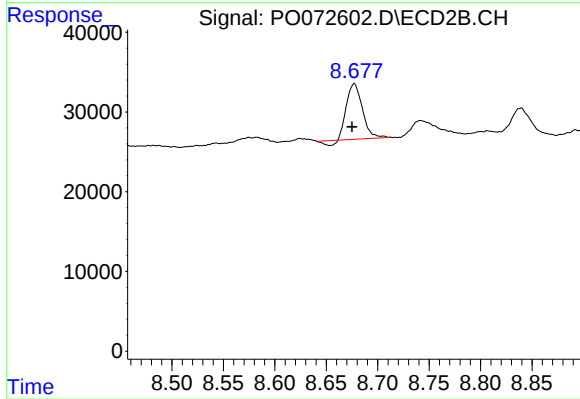

#2 Decachlorobiphenyl

R.T.: 8.677 min
Delta R.T.: 0.002 min
Response: 71954
Conc: 1.39 ng/ml