

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102120\
 Data File : PO072605.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Oct 2020 13:12
 Operator : DD\AJ
 Sample : L4457-01RE
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SUTTON-PR-2152-SEDRE

Manual Integrations
 APPROVED

Ankita
 10/22/2020 12:12:43 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 14:12:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 14 17:47:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.321	3.503	1320049	643566	15.563m	15.279
2) SA Decachlor...	9.921	8.667	883399	466018	8.009m	9.015

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102120\
Data File : PO072605.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Oct 2020 13:12
Operator : DD\AJ
Sample : L4457-01RE
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SUTTON-PR-2152-SEDRE


Manual Integrations
APPROVED

Ankita
10/22/2020 12:12:43 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 14:12:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 14 17:47:24 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

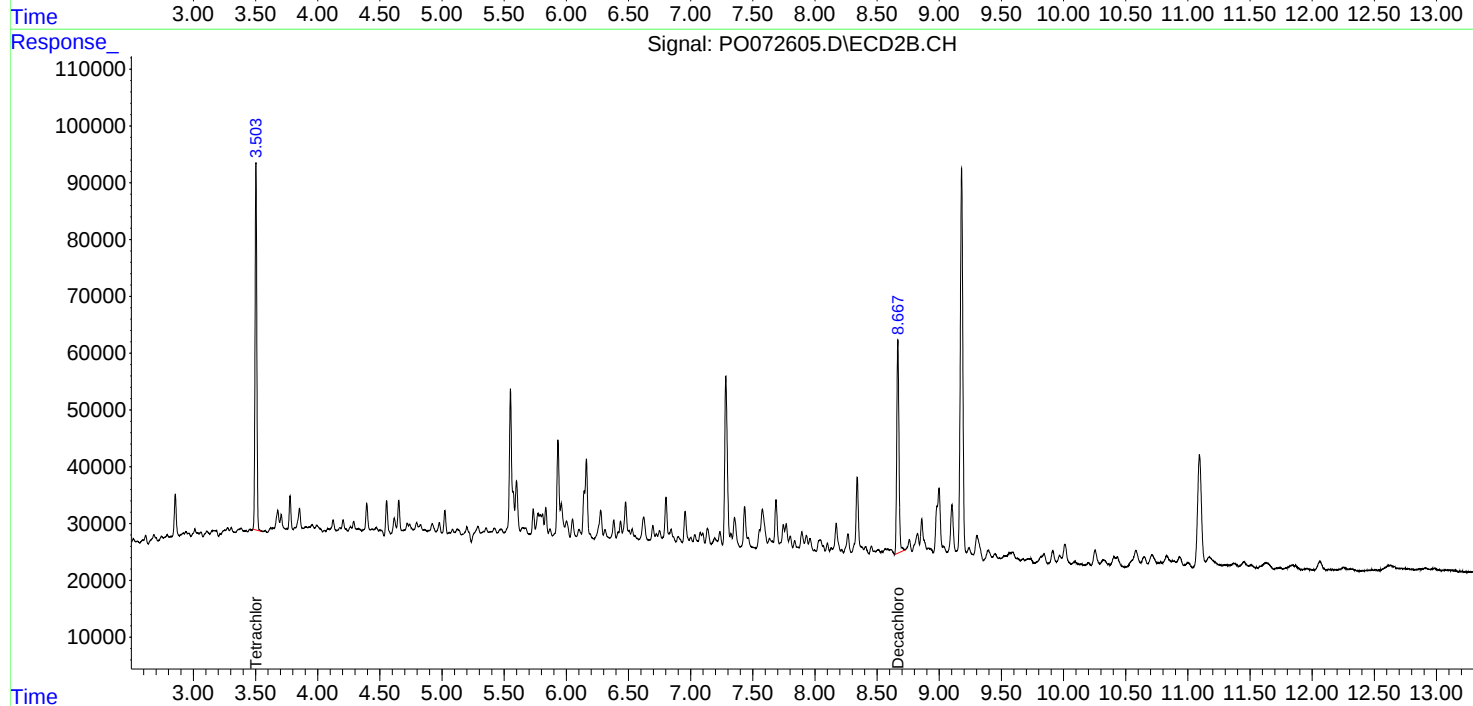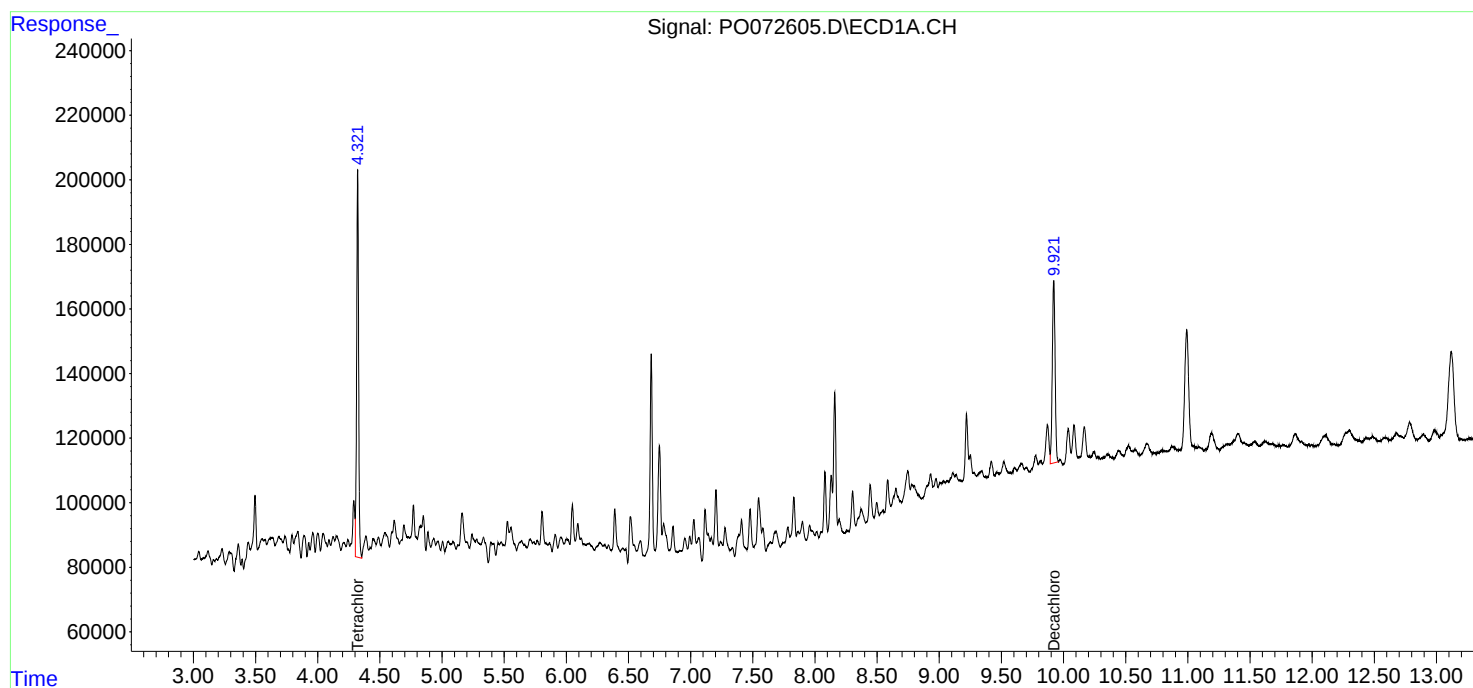

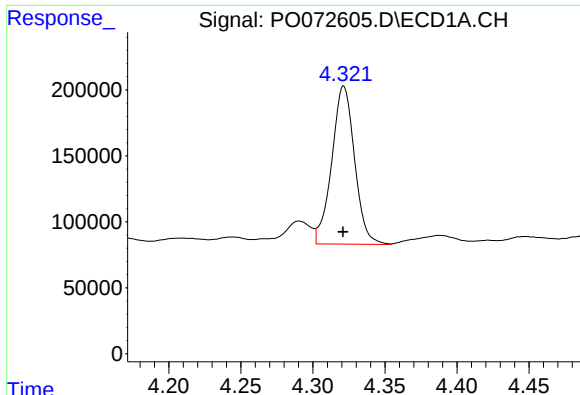


#1 Tetrachloro-m-xylene

R.T.: 4.321 min
Delta R.T.: 0.000 min
Response: 1320049
Conc: 15.56 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SUTTON-PR-2152-SEDRE


Manual Integrations
APPROVED

Ankita
10/22/2020 12:12:43 PM

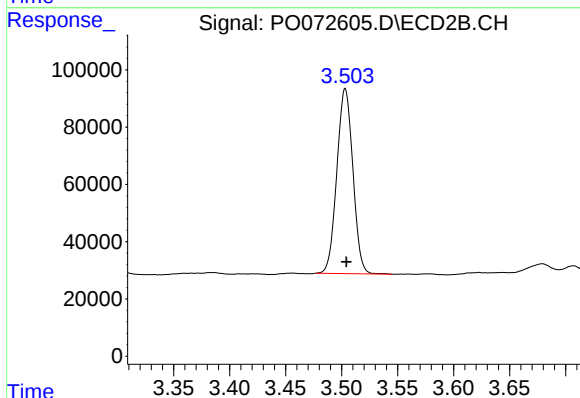


#1 Tetrachloro-m-xylene

R.T.: 3.503 min
Delta R.T.: 0.000 min
Response: 643566
Conc: 15.28 ng/ml

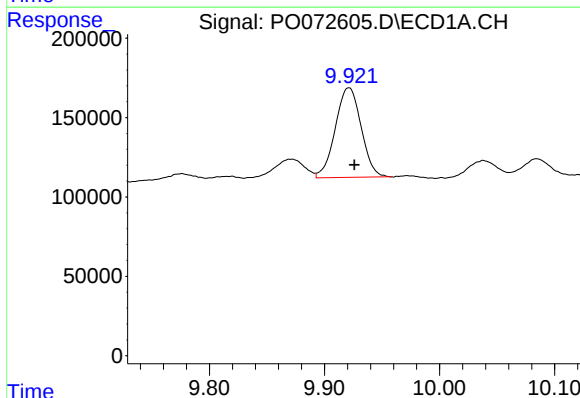

#2 Decachlorobiphenyl

R.T.: 9.921 min
Delta R.T.: -0.005 min
Response: 883399
Conc: 8.01 ng/ml m

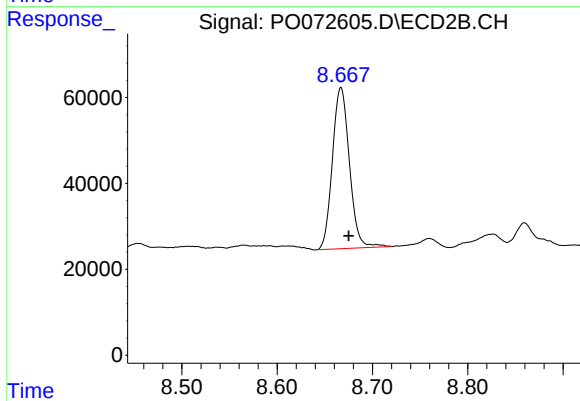

#2 Decachlorobiphenyl

R.T.: 8.667 min
Delta R.T.: -0.008 min
Response: 466018
Conc: 9.01 ng/ml