

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102120\
 Data File : P0072606.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Oct 2020 13:29
 Operator : DD\AJ
 Sample : L4455-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HP-627

Manual Integrations
 APPROVED

Ankita
 10/22/2020 12:12:44 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 14:13:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 14 17:47:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.320	3.504	2273196	1085191	26.801	25.763m
2) SA Decachlor...	9.923	8.669	2196315	936433	19.911	18.115

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102120\
Data File : PO072606.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Oct 2020 13:29
Operator : DD\AJ
Sample : L4455-03
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HP-627


Manual Integrations
APPROVED

Ankita
10/22/2020 12:12:44 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 14:13:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 14 17:47:24 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

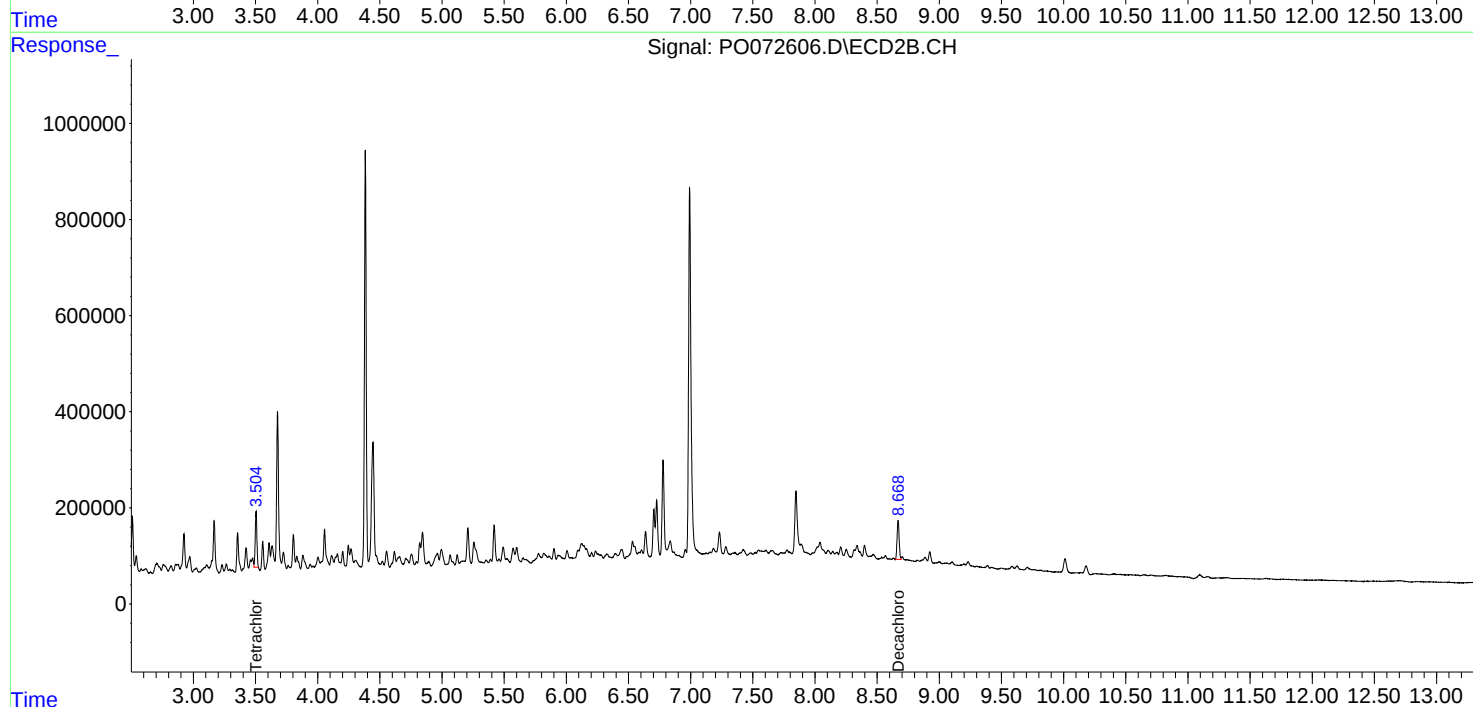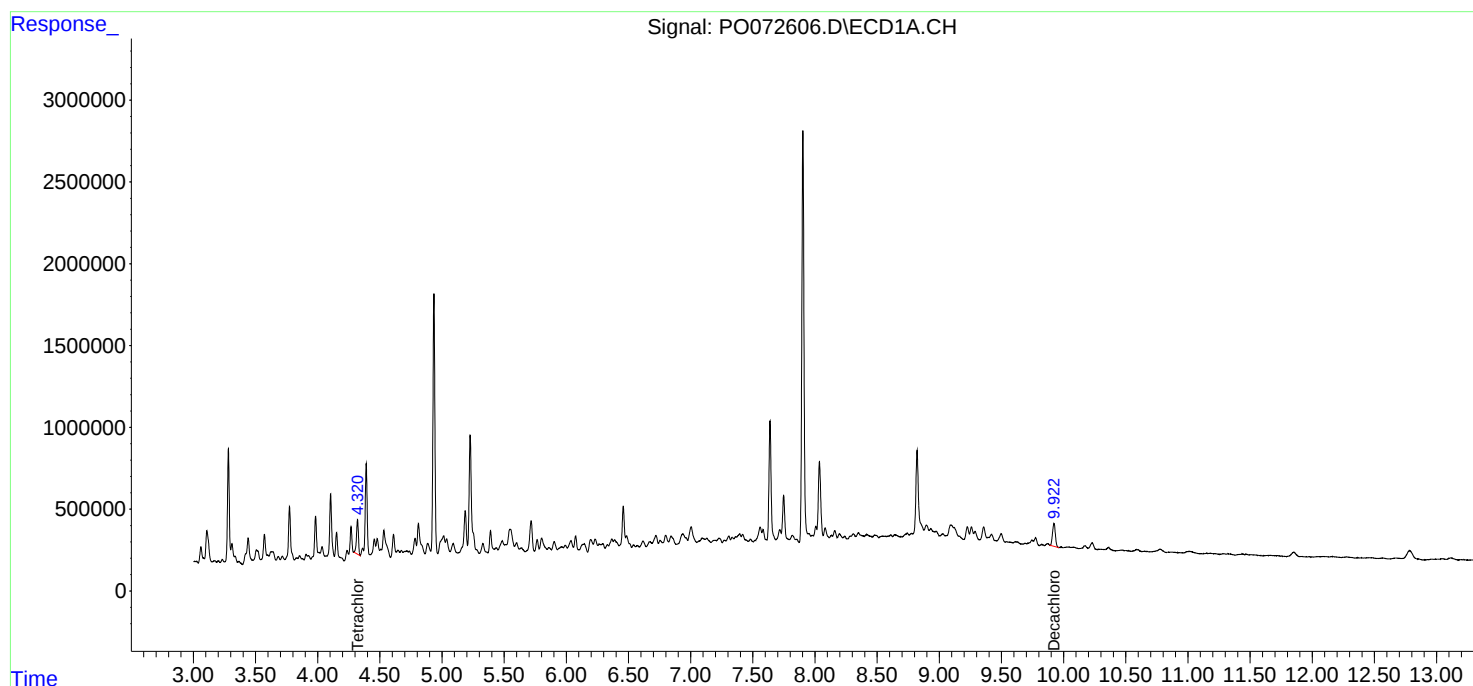

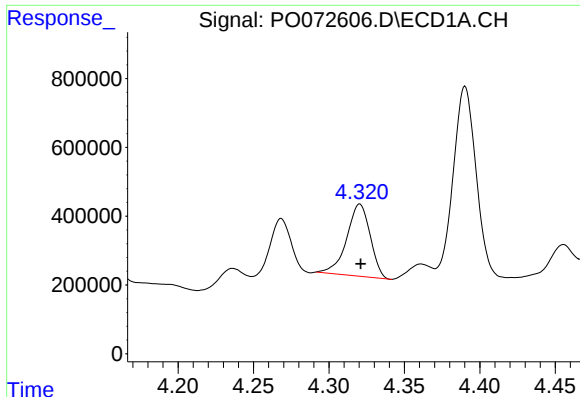


#1 Tetrachloro-m-xylene

R.T.: 4.320 min
Delta R.T.: 0.000 min
Response: 2273196
Conc: 26.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
HP-627


Manual Integrations
APPROVED

Ankita
10/22/2020 12:12:44 PM

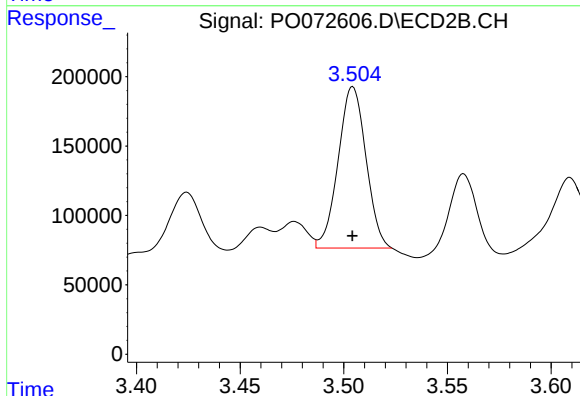


#1 Tetrachloro-m-xylene

R.T.: 3.504 min
Delta R.T.: 0.000 min
Response: 1085191
Conc: 25.76 ng/ml m

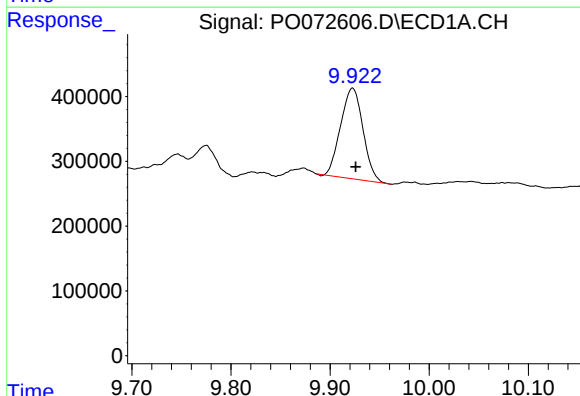

#2 Decachlorobiphenyl

R.T.: 9.923 min
Delta R.T.: -0.003 min
Response: 2196315
Conc: 19.91 ng/ml

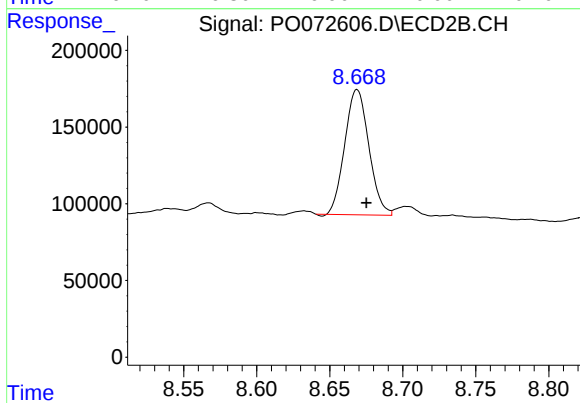

#2 Decachlorobiphenyl

R.T.: 8.669 min
Delta R.T.: -0.006 min
Response: 936433
Conc: 18.11 ng/ml