

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\PO102120\  
 Data File : PO072607.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 21 Oct 2020 13:46  
 Operator : DD\AJ  
 Sample : L4456-03  
 Misc :  
 ALS Vial : 18 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 HP-640

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Oct 21 14:13:33 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\PO101420.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Oct 14 17:47:24 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1  | RT#2  | Resp#1  | Resp#2  | ng/ml  | ng/ml  |
|-----------------------------|-------|-------|---------|---------|--------|--------|
| -----                       |       |       |         |         |        |        |
| System Monitoring Compounds |       |       |         |         |        |        |
| 1) SA Tetrachlo...          | 4.319 | 3.502 | 2160523 | 1048026 | 25.472 | 24.881 |
| 2) SA Decachlor...          | 9.918 | 8.667 | 1565871 | 695204  | 14.196 | 13.448 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\PO102120\  
Data File : PO072607.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 13:46  
Operator : DD\AJ  
Sample : L4456-03  
Misc :  
ALS Vial : 18 Sample Multiplier: 1

Instrument :  
ECD\_O  
ClientSampleId :  
HP-640

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Oct 21 14:13:33 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\PO101420.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Wed Oct 14 17:47:24 2020  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

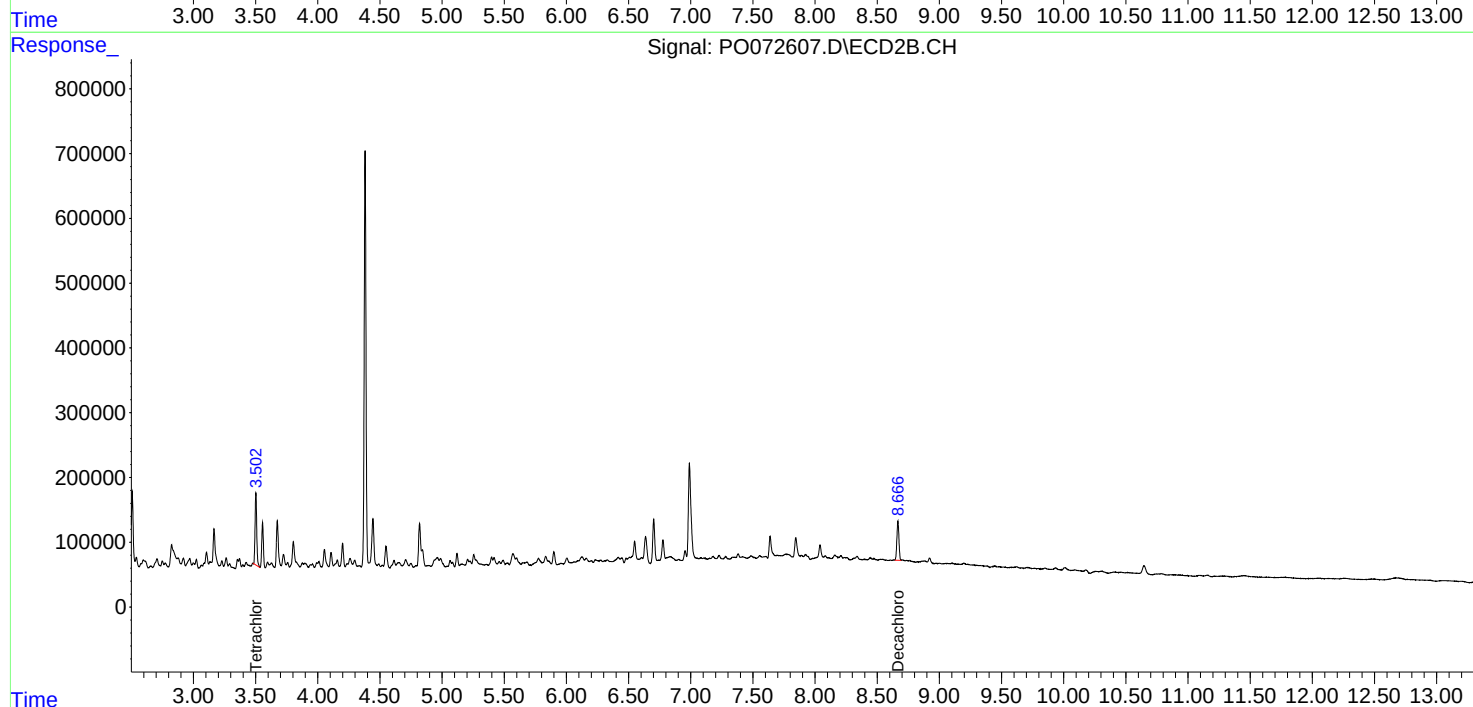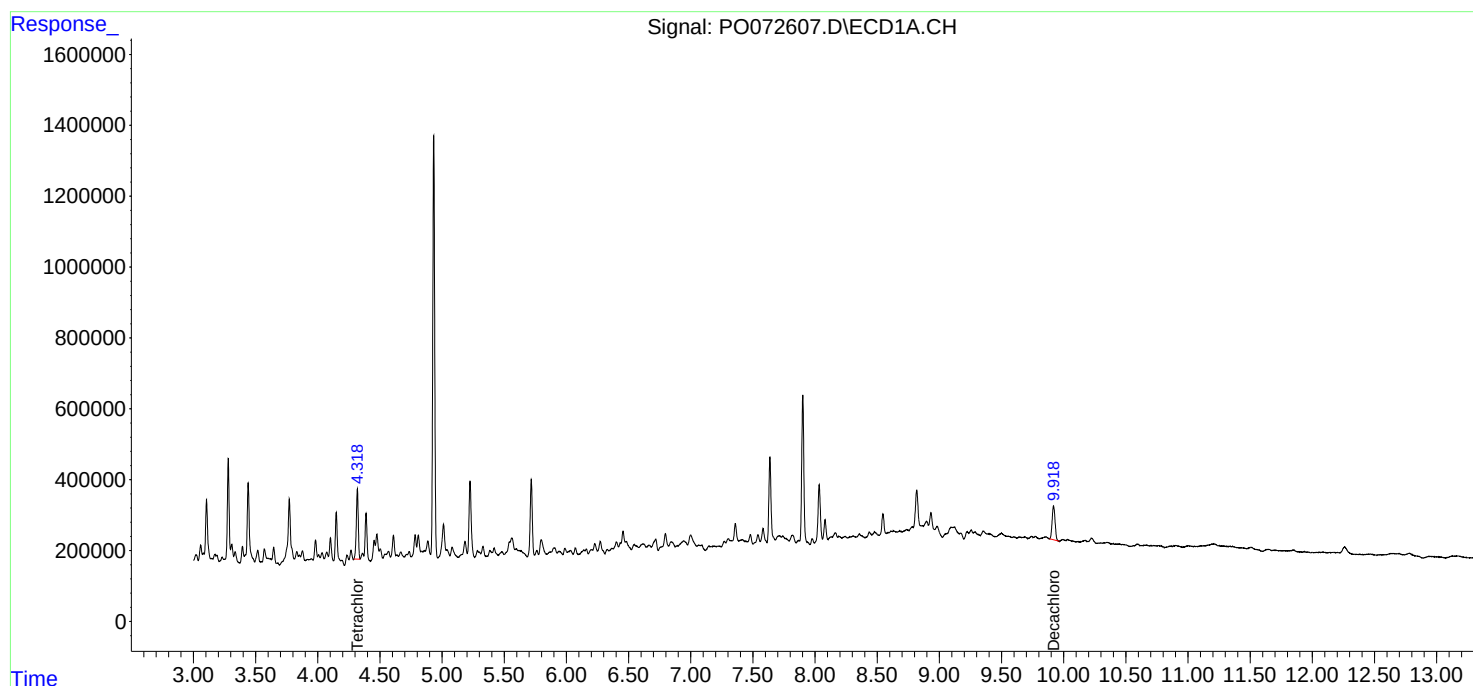


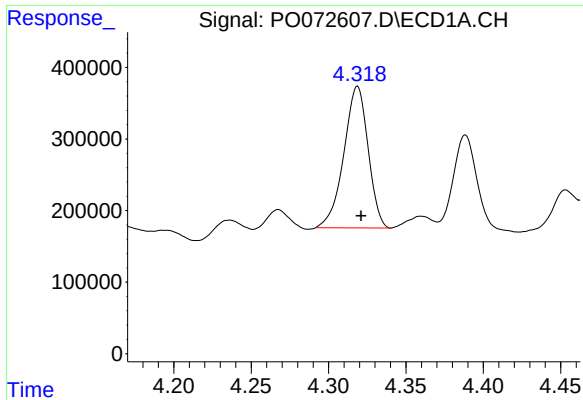

#1 Tetrachloro-m-xylene


R.T.: 4.319 min  
Delta R.T.: -0.002 min  
Response: 2160523  
Conc: 25.47 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
HP-640

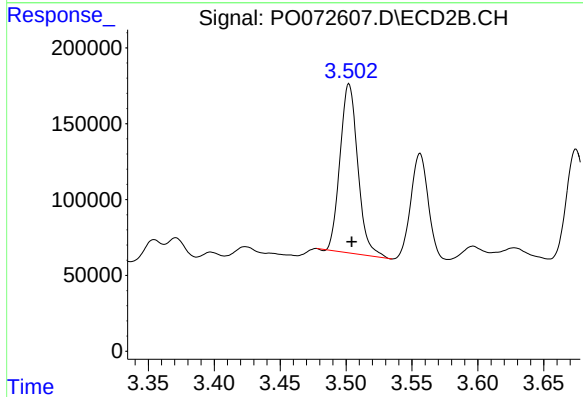


#1 Tetrachloro-m-xylene

R.T.: 3.502 min  
Delta R.T.: -0.002 min  
Response: 1048026  
Conc: 24.88 ng/ml

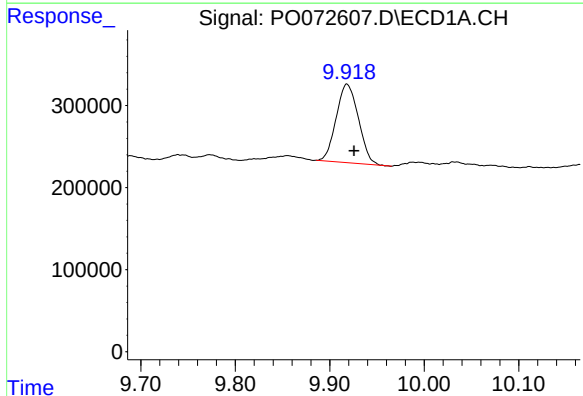

#2 Decachlorobiphenyl

R.T.: 9.918 min  
Delta R.T.: -0.008 min  
Response: 1565871  
Conc: 14.20 ng/ml

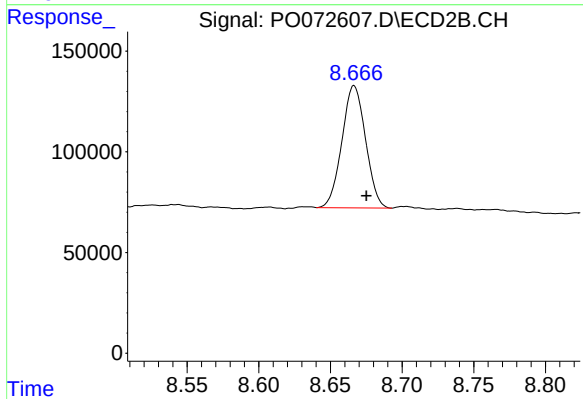

#2 Decachlorobiphenyl

R.T.: 8.667 min  
Delta R.T.: -0.009 min  
Response: 695204  
Conc: 13.45 ng/ml