

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102120\
 Data File : P0072618.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Oct 2020 17:14
 Operator : DD\AJ
 Sample : L4463-02
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 VNJ-238

Manual Integrations
 APPROVED

Ankita
 10/22/2020 12:12:52 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 07:36:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 14 17:47:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.318	3.501	2030291	1051811	23.937	24.971
2) SA Decachlor...	9.917	8.666	2155659	1160298	19.543	22.445m
Target Compounds						
26) L6 AR-1254-1	6.507	5.572	401646	291635	95.077m	105.504
27) L6 AR-1254-2	6.738	5.732	744269	230912	114.840m	94.976
28) L6 AR-1254-3	7.113	6.140	709156	367783	104.337m	95.576
29) L6 AR-1254-4	7.409	6.381	843460	310738	127.252	115.720
30) L6 AR-1254-5	7.830	6.801	687008	437876	107.249	119.484

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102120\
Data File : PO072618.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Oct 2020 17:14
Operator : DD\AJ
Sample : L4463-02
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
VNJ-238


Manual Integrations
APPROVED

Ankita
10/22/2020 12:12:52 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 07:36:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 14 17:47:24 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

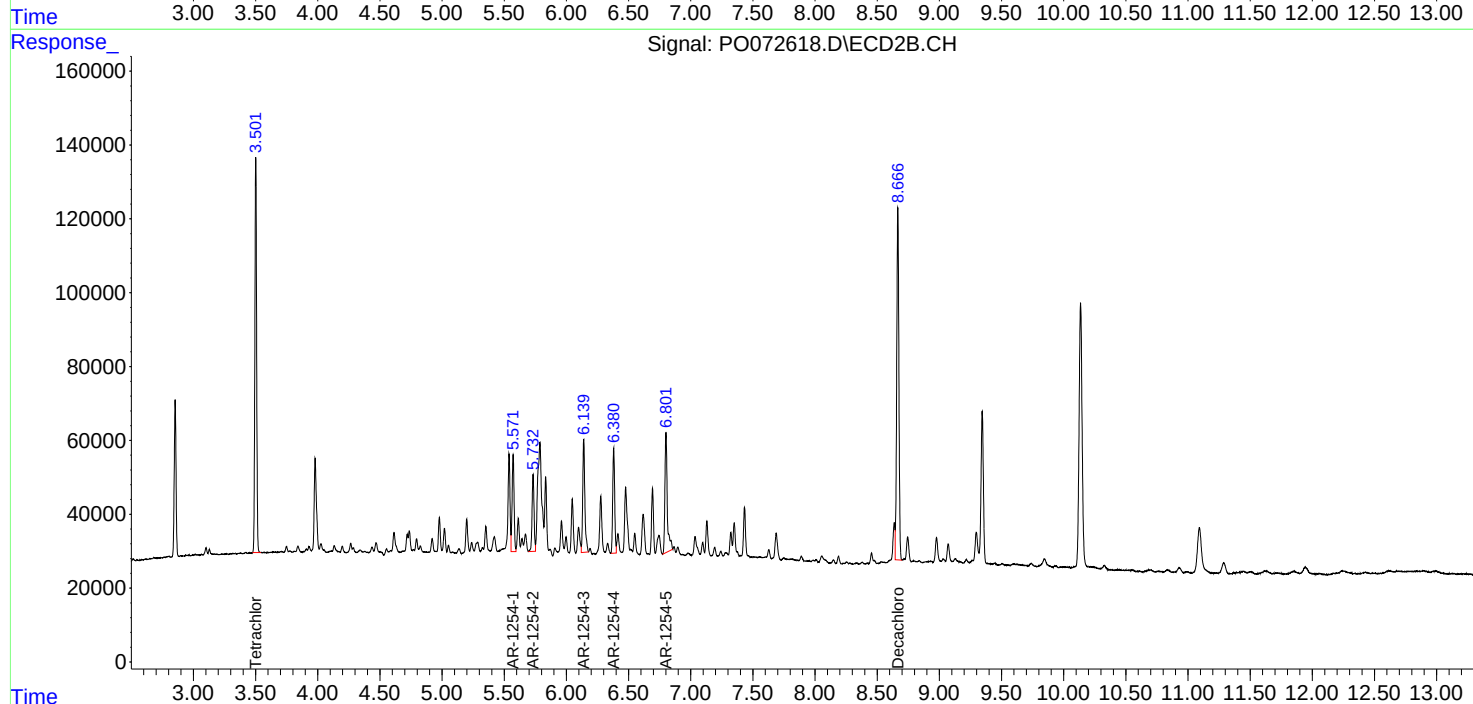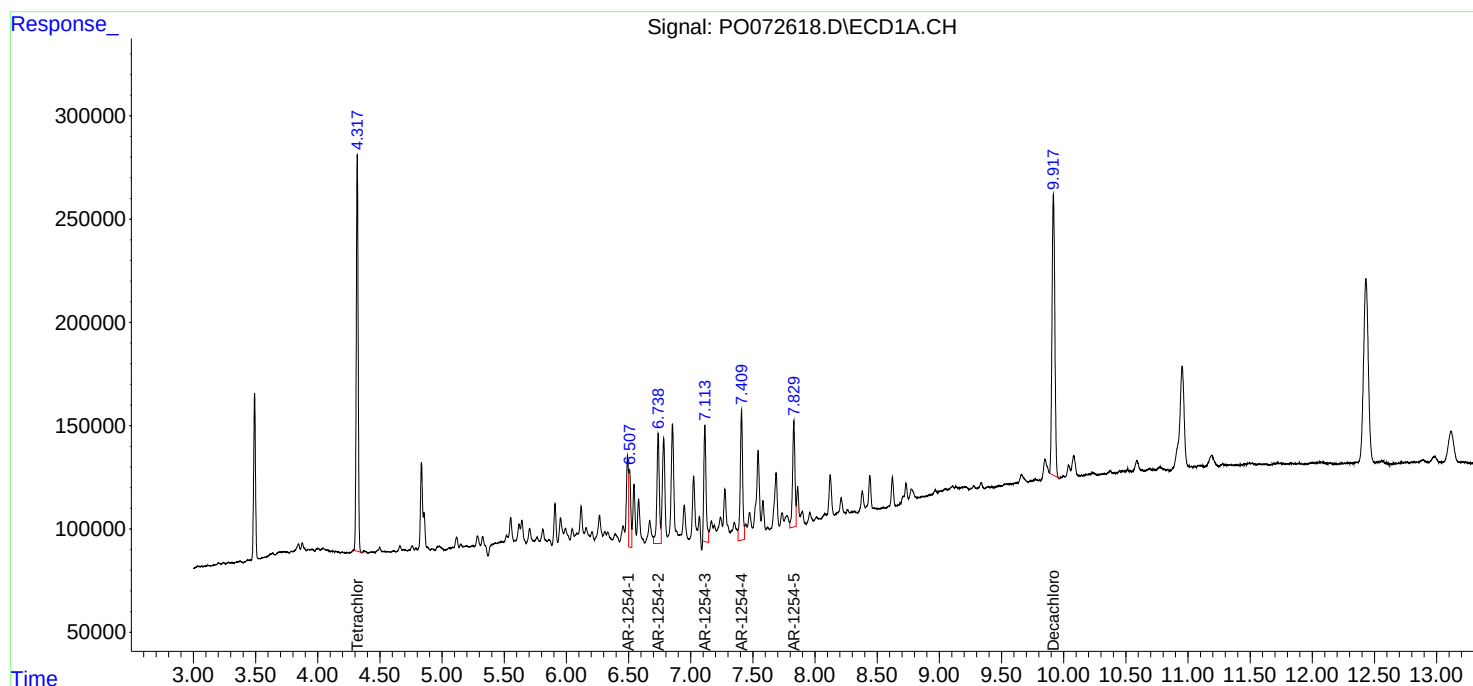

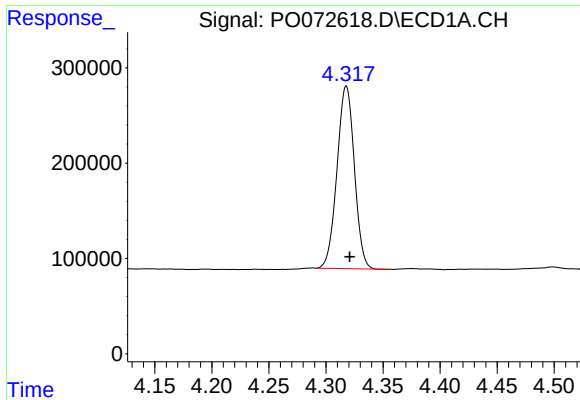


#1 Tetrachloro-m-xylene

R.T.: 4.318 min
Delta R.T.: -0.003 min
Response: 2030291
Conc: 23.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
VNJ-238


Manual Integrations
APPROVED

Ankita
10/22/2020 12:12:52 PM

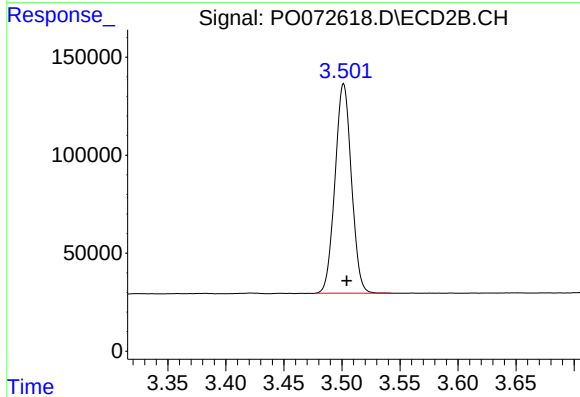


#1 Tetrachloro-m-xylene

R.T.: 3.501 min
Delta R.T.: -0.003 min
Response: 1051811
Conc: 24.97 ng/ml

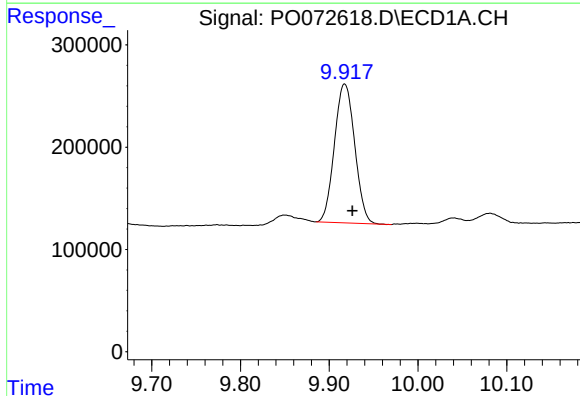


#2 Decachlorobiphenyl

R.T.: 9.917 min
Delta R.T.: -0.009 min
Response: 2155659
Conc: 19.54 ng/ml

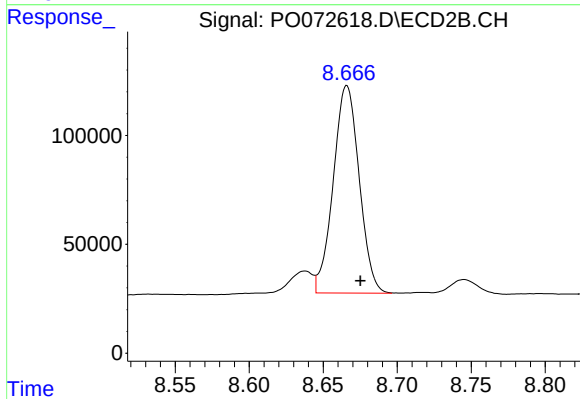

#2 Decachlorobiphenyl

R.T.: 8.666 min
Delta R.T.: -0.010 min
Response: 1160298
Conc: 22.45 ng/ml m

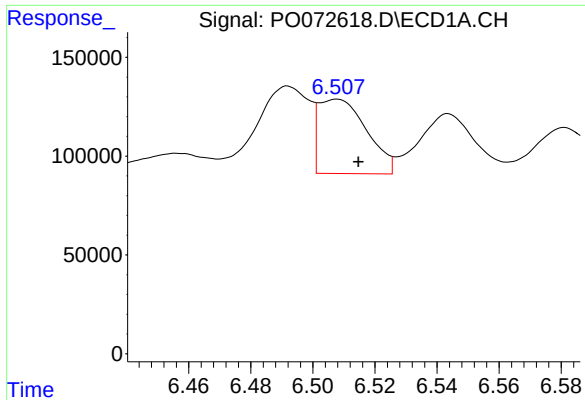


#26 AR-1254-1

R.T.: 6.507 min
Delta R.T.: -0.007 min
Response: 401646
Conc: 95.08 ng/ml m

Instrument :
ECD_O
ClientSampleId :
VNJ-238


Manual Integrations
APPROVED

Ankita
10/22/2020 12:12:52 PM

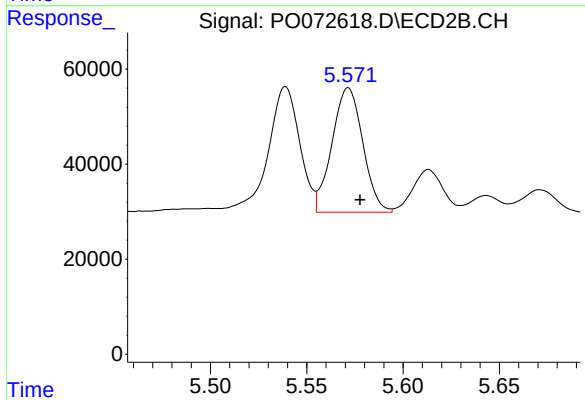


#26 AR-1254-1

R.T.: 5.572 min
Delta R.T.: -0.006 min
Response: 291635
Conc: 105.50 ng/ml

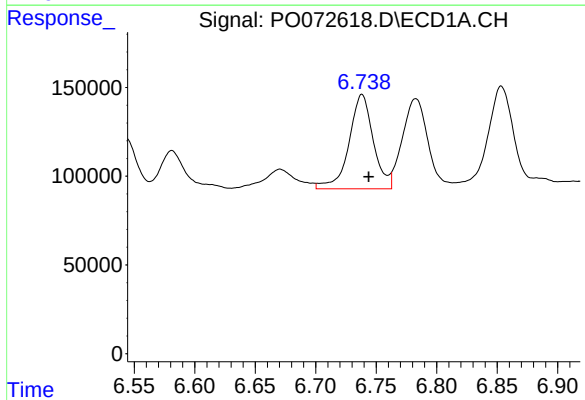


#27 AR-1254-2

R.T.: 6.738 min
Delta R.T.: -0.006 min
Response: 744269
Conc: 114.84 ng/ml m

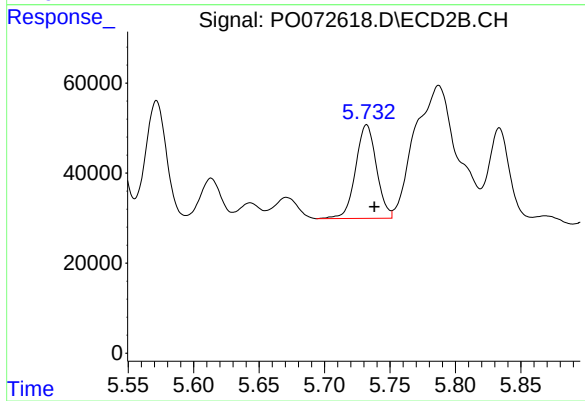

#27 AR-1254-2

R.T.: 5.732 min
Delta R.T.: -0.006 min
Response: 230912
Conc: 94.98 ng/ml

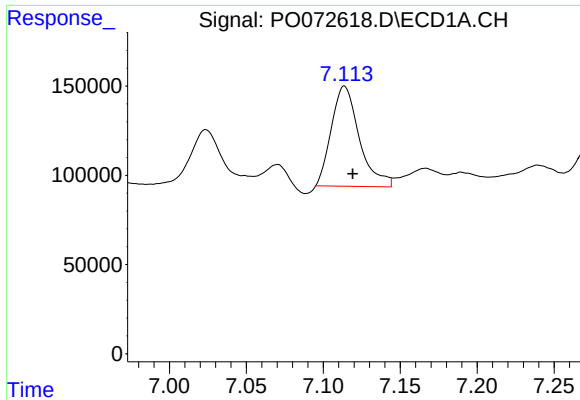


#28 AR-1254-3

R.T.: 7.113 min
Delta R.T.: -0.006 min
Response: 709156
Conc: 104.34 ng/ml m

Instrument :
ECD_O
ClientSampleId :
VNJ-238


Manual Integrations
APPROVED

Ankita
10/22/2020 12:12:52 PM

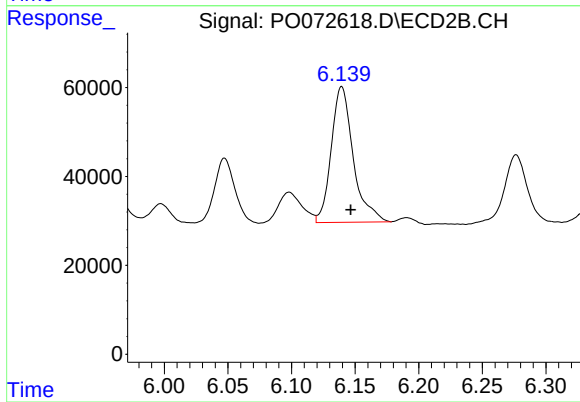


#28 AR-1254-3

R.T.: 6.140 min
Delta R.T.: -0.007 min
Response: 367783
Conc: 95.58 ng/ml

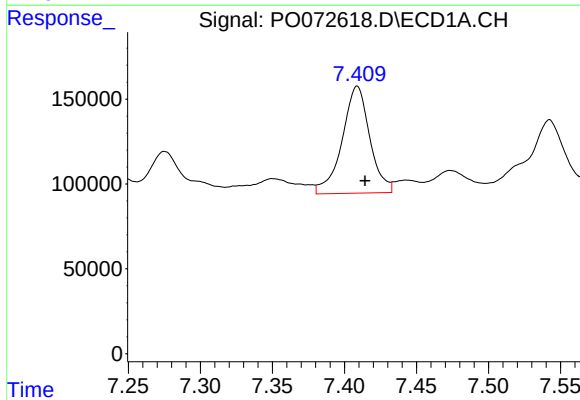


#29 AR-1254-4

R.T.: 7.409 min
Delta R.T.: -0.005 min
Response: 843460
Conc: 127.25 ng/ml

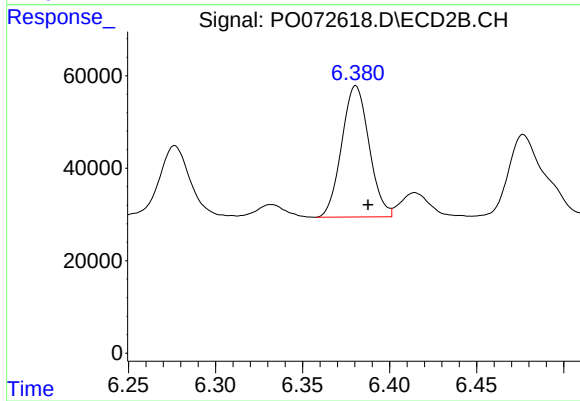

#29 AR-1254-4

R.T.: 6.381 min
Delta R.T.: -0.007 min
Response: 310738
Conc: 115.72 ng/ml

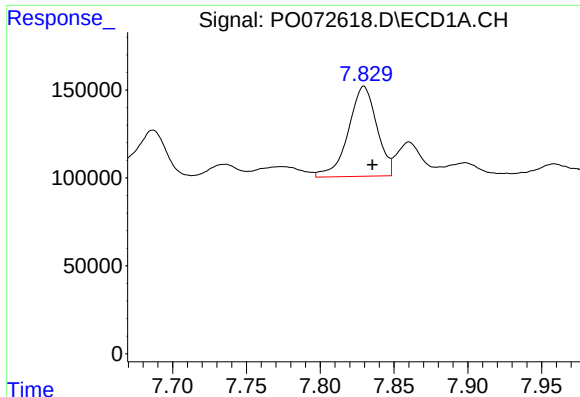


#30 AR-1254-5

R.T.: 7.830 min
Delta R.T.: -0.006 min
Response: 687008
Conc: 107.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
VNJ-238

Manual Integrations
APPROVED

Ankita
10/22/2020 12:12:52 PM

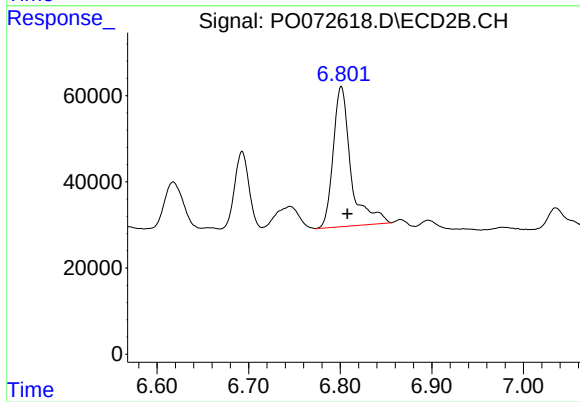

#30 AR-1254-5

R.T.: 6.801 min
Delta R.T.: -0.007 min
Response: 437876
Conc: 119.48 ng/ml