

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102120\
 Data File : P0072629.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Oct 2020 20:22
 Operator : DD\AJ
 Sample : L4472-03
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PCB-101720-SR-03

Manual Integrations
 APPROVED

Ankita
 10/22/2020 12:13:05 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 07:55:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 14 17:47:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.318	3.502	2025153	1050117	23.876	24.930
2) SA Decachlor...	9.918	8.665	2402394	1376886	21.780	26.635m
Target Compounds						
26) L6 AR-1254-1	6.511	5.571	144427	103112	34.189	37.303
27) L6 AR-1254-2	6.737	5.733	212821	97118	32.838	39.945
28) L6 AR-1254-3	7.113	6.140	246111	115460	36.210	30.005
29) L6 AR-1254-4	7.410	6.380	282561	122450	42.630	45.601
30) L6 AR-1254-5	7.827	6.801	486566	193120	75.958	52.697 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102120\
Data File : PO072629.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Oct 2020 20:22
Operator : DD\AJ
Sample : L4472-03
Misc :
ALS Vial : 38 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PCB-101720-SR-03


Manual Integrations
APPROVED

Ankita
10/22/2020 12:13:05 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 07:55:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 14 17:47:24 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

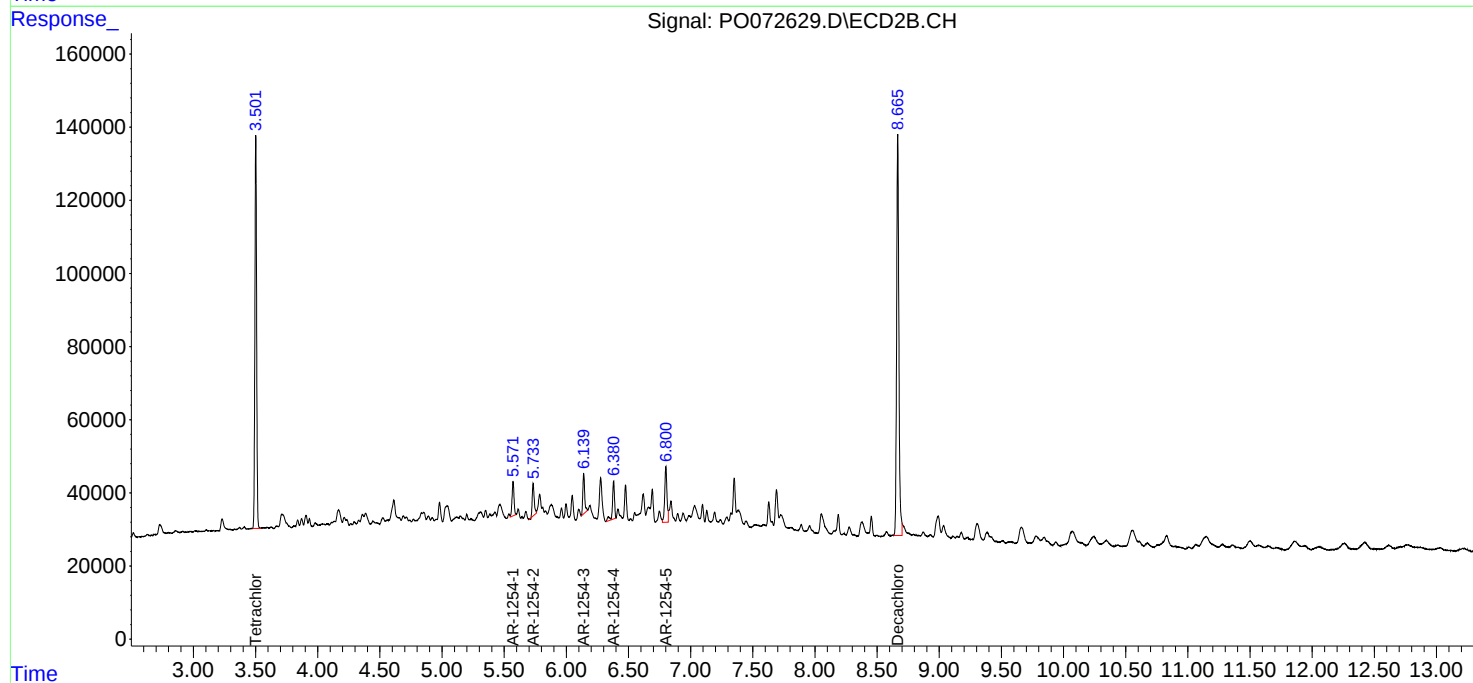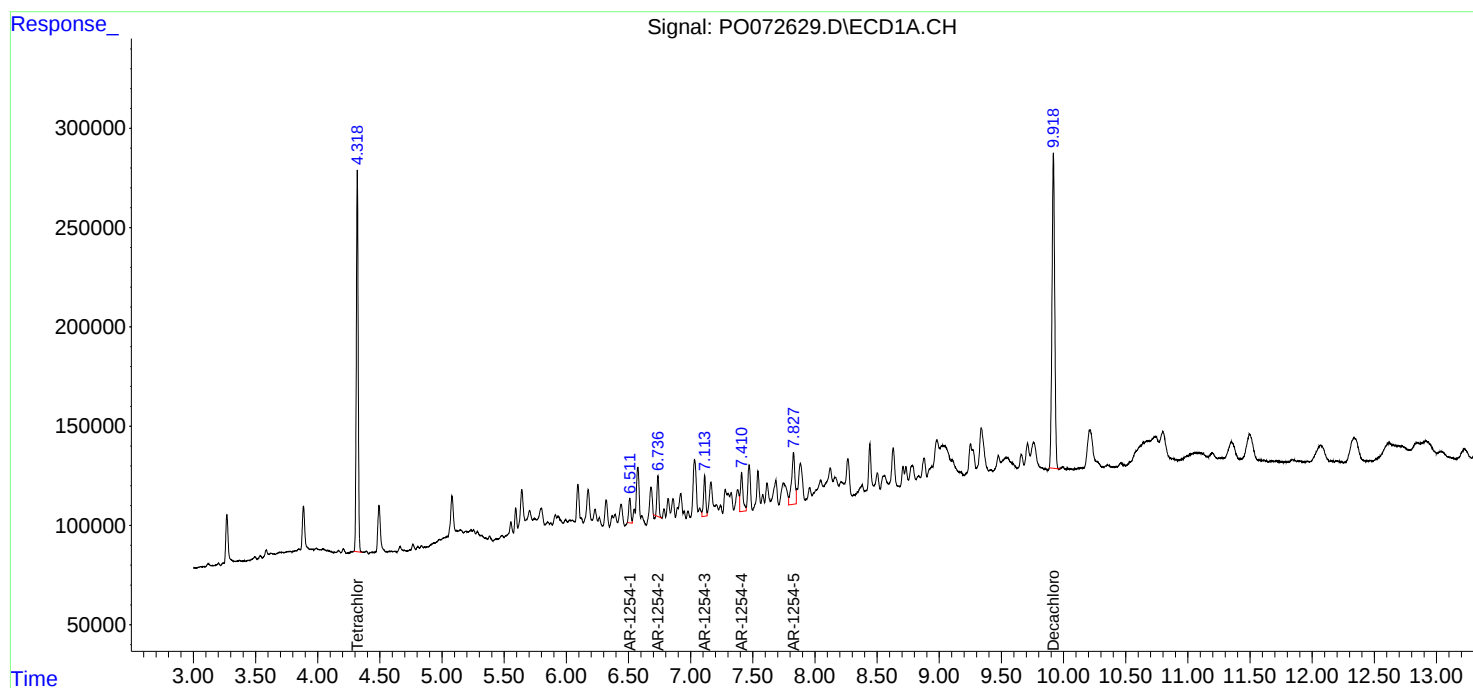

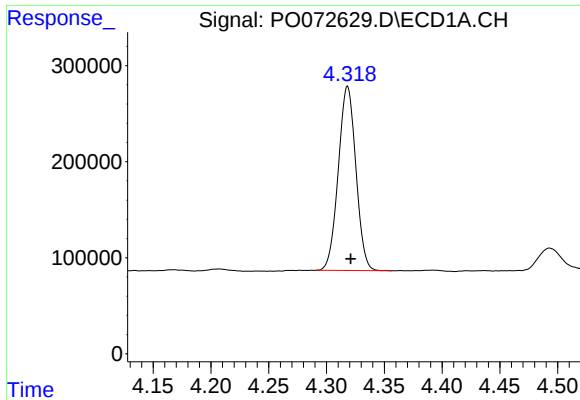


#1 Tetrachloro-m-xylene

R.T.: 4.318 min
Delta R.T.: -0.003 min
Response: 2025153
Conc: 23.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-101720-SR-03


Manual Integrations
APPROVED

Ankita
10/22/2020 12:13:05 PM

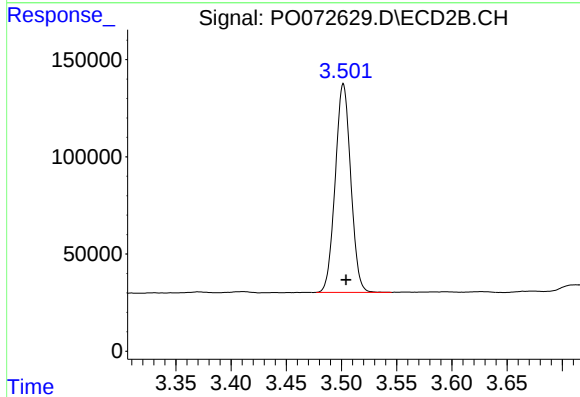


#1 Tetrachloro-m-xylene

R.T.: 3.502 min
Delta R.T.: -0.003 min
Response: 1050117
Conc: 24.93 ng/ml

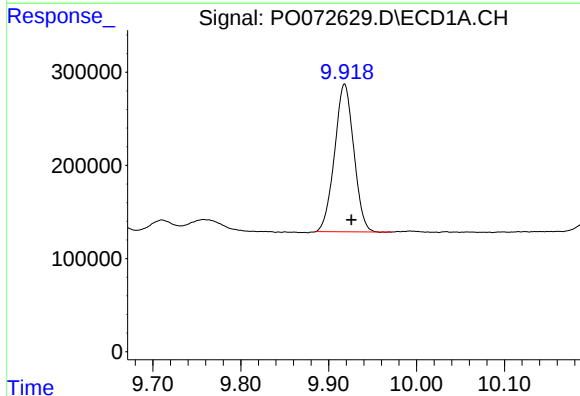


#2 Decachlorobiphenyl

R.T.: 9.918 min
Delta R.T.: -0.008 min
Response: 2402394
Conc: 21.78 ng/ml

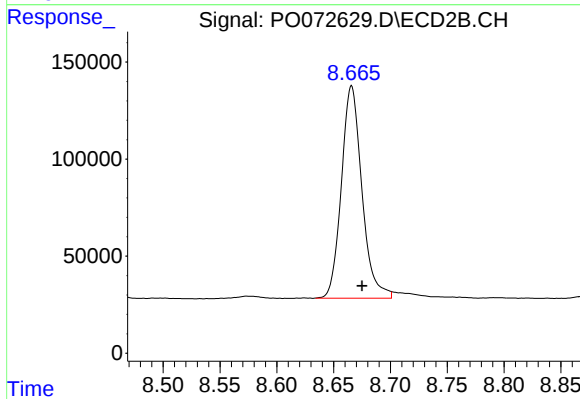

#2 Decachlorobiphenyl

R.T.: 8.665 min
Delta R.T.: -0.010 min
Response: 1376886
Conc: 26.63 ng/ml m

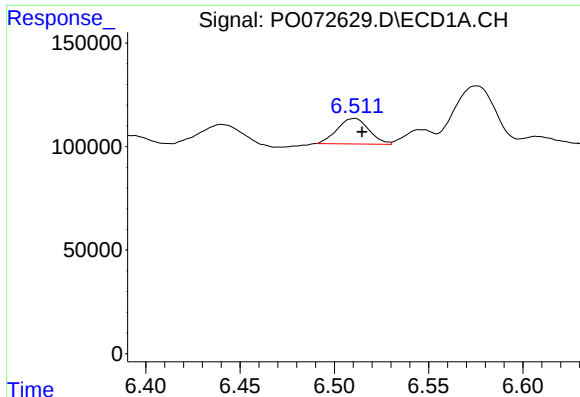


#26 AR-1254-1

R.T.: 6.511 min
Delta R.T.: -0.004 min
Response: 144427
Conc: 34.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-101720-SR-03


Manual Integrations
APPROVED

Ankita
10/22/2020 12:13:05 PM

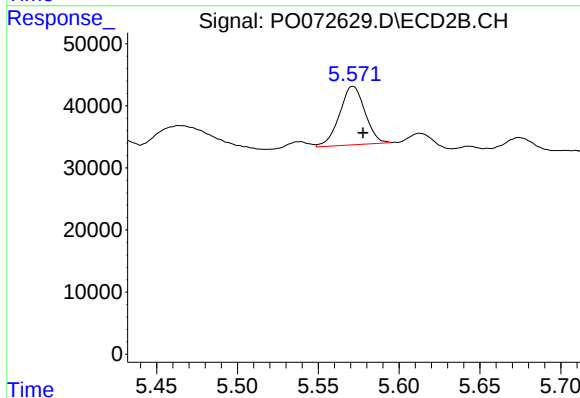


#26 AR-1254-1

R.T.: 5.571 min
Delta R.T.: -0.006 min
Response: 103112
Conc: 37.30 ng/ml

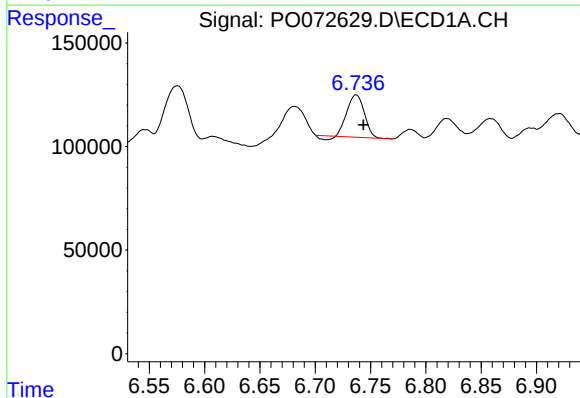


#27 AR-1254-2

R.T.: 6.737 min
Delta R.T.: -0.007 min
Response: 212821
Conc: 32.84 ng/ml

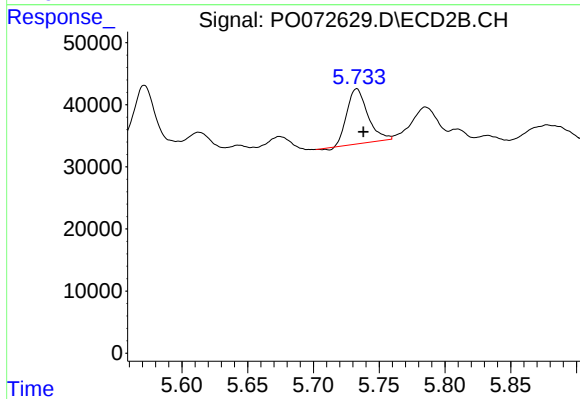

#27 AR-1254-2

R.T.: 5.733 min
Delta R.T.: -0.005 min
Response: 97118
Conc: 39.95 ng/ml

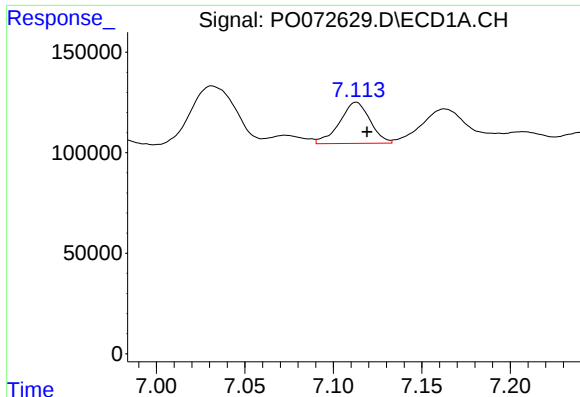


#28 AR-1254-3

R.T.: 7.113 min
Delta R.T.: -0.006 min
Response: 246111
Conc: 36.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-101720-SR-03


Manual Integrations
APPROVED

Ankita
10/22/2020 12:13:05 PM

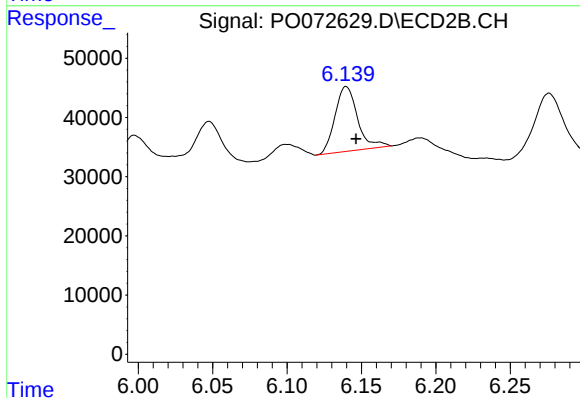


#28 AR-1254-3

R.T.: 6.140 min
Delta R.T.: -0.007 min
Response: 115460
Conc: 30.00 ng/ml

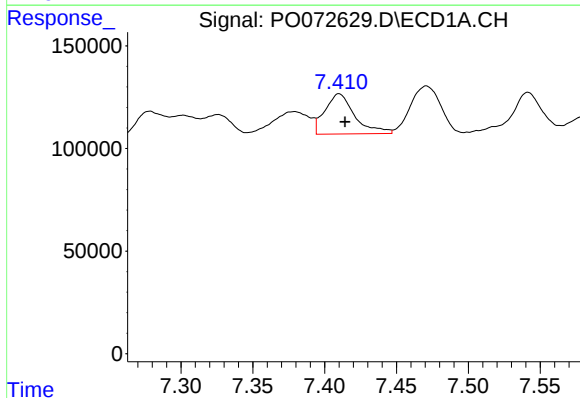


#29 AR-1254-4

R.T.: 7.410 min
Delta R.T.: -0.004 min
Response: 282561
Conc: 42.63 ng/ml

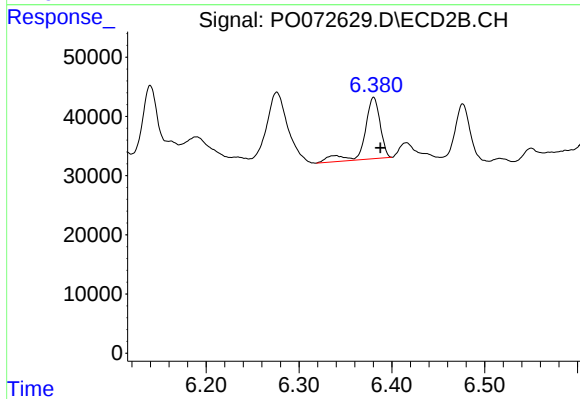

#29 AR-1254-4

R.T.: 6.380 min
Delta R.T.: -0.007 min
Response: 122450
Conc: 45.60 ng/ml

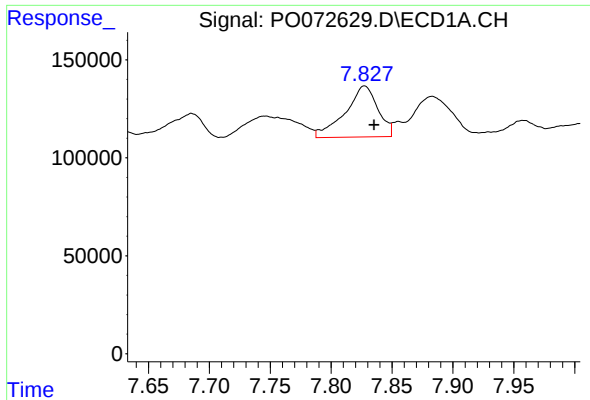


#30 AR-1254-5

R.T.: 7.827 min
Delta R.T.: -0.008 min
Response: 486566
Conc: 75.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-101720-SR-03

Manual Integrations
APPROVED

Ankita
10/22/2020 12:13:05 PM

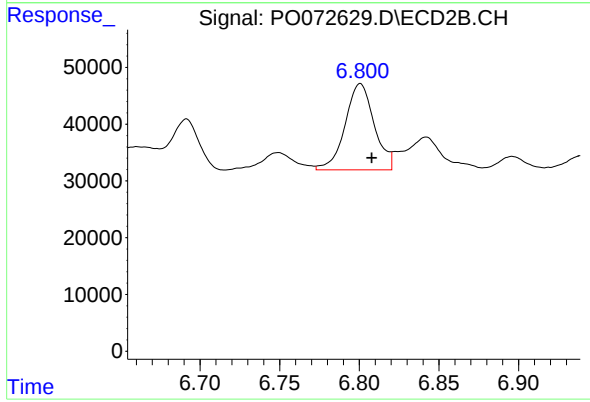

#30 AR-1254-5

R.T.: 6.801 min
Delta R.T.: -0.007 min
Response: 193120
Conc: 52.70 ng/ml