

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102120\
 Data File : P0072638.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Oct 2020 22:56
 Operator : DD\AJ
 Sample : L4221-10
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OK-03-102020

Manual Integrations
 APPROVED

Ankita
 10/22/2020 12:13:17 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 08:12:35 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 14 17:47:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.318	3.502	2034453	1031250	23.986m	24.482
2) SA Decachlor...	9.920	8.667	1999078	995801	18.123	19.263

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102120\
Data File : PO072638.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Oct 2020 22:56
Operator : DD\AJ
Sample : L4221-10
Misc :
ALS Vial : 45 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OK-03-102020


Manual Integrations
APPROVED

Ankita
10/22/2020 12:13:17 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 08:12:35 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 14 17:47:24 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

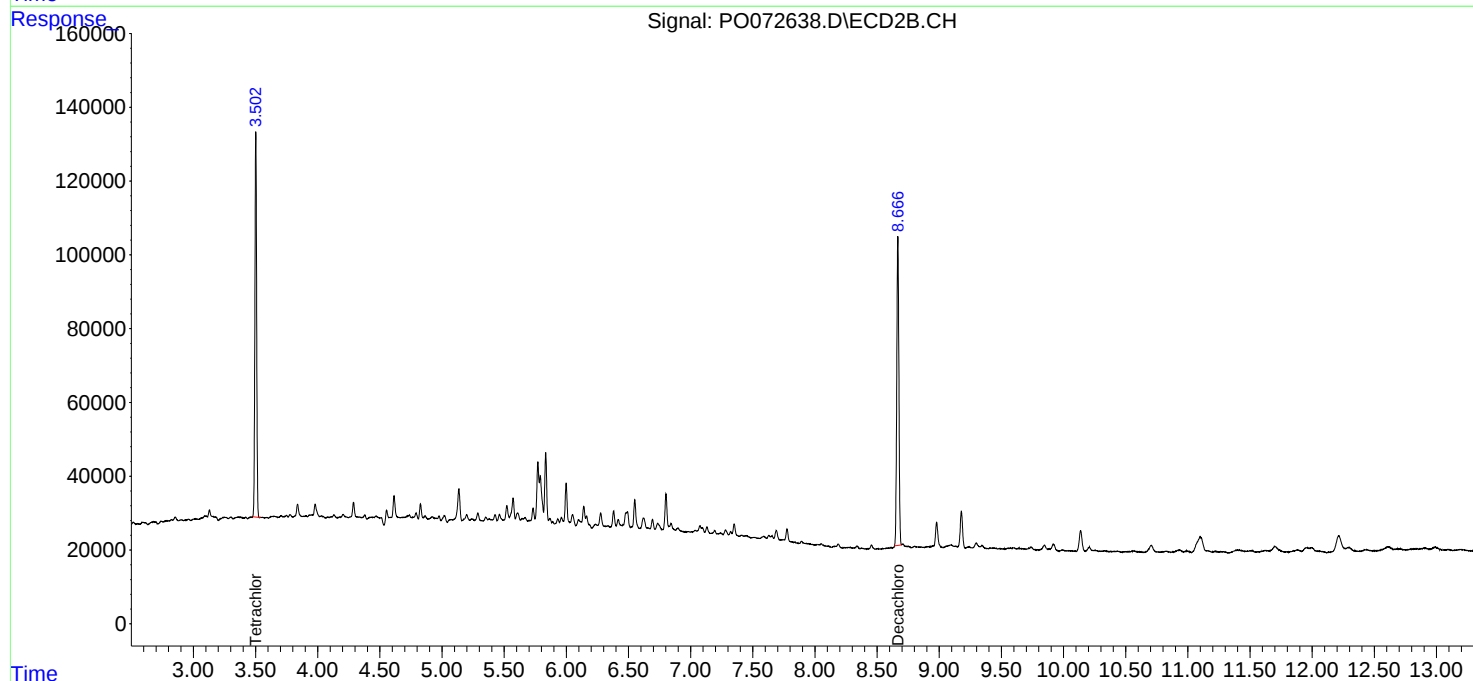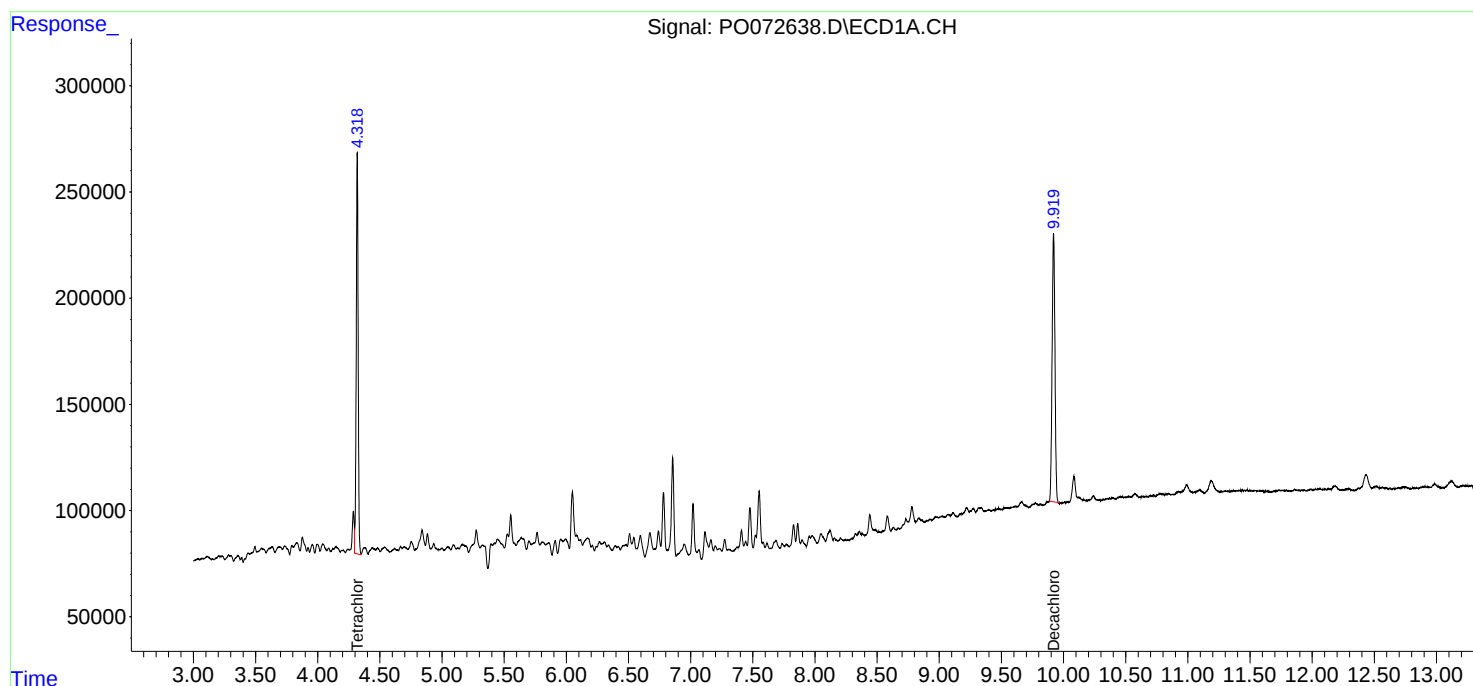

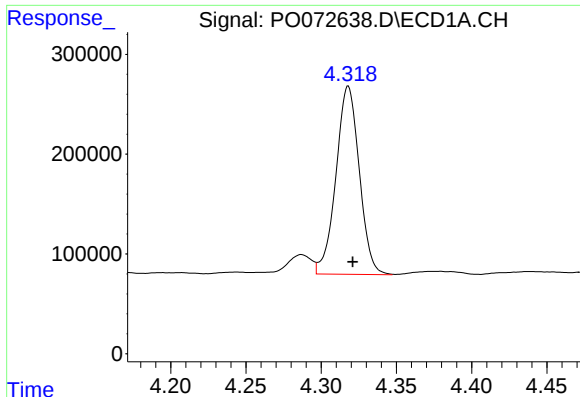


#1 Tetrachloro-m-xylene

R.T.: 4.318 min
Delta R.T.: -0.003 min
Response: 2034453
Conc: 23.99 ng/ml m

Instrument :
ECD_O
ClientSampleId :
OK-03-102020


Manual Integrations
APPROVED

Ankita
10/22/2020 12:13:17 PM

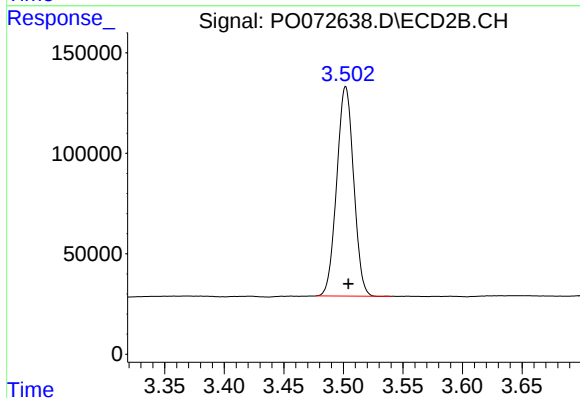


#1 Tetrachloro-m-xylene

R.T.: 3.502 min
Delta R.T.: -0.002 min
Response: 1031250
Conc: 24.48 ng/ml

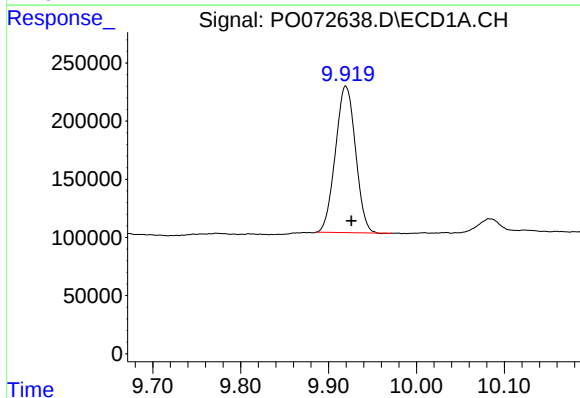

#2 Decachlorobiphenyl

R.T.: 9.920 min
Delta R.T.: -0.006 min
Response: 1999078
Conc: 18.12 ng/ml

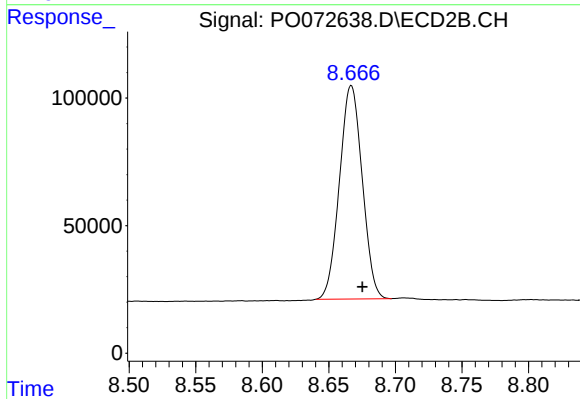

#2 Decachlorobiphenyl

R.T.: 8.667 min
Delta R.T.: -0.008 min
Response: 995801
Conc: 19.26 ng/ml