

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102218\
 Data File : PO050365.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Oct 2018 12:48
 Operator : SM/SJ
 Sample : J5577-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SSSI-1016-S-DH-22

Manual Integrations
 APPROVED

Sohil
 10/23/2018 9:41:13 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 13:46:15 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101818.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 19 02:02:26 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.357	3.355	4827615	4157499	16.179m	21.147 #
2) SA Decachlor...	10.021	8.108	3664328	3373397	16.887m	17.648m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102218\
Data File : P0050365.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Oct 2018 12:48
Operator : SM/SJ
Sample : J5577-02
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SSSI-1016-S-DH-22


Manual Integrations
APPROVED

Sohil
10/23/2018 9:41:13 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 13:46:15 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101818.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 19 02:02:26 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

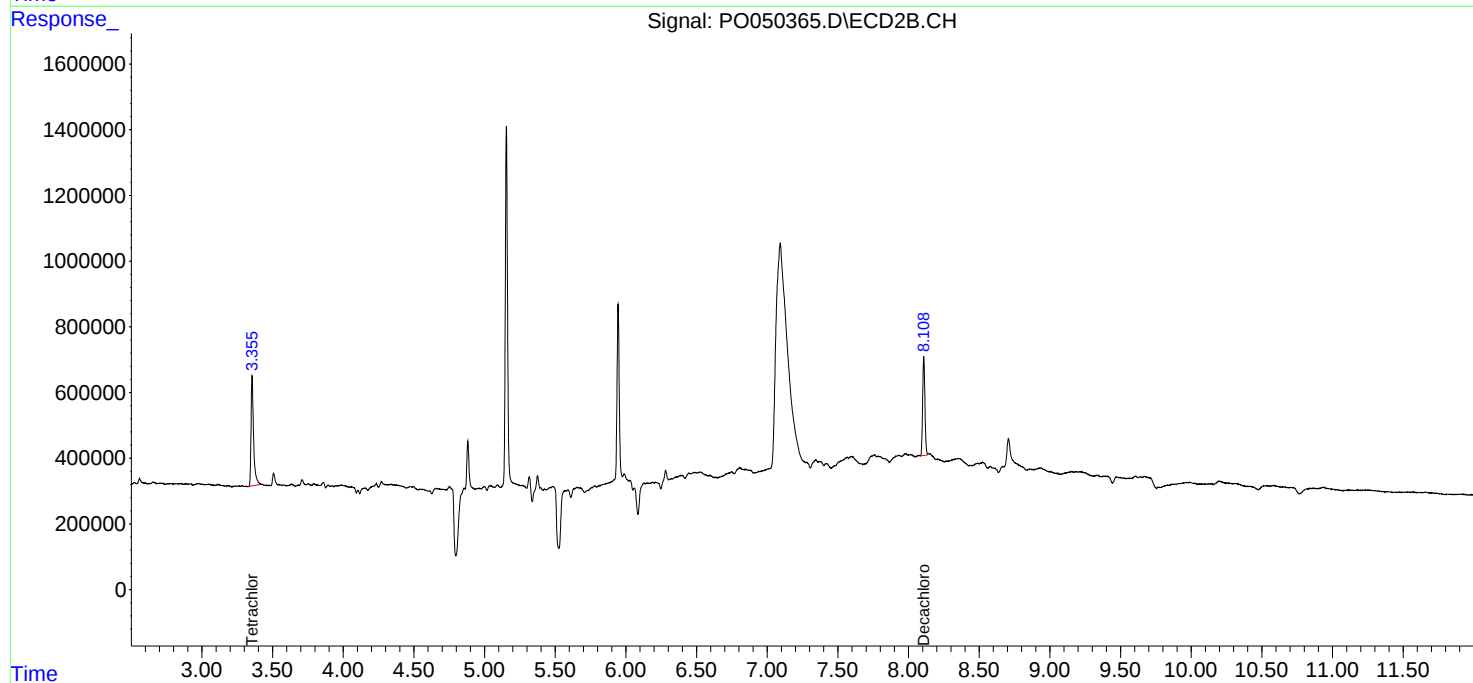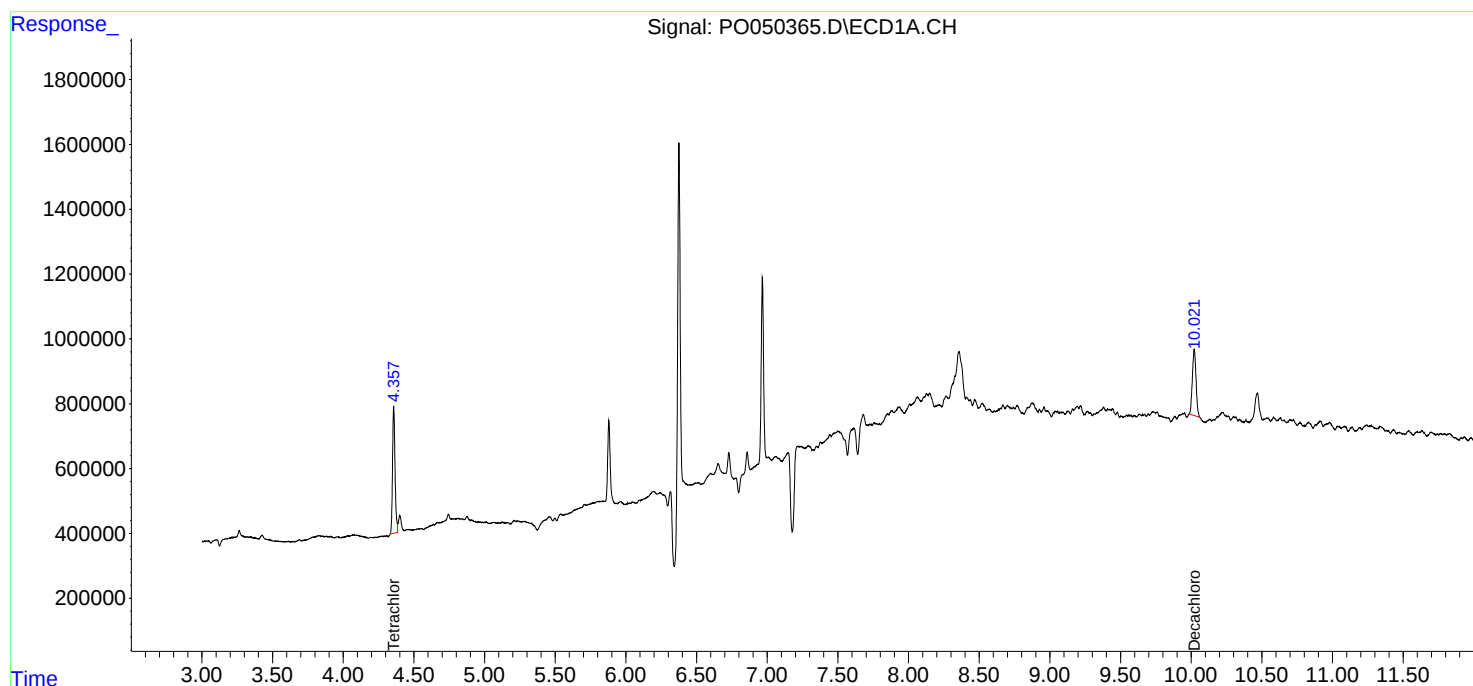

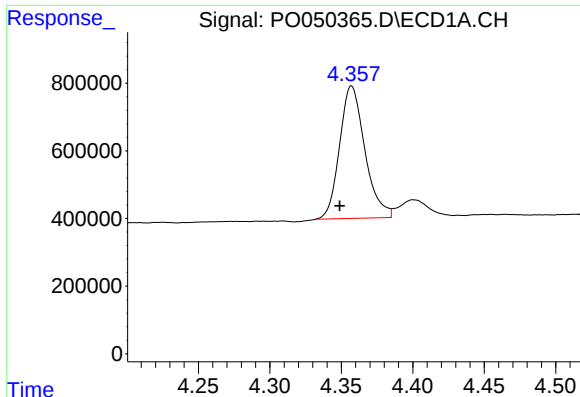


#1 Tetrachloro-m-xylene

R.T.: 4.357 min
Delta R.T.: 0.008 min
Response: 4827615
Conc: 16.18 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SSSI-1016-S-DH-22


Manual Integrations
APPROVED

Sohil
10/23/2018 9:41:13 AM

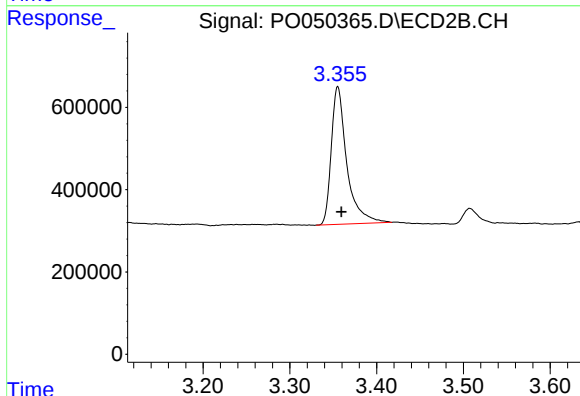


#1 Tetrachloro-m-xylene

R.T.: 3.355 min
Delta R.T.: -0.004 min
Response: 4157499
Conc: 21.15 ng/ml

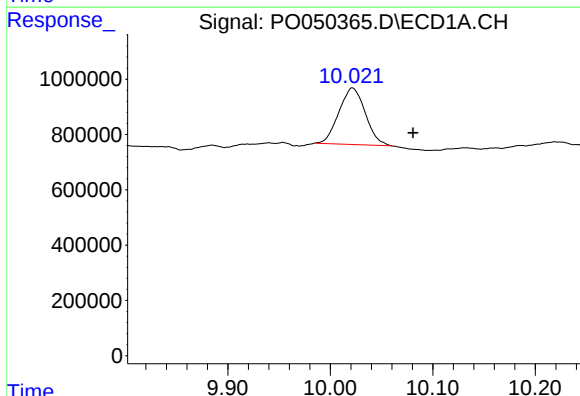

#2 Decachlorobiphenyl

R.T.: 10.021 min
Delta R.T.: -0.060 min
Response: 3664328
Conc: 16.89 ng/ml m

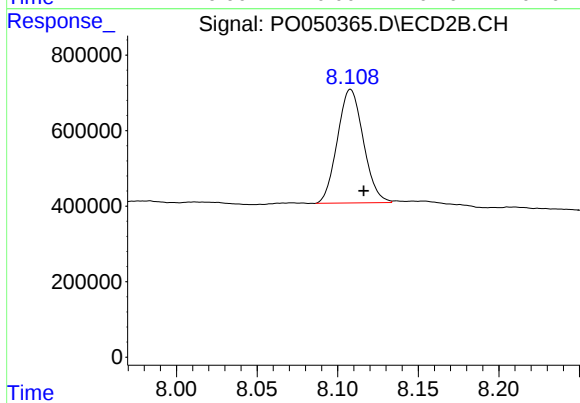

#2 Decachlorobiphenyl

R.T.: 8.108 min
Delta R.T.: -0.009 min
Response: 3373397
Conc: 17.65 ng/ml m