

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102218\
 Data File : P0050381.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Oct 2018 17:55
 Operator : SM/SJ
 Sample : J5604-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MS-VB-25868-BOX-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 00:46:57 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101818.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 19 02:02:26 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.358	3.356	2229425	2057965	7.471	10.468 #
2) SA Decachlor...	10.023	8.108	1049103	1011303	4.835m	5.291

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102218\
Data File : PO050381.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Oct 2018 17:55
Operator : SM/SJ
Sample : J5604-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MS-VB-25868-BOX-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 00:46:57 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101818.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 19 02:02:26 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

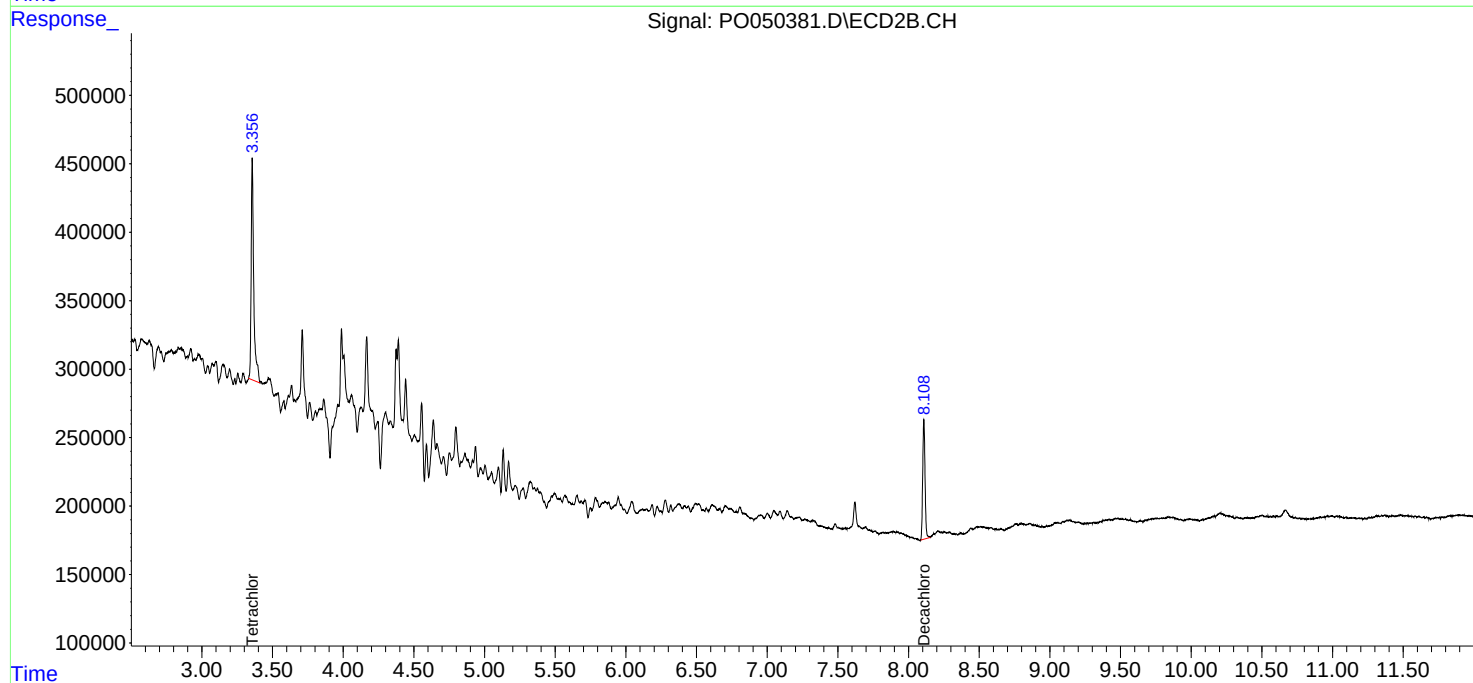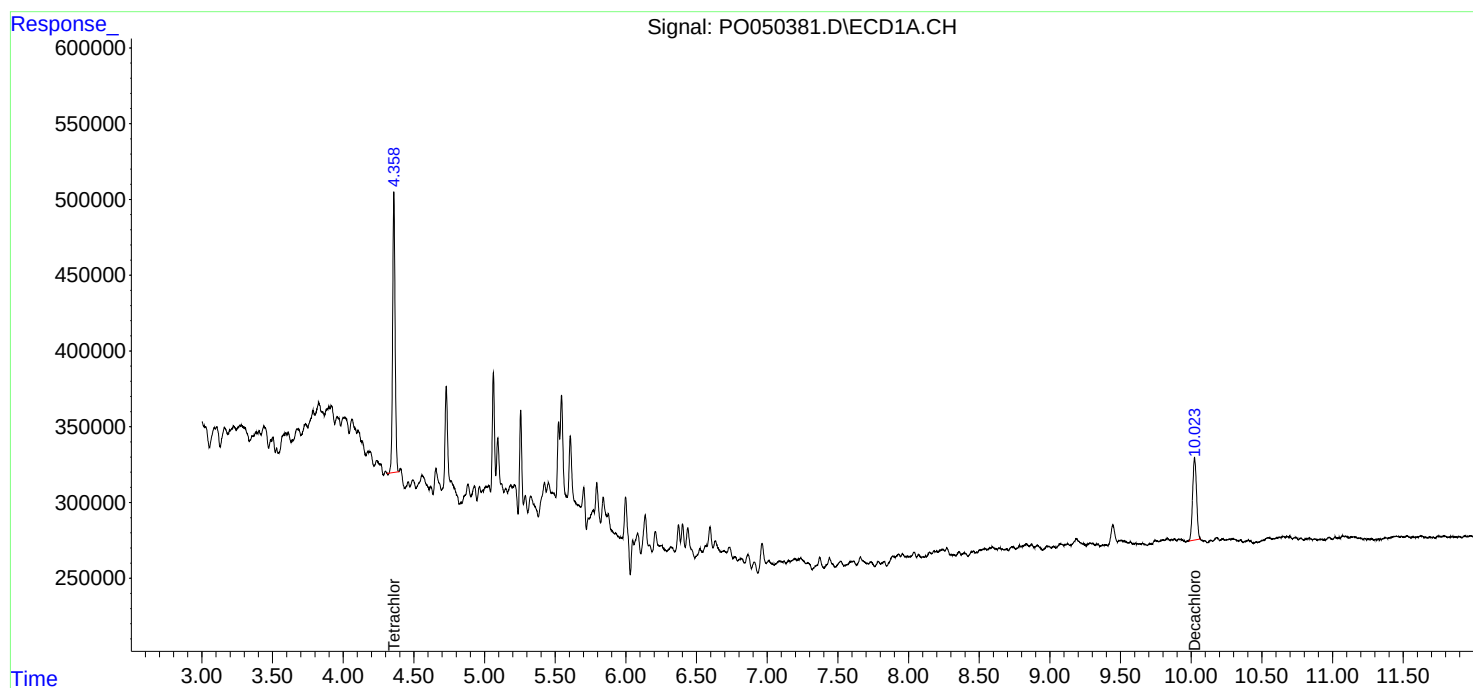


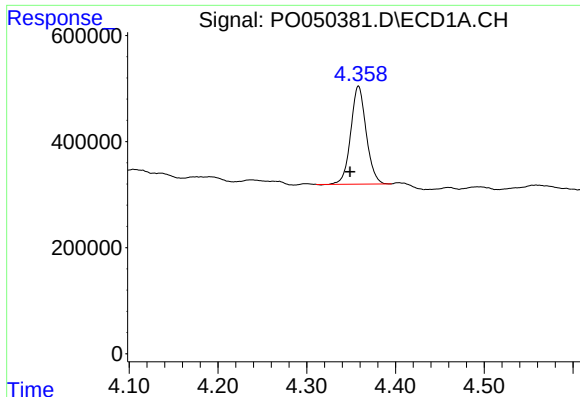

#1 Tetrachloro-m-xylene


R.T.: 4.358 min
Delta R.T.: 0.009 min
Response: 2229425
Conc: 7.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
MS-VB-25868-BOX-1

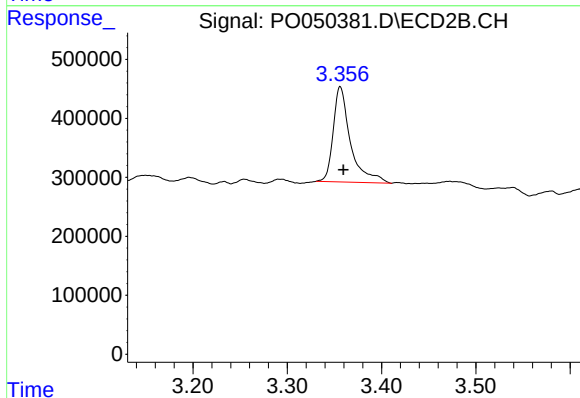


#1 Tetrachloro-m-xylene

R.T.: 3.356 min
Delta R.T.: -0.003 min
Response: 2057965
Conc: 10.47 ng/ml

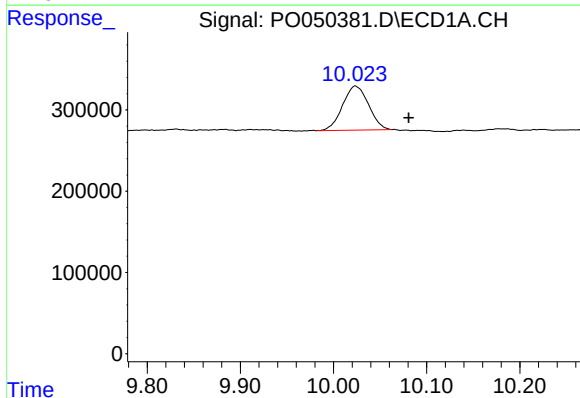

#2 Decachlorobiphenyl

R.T.: 10.023 min
Delta R.T.: -0.058 min
Response: 1049103
Conc: 4.83 ng/ml m

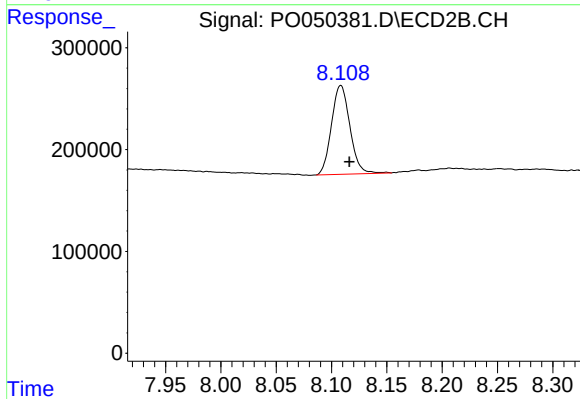

#2 Decachlorobiphenyl

R.T.: 8.108 min
Delta R.T.: -0.008 min
Response: 1011303
Conc: 5.29 ng/ml