

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102220\
 Data File : PO072693.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Oct 2020 1:46
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 06:06:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 14 17:47:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.318	3.502	1933024	1035338	22.790	24.580
2)	SA Decachlor...	9.918	8.665	2095677	1081406	18.999	20.919
Target Compounds							
20)	L4 AR-1242-5	0.000	5.591	0	139295	N.D.	101.458 #
24)	L5 AR-1248-4	6.524f	0.000	361031	0	81.641	N.D. #
25)	L5 AR-1248-5	0.000	5.591f	0	139295	N.D.	75.416 #
26)	L6 AR-1254-1	6.524	5.591	361031	139295	85.463	50.392 #
28)	L6 AR-1254-3	7.144f	6.140	112772	45216	16.592	11.750 #
39)	L8 AR-1262-4	8.777f	0.000	76089	0	19.040	N.D. #
42)	L9 AR-1268-2	8.777f	0.000	76089	0	4.609	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102220\
Data File : PO072693.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Oct 2020 1:46
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 06:06:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 14 17:47:24 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

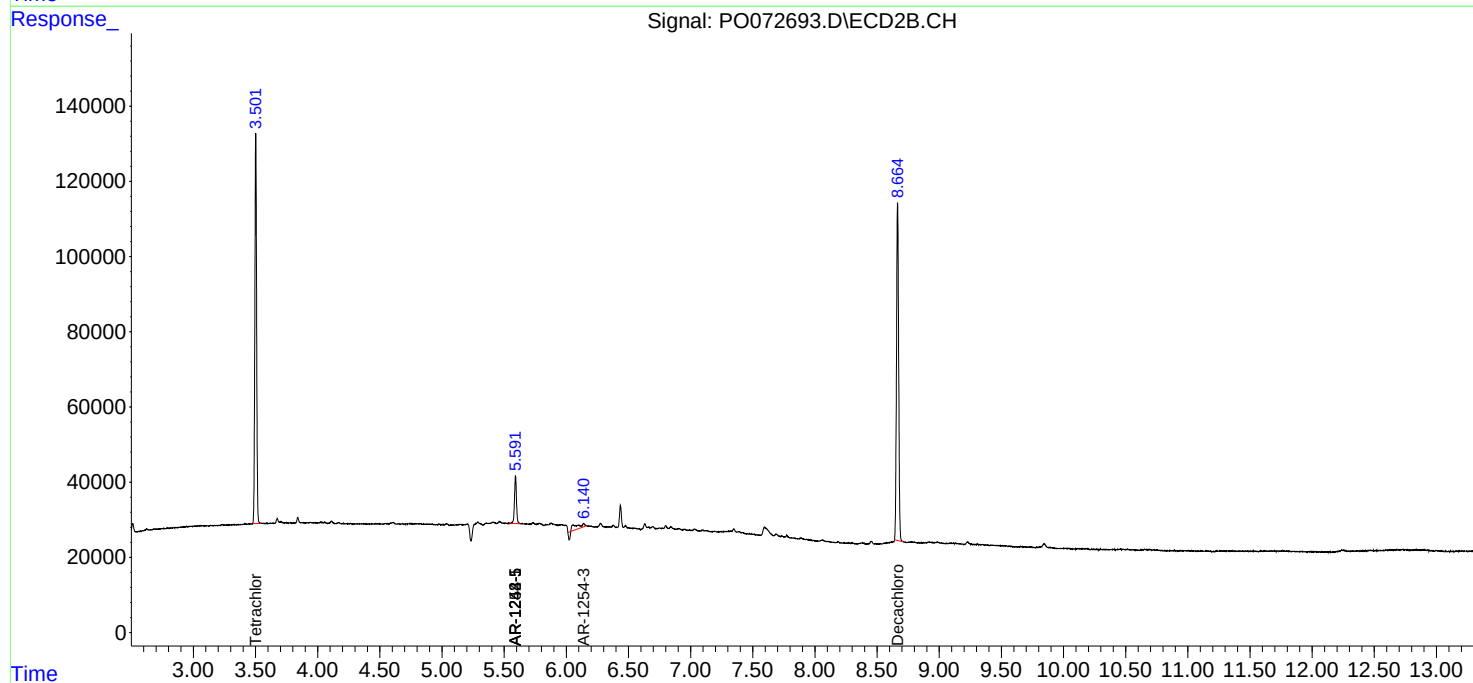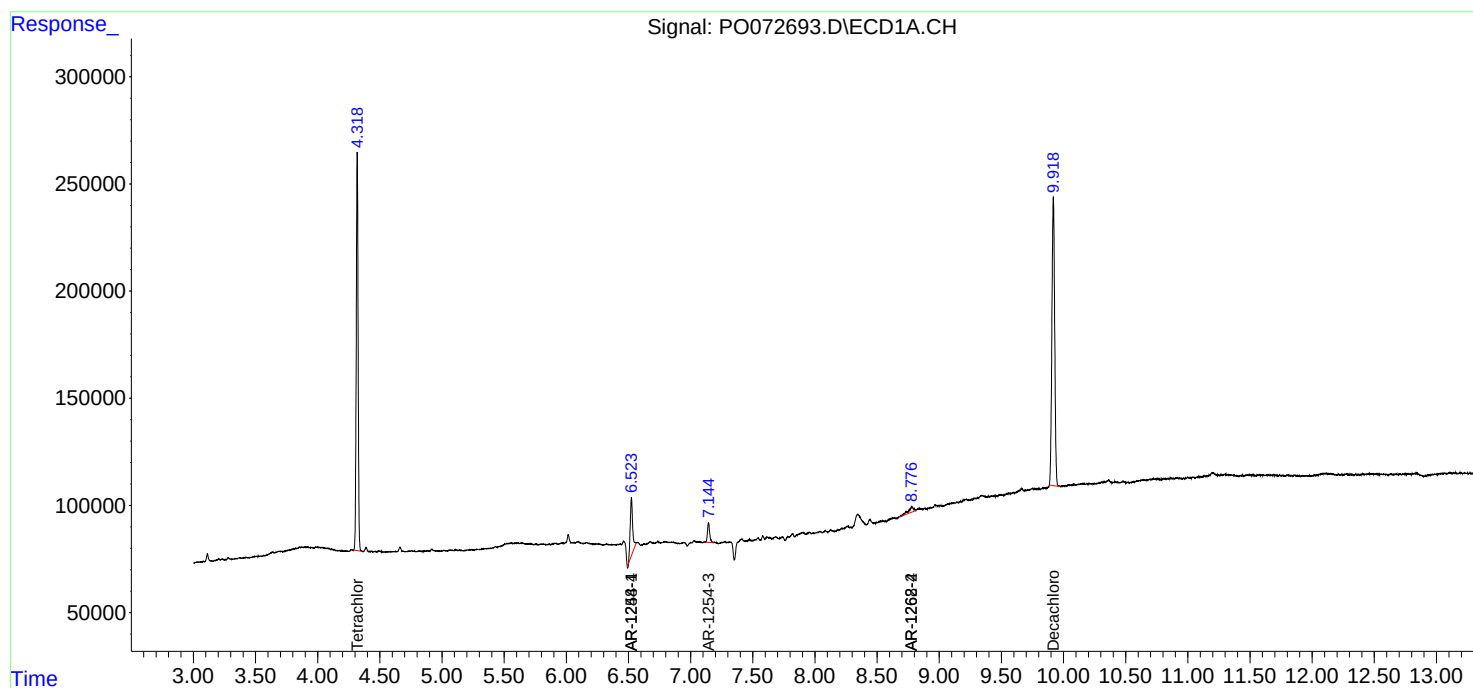


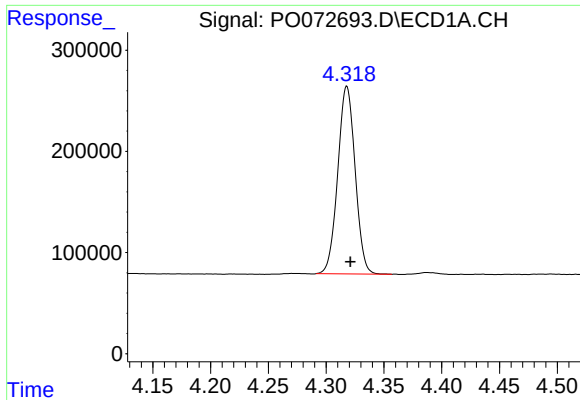

#1 Tetrachloro-m-xylene


R.T.: 4.318 min
Delta R.T.: -0.003 min
Response: 1933024
Conc: 22.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

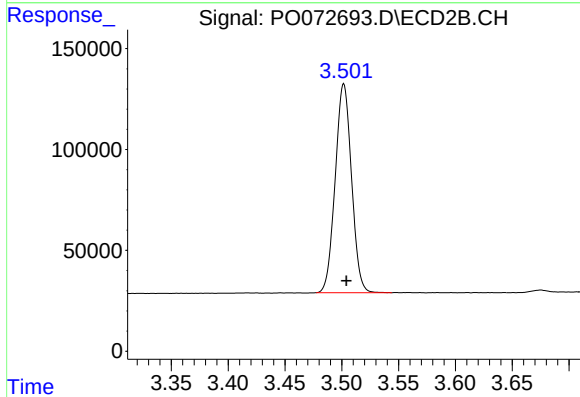


#1 Tetrachloro-m-xylene

R.T.: 3.502 min
Delta R.T.: -0.002 min
Response: 1035338
Conc: 24.58 ng/ml

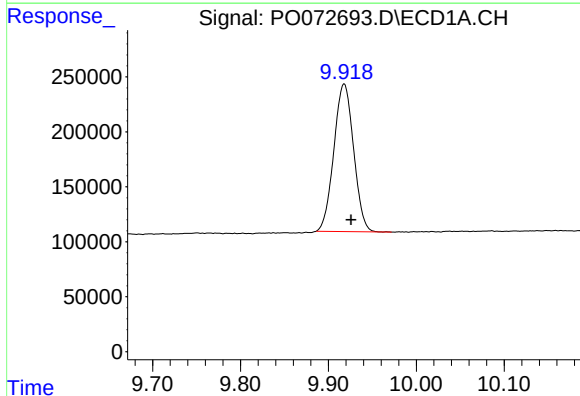


#2 Decachlorobiphenyl

R.T.: 9.918 min
Delta R.T.: -0.008 min
Response: 2095677
Conc: 19.00 ng/ml

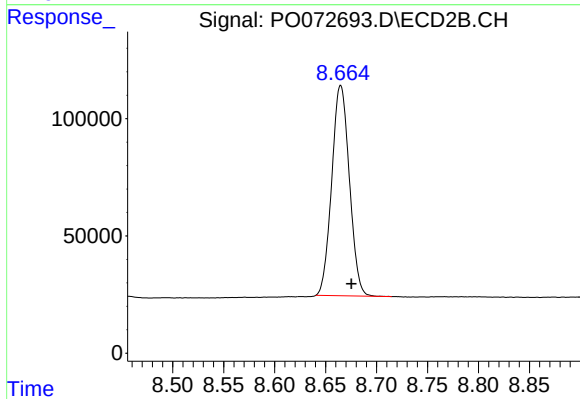

#2 Decachlorobiphenyl


R.T.: 8.665 min
Delta R.T.: -0.010 min
Response: 1081406
Conc: 20.92 ng/ml

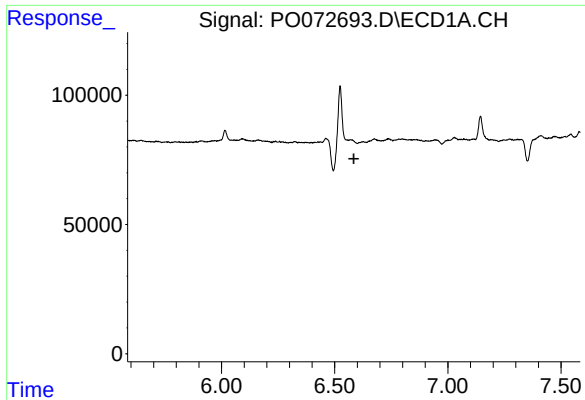

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 6.585 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

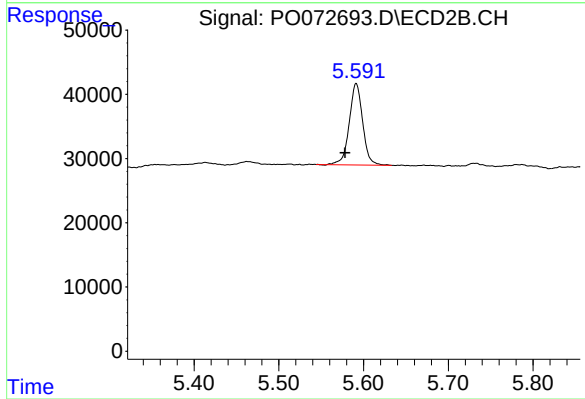


#20 AR-1242-5

R.T.: 5.591 min
Delta R.T.: 0.013 min
Response: 139295
Conc: 101.46 ng/ml

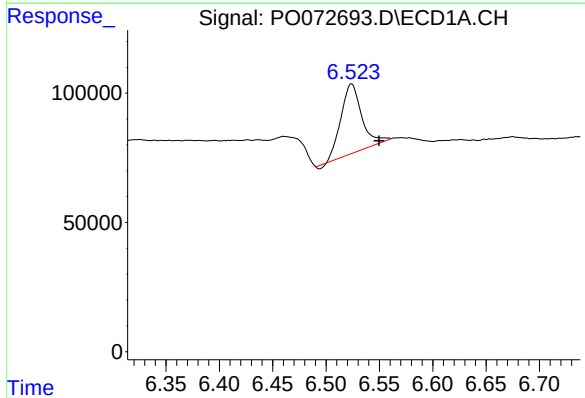


#24 AR-1248-4

R.T.: 6.524 min
Delta R.T.: -0.026 min
Response: 361031
Conc: 81.64 ng/ml

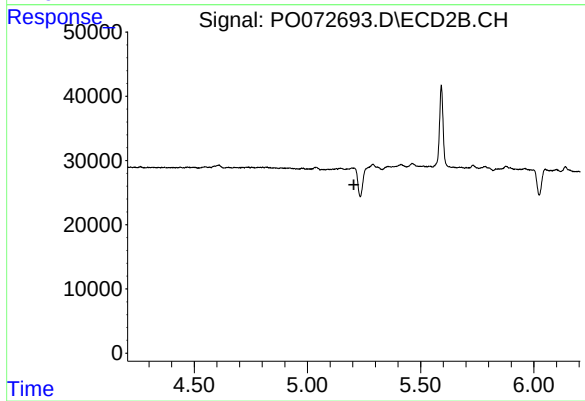

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.205 min
Response: 0
Conc: N.D.

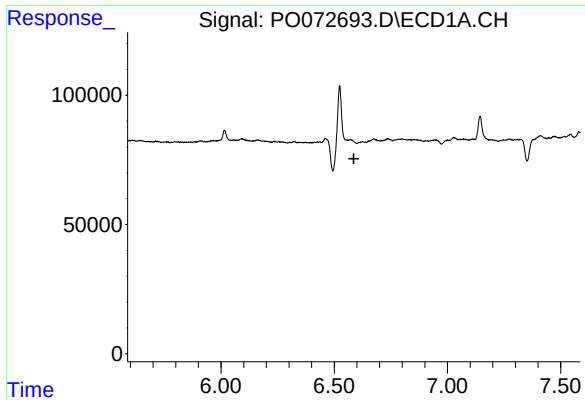

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 6.587 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

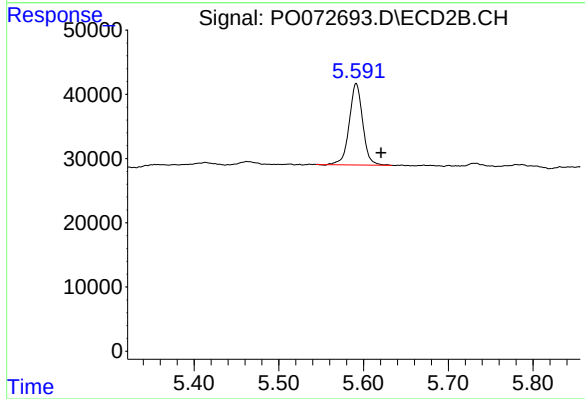


#25 AR-1248-5

R.T.: 5.591 min
Delta R.T.: -0.029 min
Response: 139295
Conc: 75.42 ng/ml

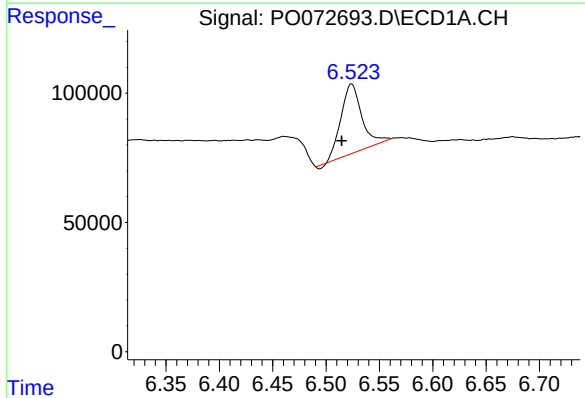


#26 AR-1254-1

R.T.: 6.524 min
Delta R.T.: 0.009 min
Response: 361031
Conc: 85.46 ng/ml

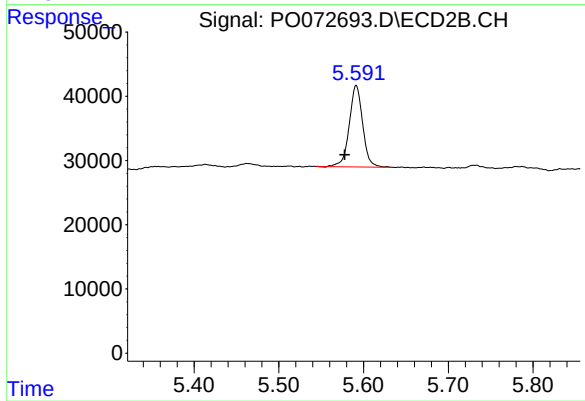

#26 AR-1254-1


R.T.: 5.591 min
Delta R.T.: 0.014 min
Response: 139295
Conc: 50.39 ng/ml

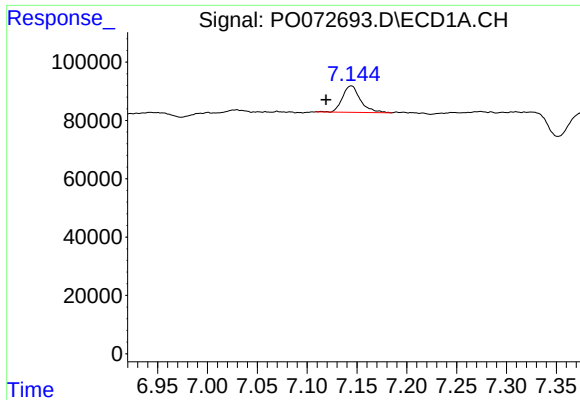

#28 AR-1254-3


R.T.: 7.144 min
Delta R.T.: 0.025 min
Response: 112772
Conc: 16.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

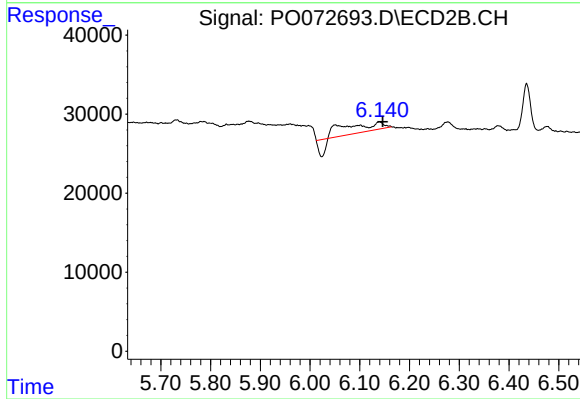


#28 AR-1254-3

R.T.: 6.140 min
Delta R.T.: -0.007 min
Response: 45216
Conc: 11.75 ng/ml

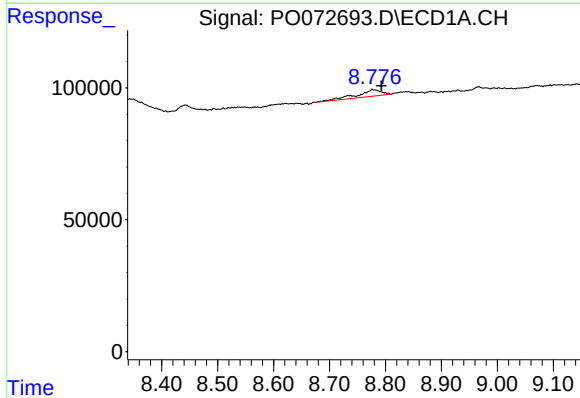


#39 AR-1262-4

R.T.: 8.777 min
Delta R.T.: -0.016 min
Response: 76089
Conc: 19.04 ng/ml

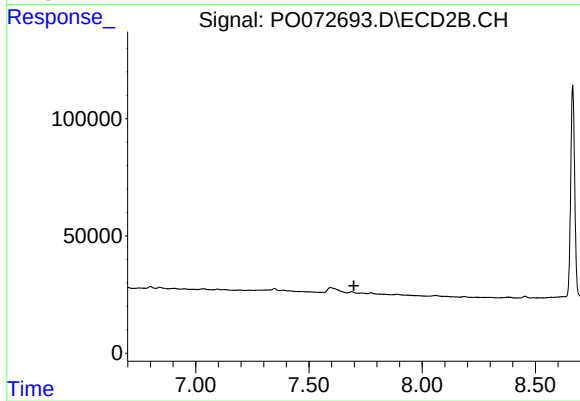

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 7.698 min
Response: 0
Conc: N.D.

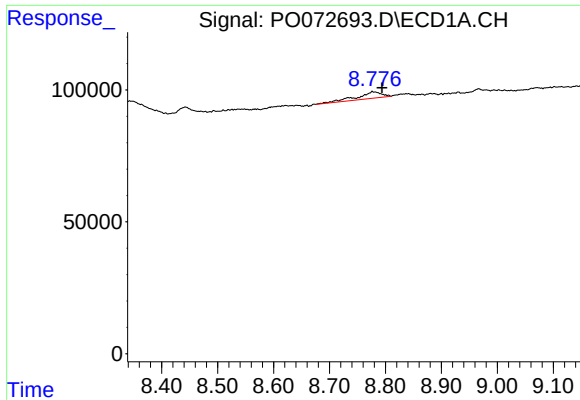

#42 AR-1268-2

R.T.: 8.777 min
Delta R.T.: -0.017 min
Response: 76089
Conc: 4.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

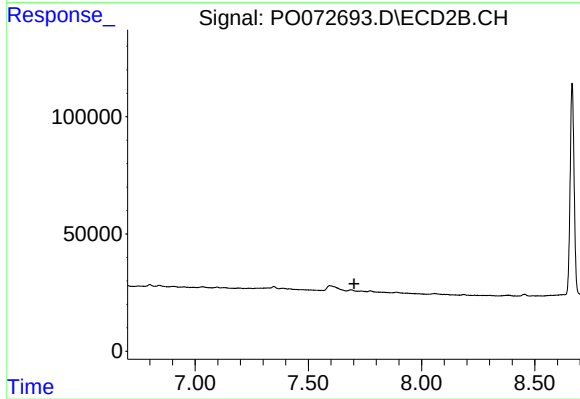

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 7.701 min
Response: 0
Conc: N.D.