

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102220\
 Data File : PO072648.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Oct 2020 10:11
 Operator : DD\AJ
 Sample : L4457-03RE
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 NOTT-AVE-PR-2150RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 05:47:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 14 17:47:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.317	3.500	3260781	1686279	38.444	40.033
2) SA Decachlor...	9.916	8.665	3671093	1560705	33.282	30.191

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102220\
Data File : P0072648.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Oct 2020 10:11
Operator : DD\AJ
Sample : L4457-03RE
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
NOTT-AVE-PR-2150RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 05:47:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 14 17:47:24 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

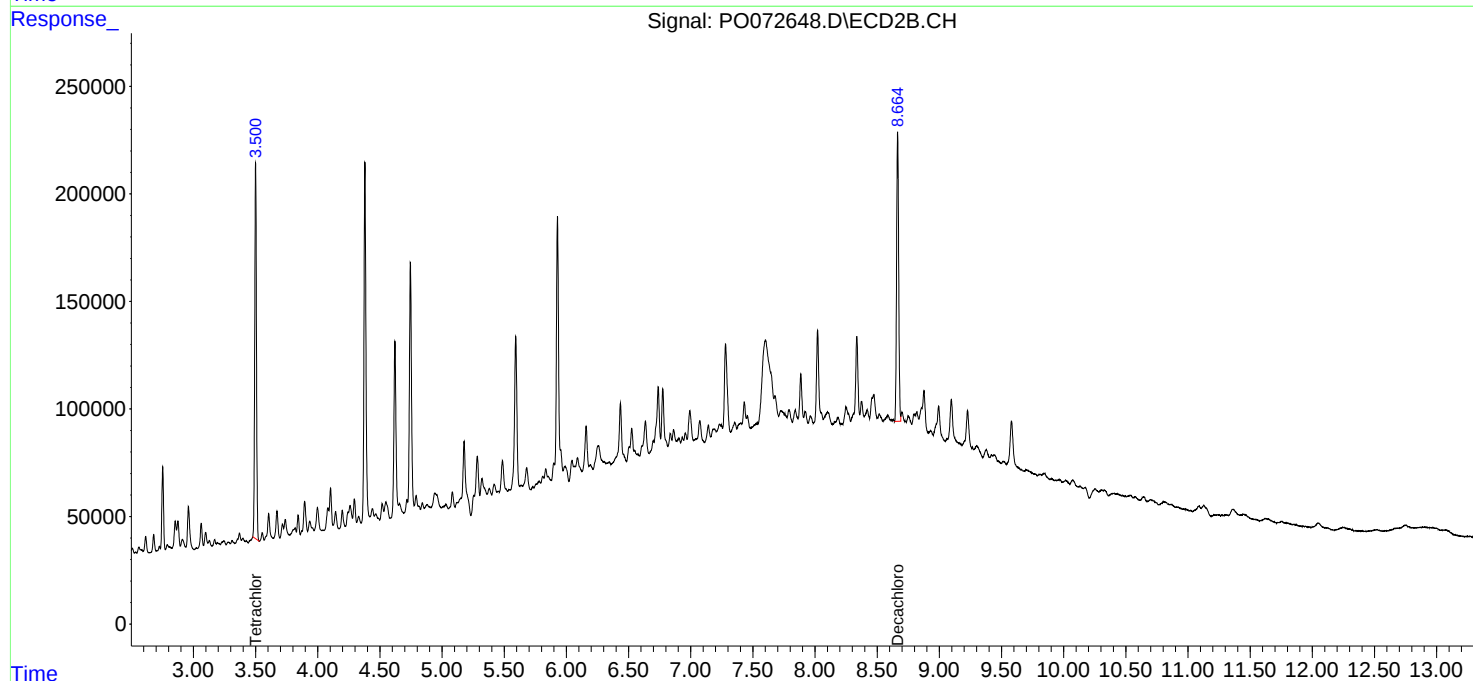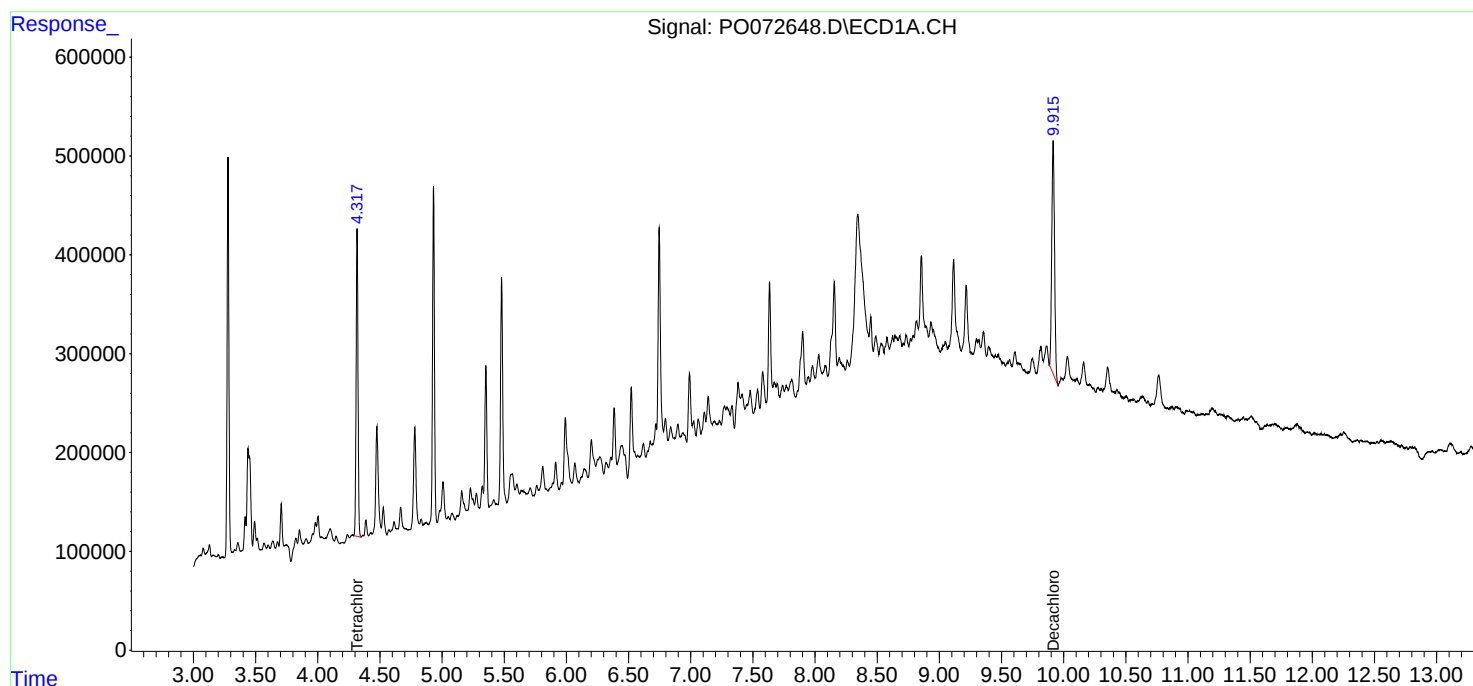


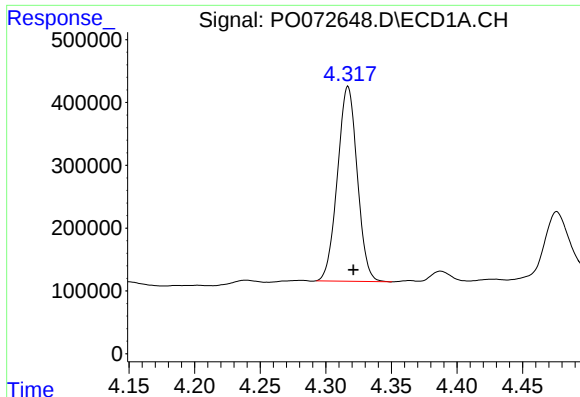

#1 Tetrachloro-m-xylene


R.T.: 4.317 min
Delta R.T.: -0.004 min
Response: 3260781
Conc: 38.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
NOTT-AVE-PR-2150RE

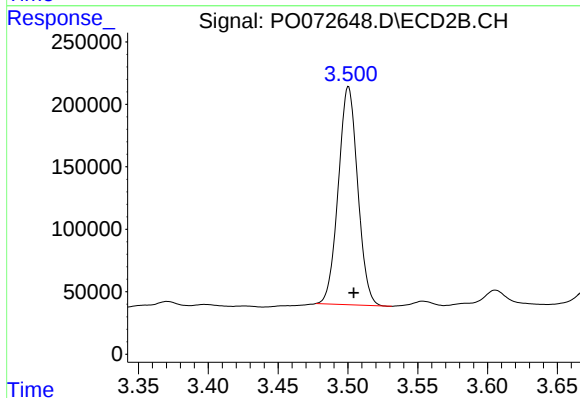


#1 Tetrachloro-m-xylene

R.T.: 3.500 min
Delta R.T.: -0.004 min
Response: 1686279
Conc: 40.03 ng/ml

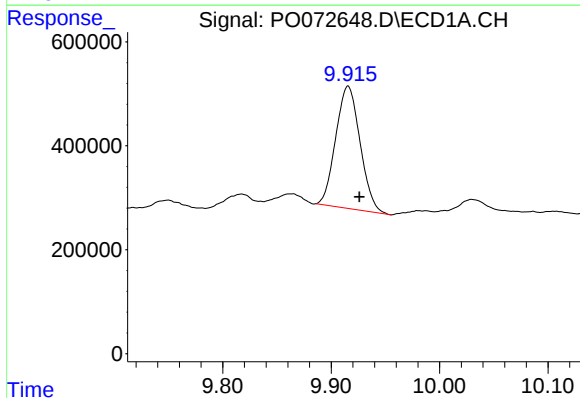

#2 Decachlorobiphenyl

R.T.: 9.916 min
Delta R.T.: -0.010 min
Response: 3671093
Conc: 33.28 ng/ml

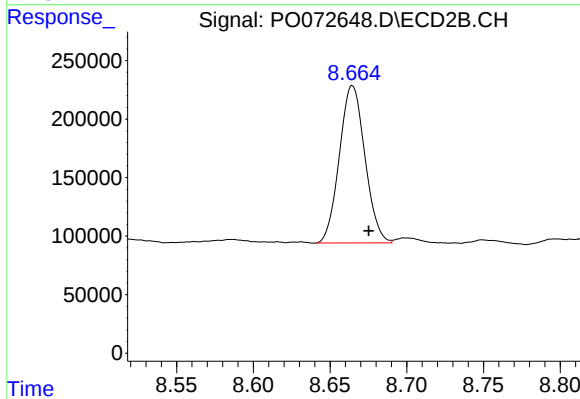

#2 Decachlorobiphenyl

R.T.: 8.665 min
Delta R.T.: -0.011 min
Response: 1560705
Conc: 30.19 ng/ml