

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102220\
 Data File : P0072649.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Oct 2020 10:28
 Operator : DD\AJ
 Sample : L4457-04RE
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ROOSEVELT-PR-2151RE

Manual Integrations
 APPROVED

mohammad
 10/26/2020 5:10:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 05:47:48 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 14 17:47:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.318	3.501	2864188	1500846	33.768	35.631m
2) SA Decachlor...	9.916	8.665	3070876	1250155	27.840	24.183

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102220\
Data File : PO072649.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Oct 2020 10:28
Operator : DD\AJ
Sample : L4457-04RE
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
ROOSEVELT-PR-2151RE


Manual Integrations
APPROVED

mohammad
10/26/2020 5:10:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 05:47:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 14 17:47:24 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

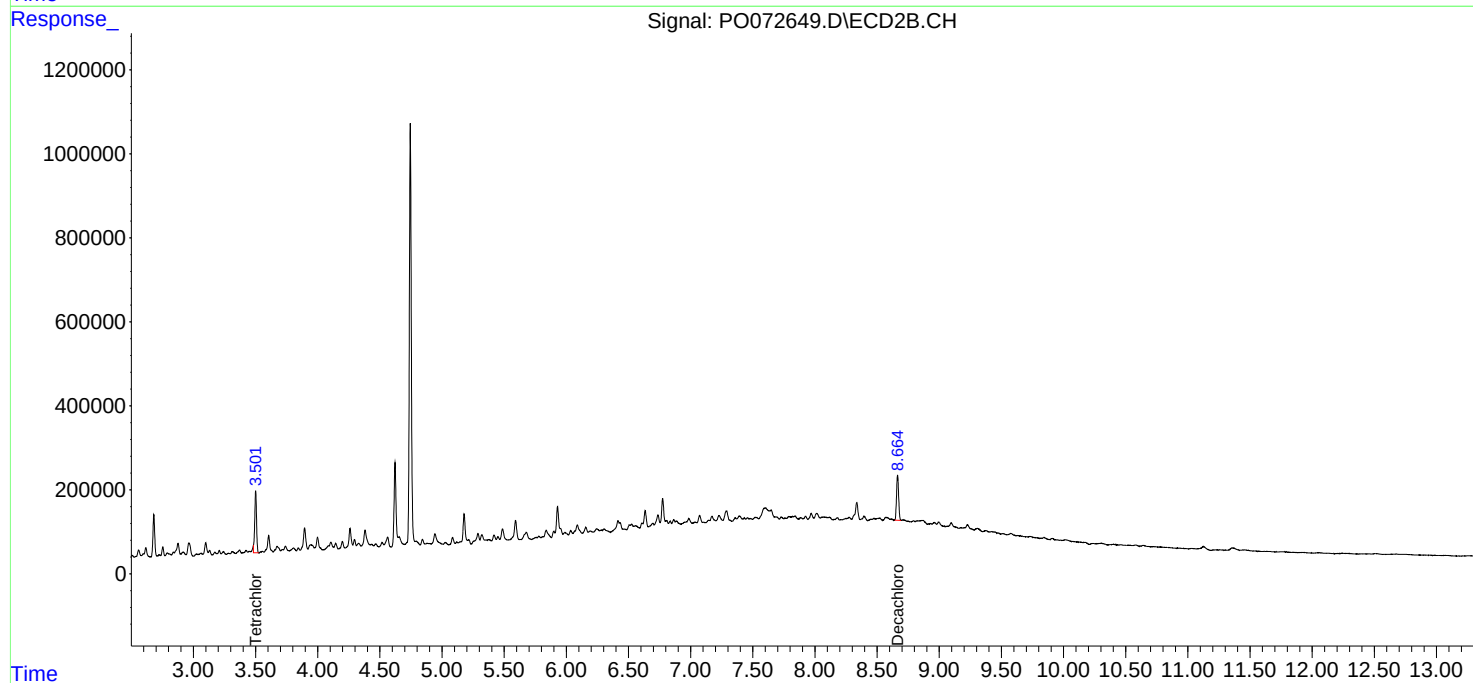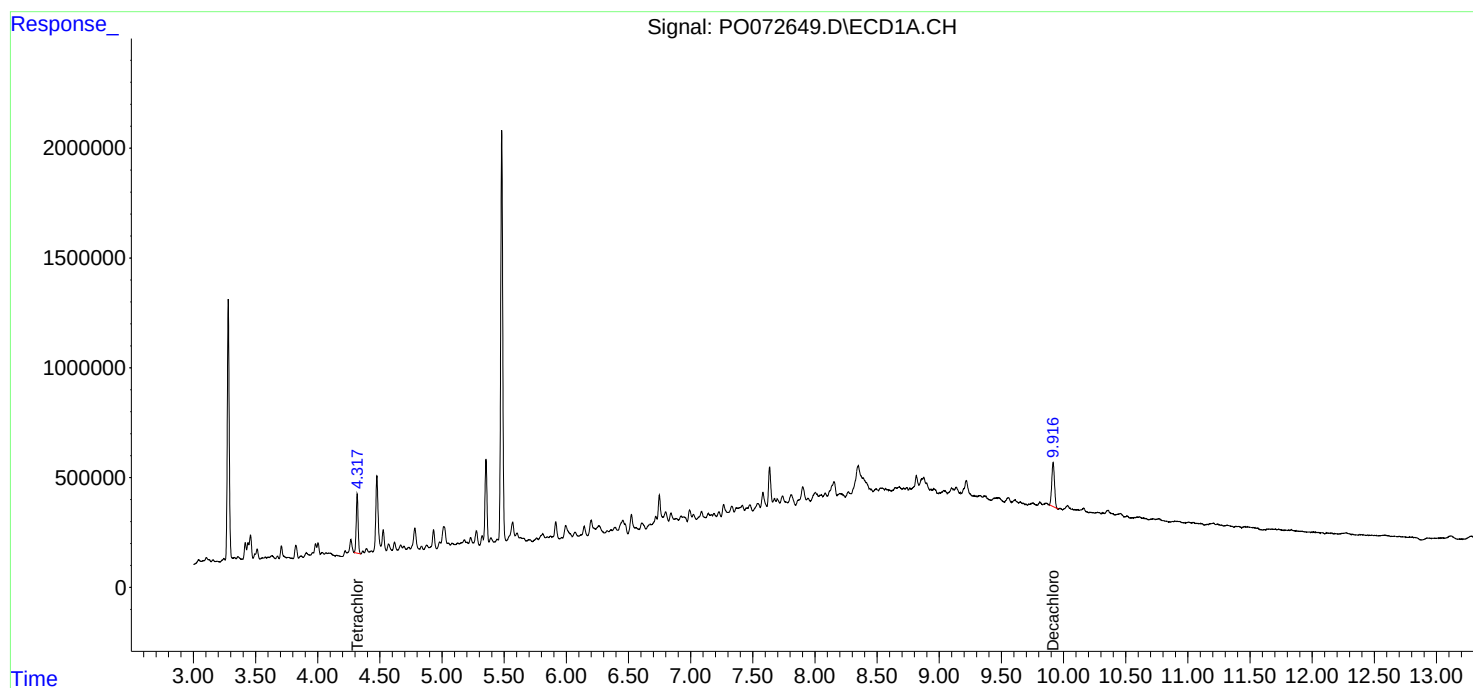

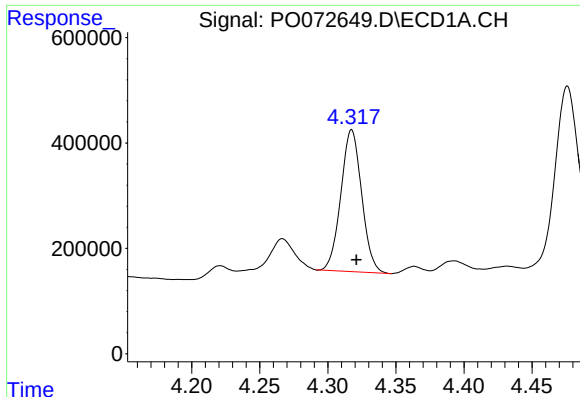


#1 Tetrachloro-m-xylene

R.T.: 4.318 min
Delta R.T.: -0.003 min
Response: 2864188
Conc: 33.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
ROOSEVELT-PR-2151RE


Manual Integrations
APPROVED

mohammad
10/26/2020 5:10:25 PM

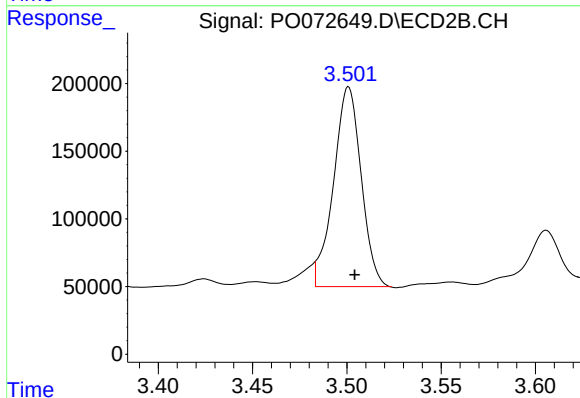


#1 Tetrachloro-m-xylene

R.T.: 3.501 min
Delta R.T.: -0.004 min
Response: 1500846
Conc: 35.63 ng/ml m

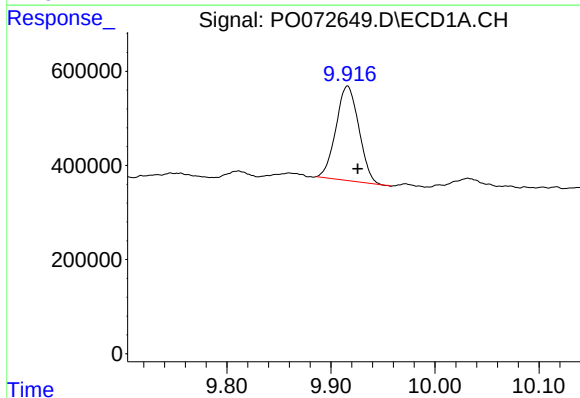

#2 Decachlorobiphenyl

R.T.: 9.916 min
Delta R.T.: -0.010 min
Response: 3070876
Conc: 27.84 ng/ml

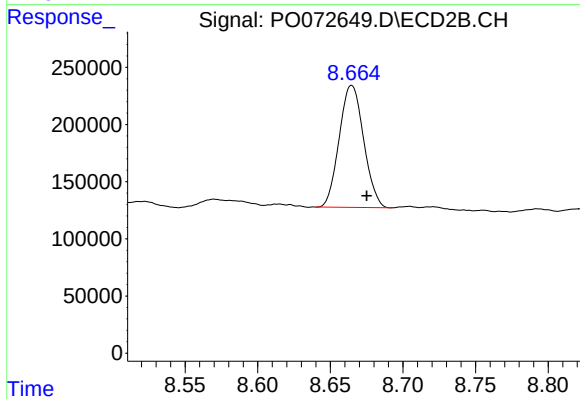

#2 Decachlorobiphenyl

R.T.: 8.665 min
Delta R.T.: -0.010 min
Response: 1250155
Conc: 24.18 ng/ml