

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102220\
 Data File : P0072672.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Oct 2020 19:47
 Operator : DD\AJ
 Sample : L4214-07
 Misc : AR1254 LOD 25 PPB
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2020

Manual Integrations
 APPROVED

mohammad
 10/26/2020 5:11:21 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 05:57:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 14 17:47:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.318	3.502	1354346	705622	15.968	16.752
2) SA Decachlor...	9.917	8.665	1664428	888214	15.089m	17.182
Target Compounds						
26) L6 AR-1254-1	6.510	5.571	141535	95121	33.504	34.412
27) L6 AR-1254-2	6.737	5.732	230002	90966	35.489	37.415
28) L6 AR-1254-3	7.113	6.140	215342	140554	31.683	36.526
29) L6 AR-1254-4	7.408	6.380	227053	72180	34.255	26.880
30) L6 AR-1254-5	7.829	6.800	365239	198770	57.018	54.239

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102220\
Data File : PO072672.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Oct 2020 19:47
Operator : DD\AJ
Sample : L4214-07
Misc : AR1254 LOD 25 PPB
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020


Manual Integrations
APPROVED

mohammad
10/26/2020 5:11:21 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 05:57:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 14 17:47:24 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

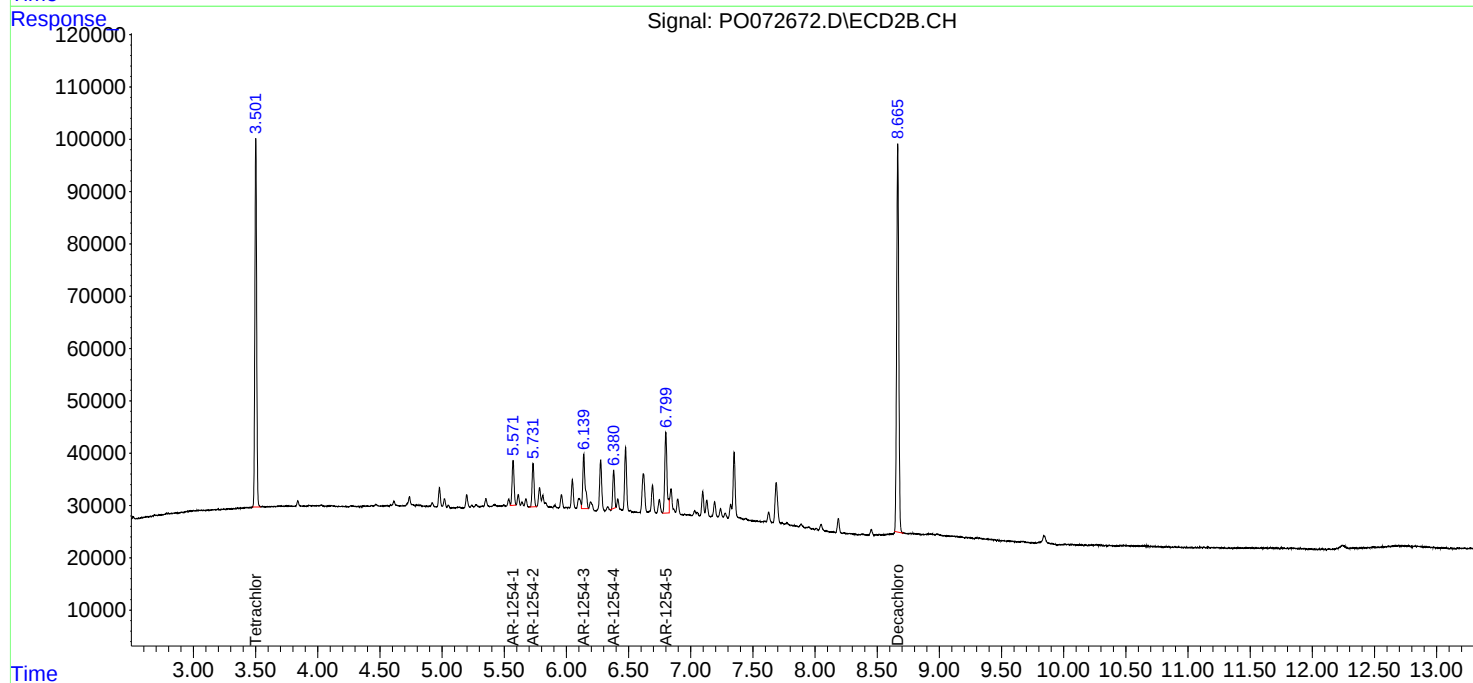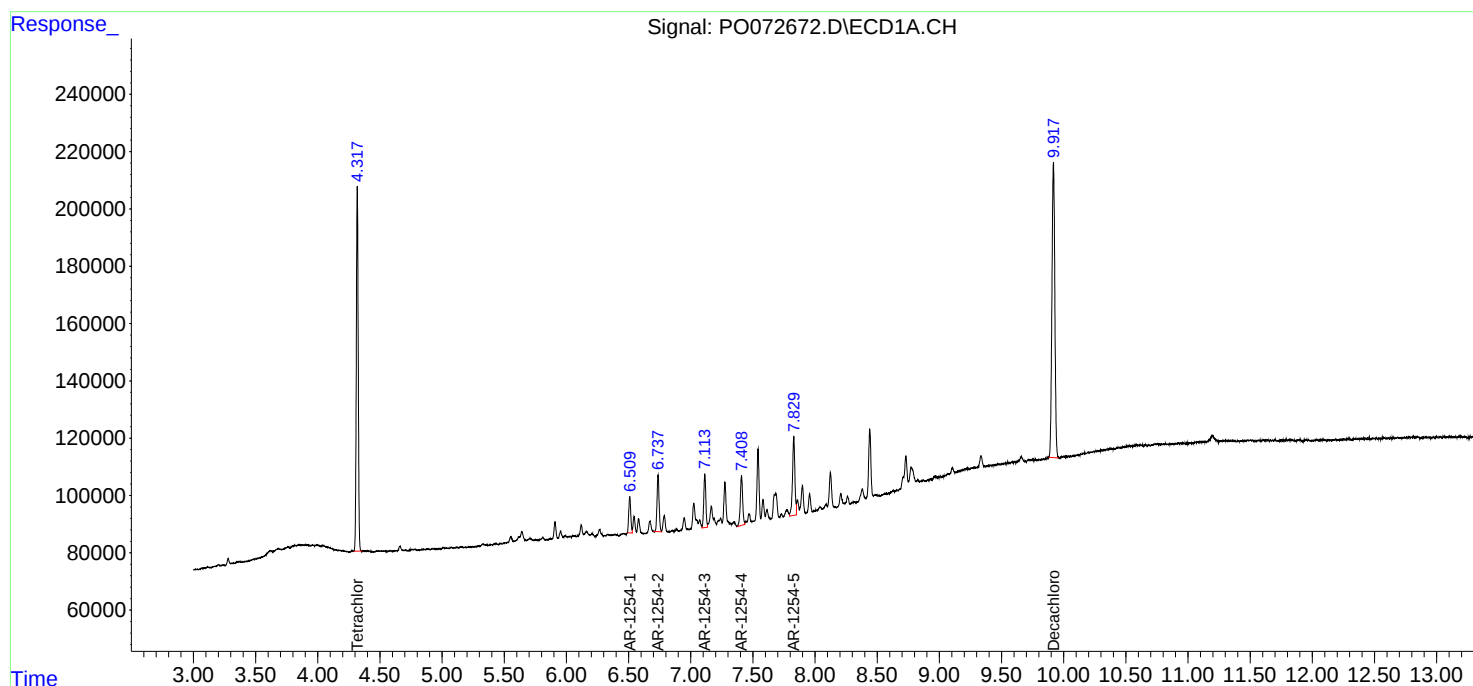

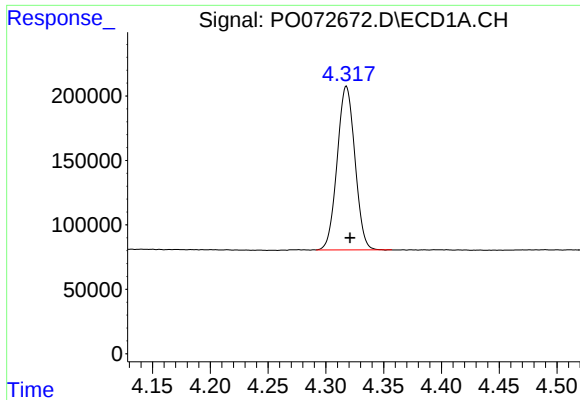


#1 Tetrachloro-m-xylene

R.T.: 4.318 min
Delta R.T.: -0.003 min
Response: 1354346
Conc: 15.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020


Manual Integrations
APPROVED

mohammad
10/26/2020 5:11:21 PM

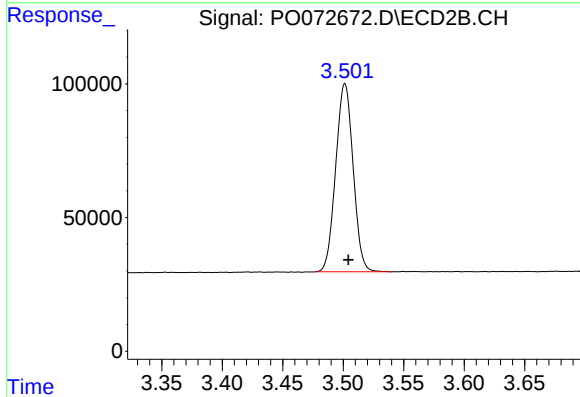


#1 Tetrachloro-m-xylene

R.T.: 3.502 min
Delta R.T.: -0.003 min
Response: 705622
Conc: 16.75 ng/ml

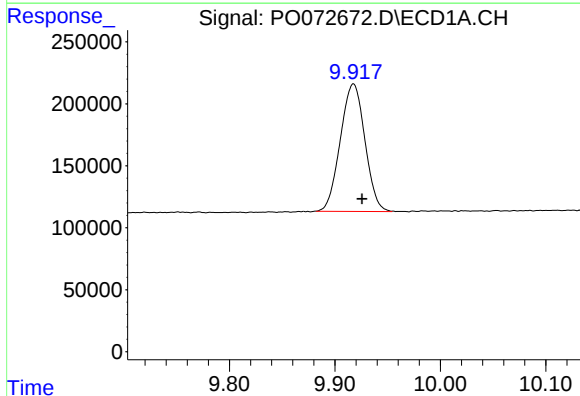


#2 Decachlorobiphenyl

R.T.: 9.917 min
Delta R.T.: -0.009 min
Response: 1664428
Conc: 15.09 ng/ml m

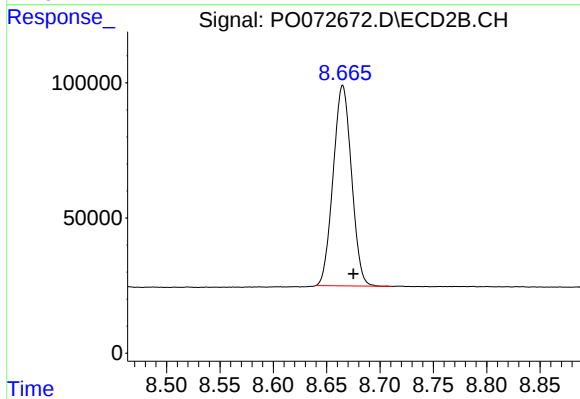

#2 Decachlorobiphenyl

R.T.: 8.665 min
Delta R.T.: -0.010 min
Response: 888214
Conc: 17.18 ng/ml

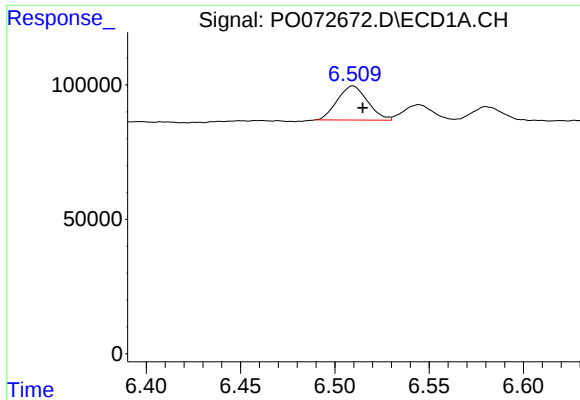


#26 AR-1254-1

R.T.: 6.510 min
Delta R.T.: -0.005 min
Response: 141535
Conc: 33.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020


Manual Integrations
APPROVED

mohammad
10/26/2020 5:11:21 PM

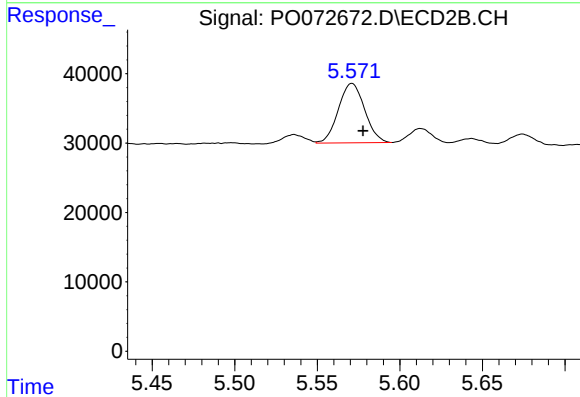


#26 AR-1254-1

R.T.: 5.571 min
Delta R.T.: -0.007 min
Response: 95121
Conc: 34.41 ng/ml

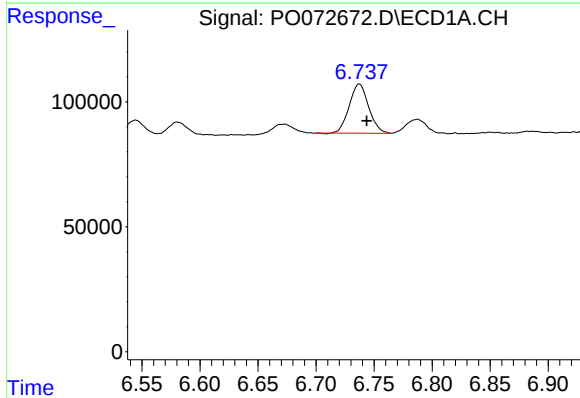


#27 AR-1254-2

R.T.: 6.737 min
Delta R.T.: -0.006 min
Response: 230002
Conc: 35.49 ng/ml

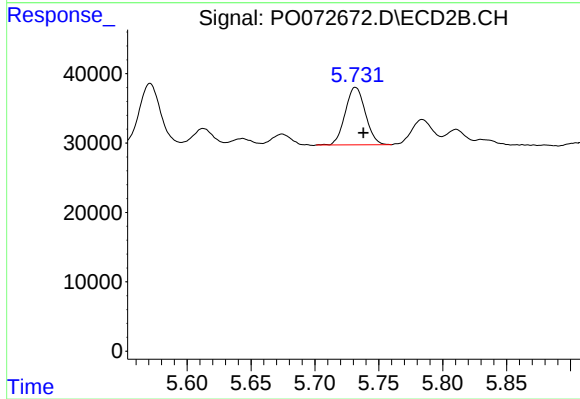

#27 AR-1254-2

R.T.: 5.732 min
Delta R.T.: -0.006 min
Response: 90966
Conc: 37.42 ng/ml

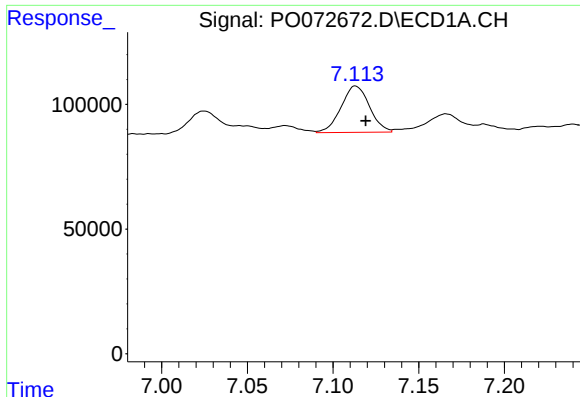


#28 AR-1254-3

R.T.: 7.113 min
Delta R.T.: -0.006 min
Response: 215342
Conc: 31.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020


Manual Integrations
APPROVED

mohammad
10/26/2020 5:11:21 PM

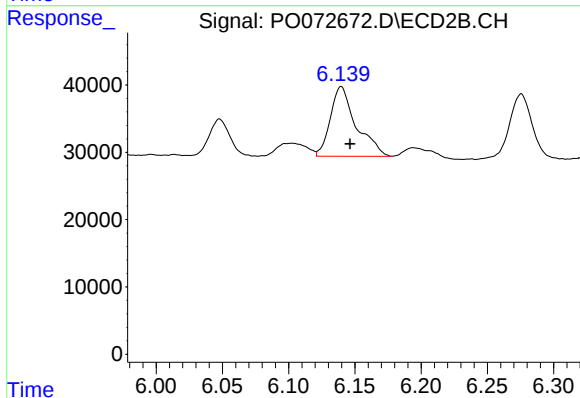


#28 AR-1254-3

R.T.: 6.140 min
Delta R.T.: -0.007 min
Response: 140554
Conc: 36.53 ng/ml

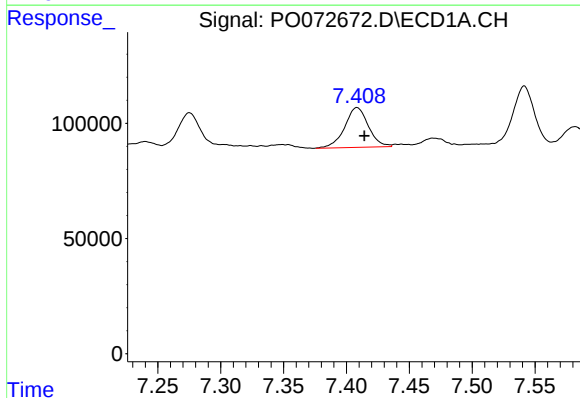


#29 AR-1254-4

R.T.: 7.408 min
Delta R.T.: -0.006 min
Response: 227053
Conc: 34.26 ng/ml

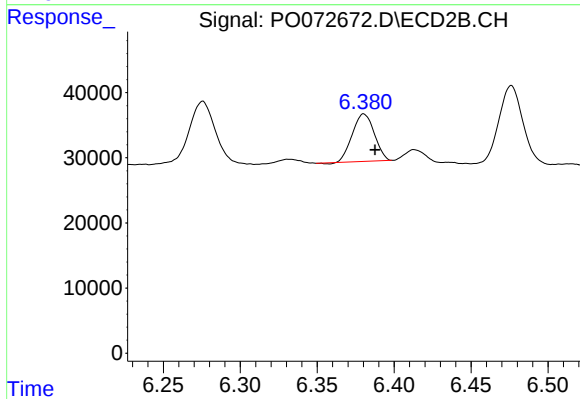

#29 AR-1254-4

R.T.: 6.380 min
Delta R.T.: -0.007 min
Response: 72180
Conc: 26.88 ng/ml

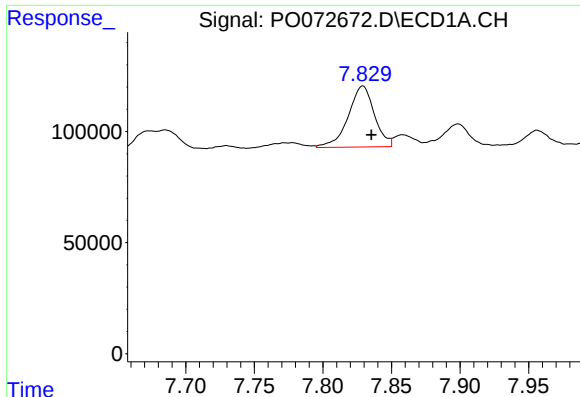


#30 AR-1254-5

R.T.: 7.829 min
Delta R.T.: -0.006 min
Response: 365239
Conc: 57.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

Manual Integrations
APPROVED

mohammad
10/26/2020 5:11:21 PM

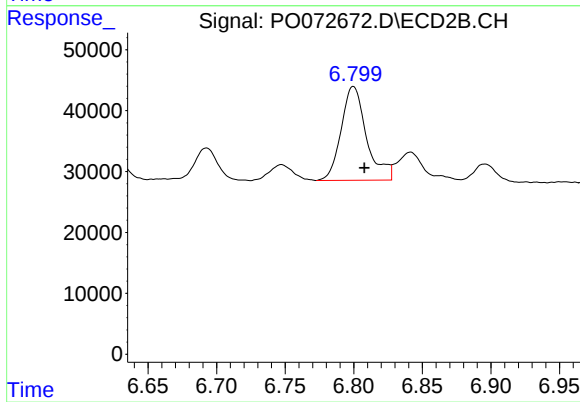

#30 AR-1254-5

R.T.: 6.800 min
Delta R.T.: -0.008 min
Response: 198770
Conc: 54.24 ng/ml