

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102220\
 Data File : P0072680.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Oct 2020 22:04
 Operator : DD\AJ
 Sample : L4479-01
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 10-21A

Manual Integrations
 APPROVED

mohammad
 10/26/2020 5:11:50 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 06:00:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 14 17:47:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.319	3.503	1709035	1065135	20.149m	25.287 #
2)	SA Decachlor...	9.919	8.666	1873554	1022054	16.985	19.771

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102220\
Data File : PO072680.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Oct 2020 22:04
Operator : DD\AJ
Sample : L4479-01
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
10-21A


Manual Integrations
APPROVED

mohammad
10/26/2020 5:11:50 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 06:00:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 14 17:47:24 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

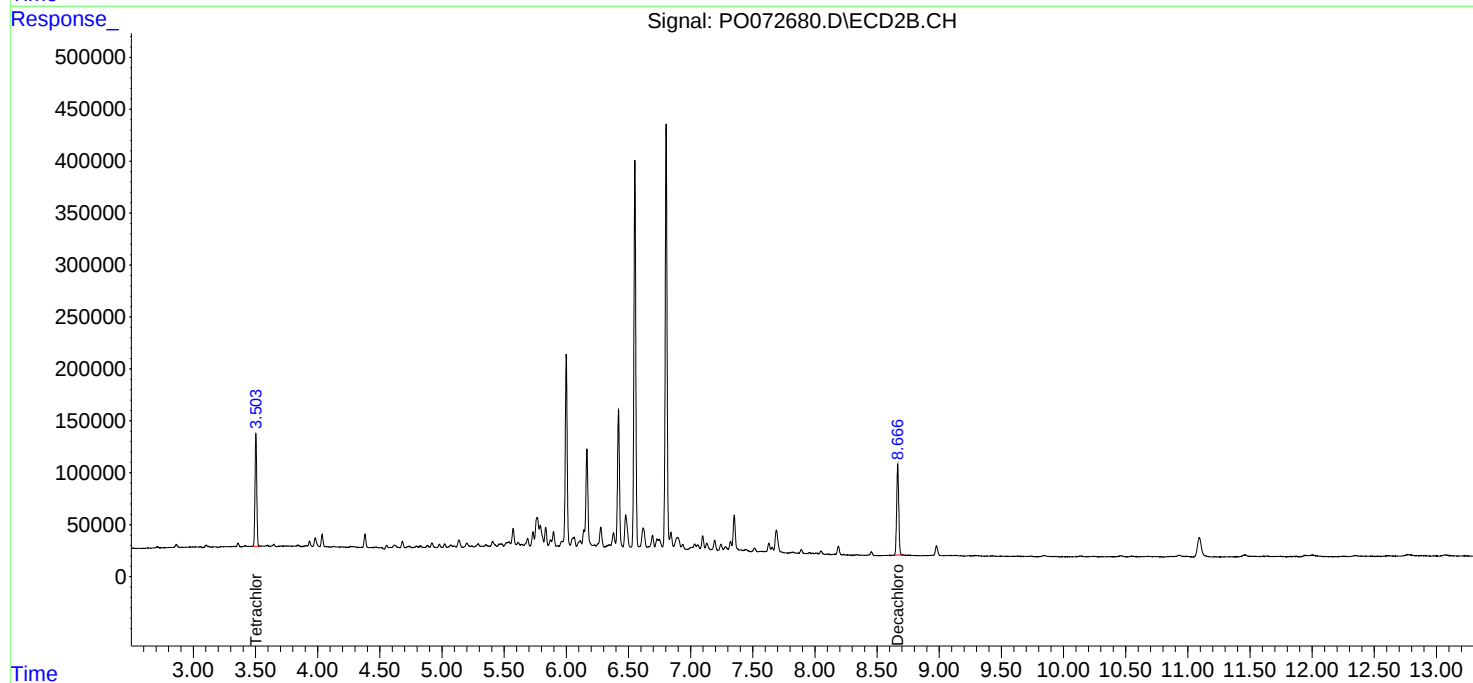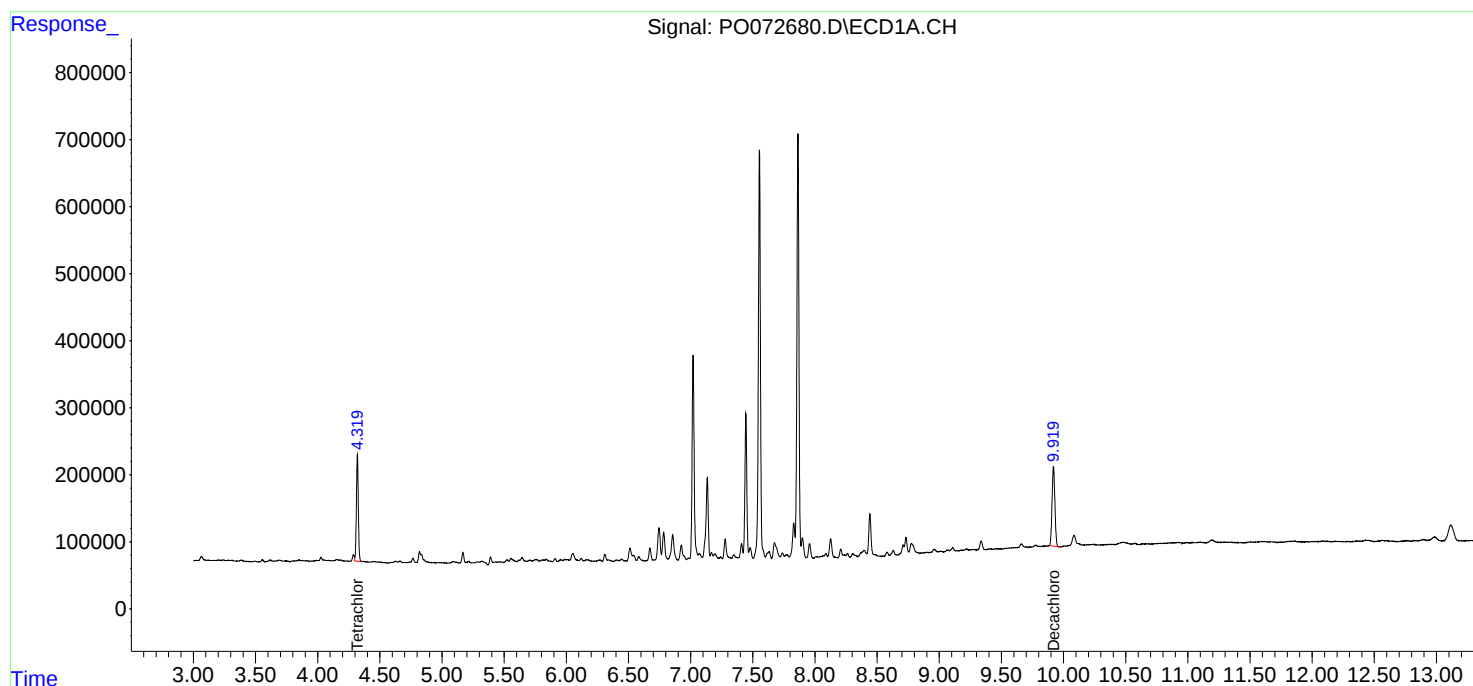

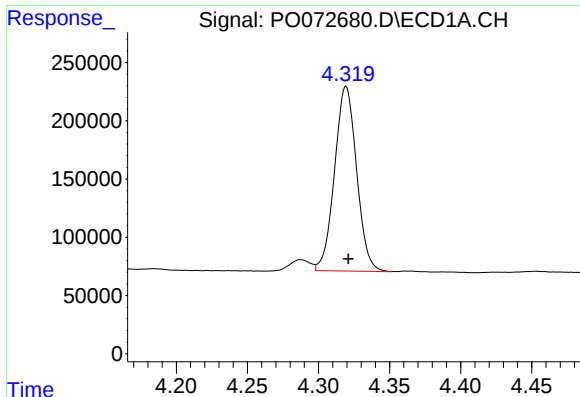


#1 Tetrachloro-m-xylene

R.T.: 4.319 min
Delta R.T.: -0.002 min
Response: 1709035
Conc: 20.15 ng/ml m

Instrument :
ECD_O
ClientSampleId :
10-21A


Manual Integrations
APPROVED

mohammad
10/26/2020 5:11:50 PM

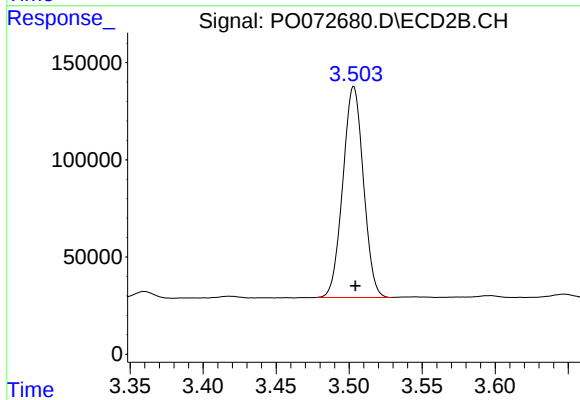


#1 Tetrachloro-m-xylene

R.T.: 3.503 min
Delta R.T.: -0.001 min
Response: 1065135
Conc: 25.29 ng/ml

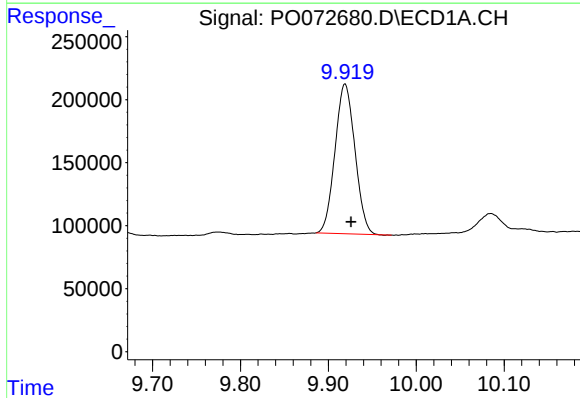

#2 Decachlorobiphenyl

R.T.: 9.919 min
Delta R.T.: -0.007 min
Response: 1873554
Conc: 16.99 ng/ml

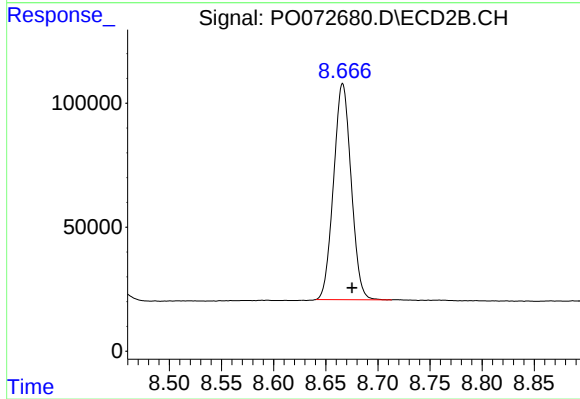

#2 Decachlorobiphenyl

R.T.: 8.666 min
Delta R.T.: -0.009 min
Response: 1022054
Conc: 19.77 ng/ml