

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102220\
 Data File : P0072698.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Oct 2020 3:12
 Operator : DD\AJ
 Sample : L4225-10
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SU-02-102120

Manual Integrations
 APPROVED

mohammad
 10/26/2020 5:12:13 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 06:08:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 14 17:47:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.318	3.502	2168533	1143084	25.567m	27.137
2) SA Decachlor...	9.918	8.665	2196298	1096570	19.911m	21.212

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102220\
Data File : PO072698.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Oct 2020 3:12
Operator : DD\AJ
Sample : L4225-10
Misc :
ALS Vial : 51 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SU-02-102120


Manual Integrations
APPROVED

mohammad
10/26/2020 5:12:13 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 06:08:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 14 17:47:24 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

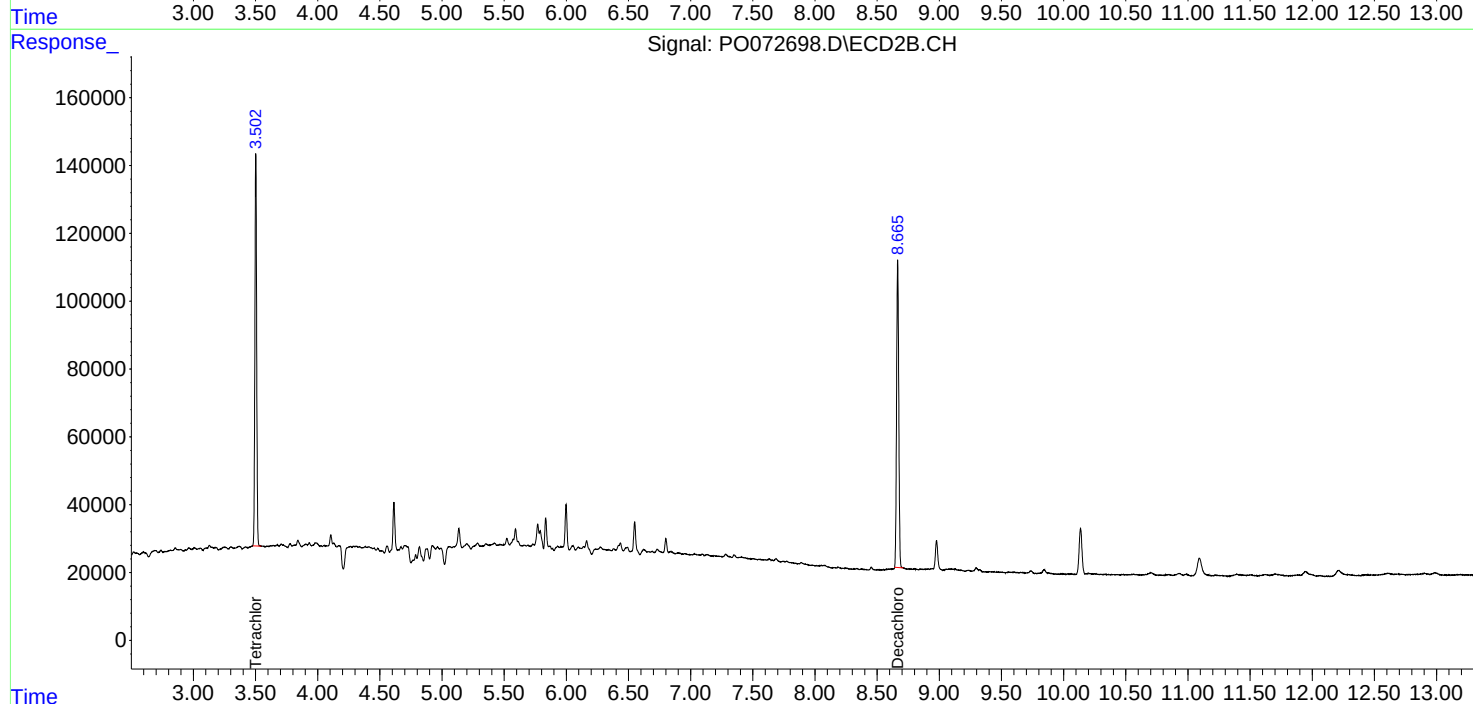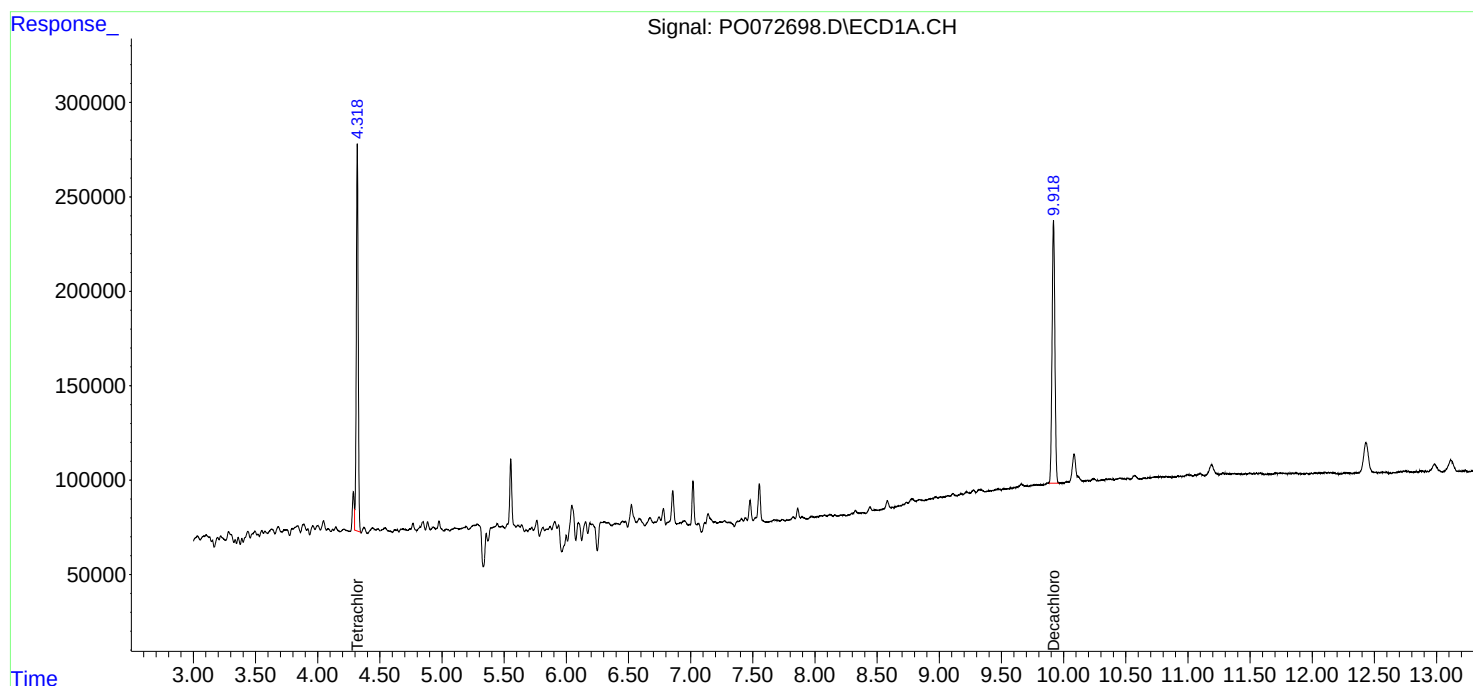

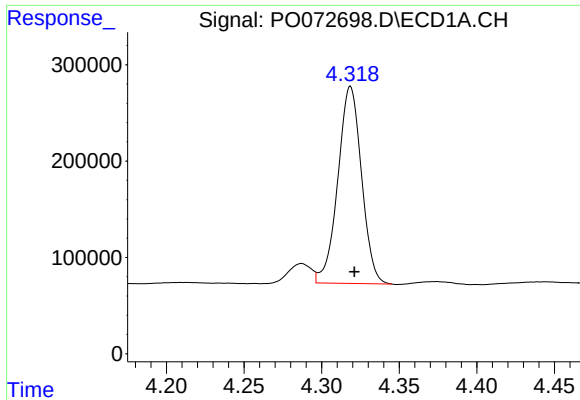


#1 Tetrachloro-m-xylene

R.T.: 4.318 min
Delta R.T.: -0.003 min
Response: 2168533
Conc: 25.57 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SU-02-102120


Manual Integrations
APPROVED

mohammad
10/26/2020 5:12:13 PM

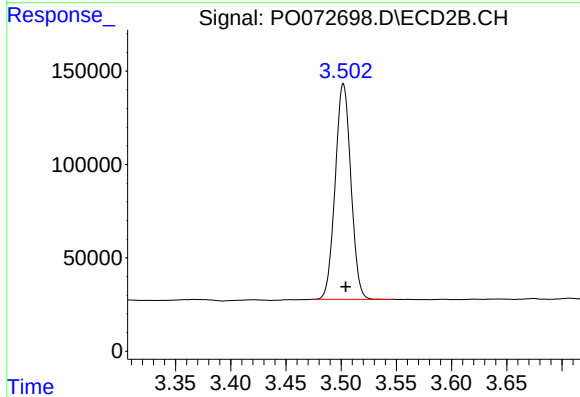


#1 Tetrachloro-m-xylene

R.T.: 3.502 min
Delta R.T.: -0.002 min
Response: 1143084
Conc: 27.14 ng/ml

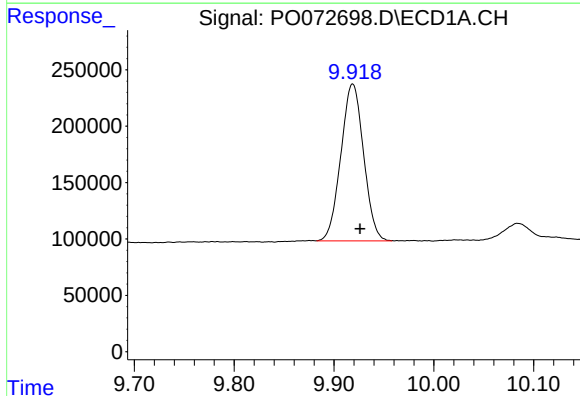

#2 Decachlorobiphenyl

R.T.: 9.918 min
Delta R.T.: -0.008 min
Response: 2196298
Conc: 19.91 ng/ml m

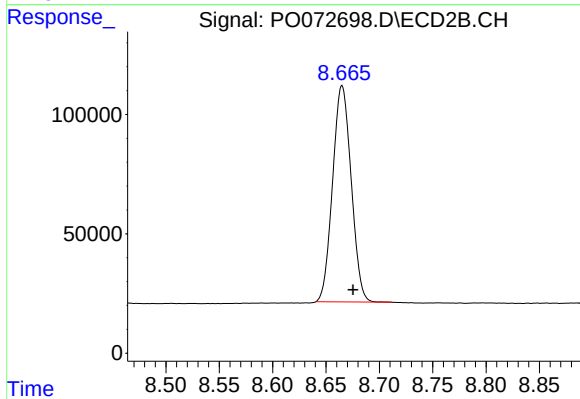

#2 Decachlorobiphenyl

R.T.: 8.665 min
Delta R.T.: -0.010 min
Response: 1096570
Conc: 21.21 ng/ml