

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102221\
 Data File : PO082110.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Oct 2021 15:21
 Operator : AJ\MA
 Sample : M4312-04 10X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 5261

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 18:08:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 19 04:37:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.981	3.975	40655	26192	0.503	0.888 #
2) SA Decachlor...	11.101	9.295	83883	57174	1.509m	2.245m#

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102221\
Data File : PO082110.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Oct 2021 15:21
Operator : AJ\MA
Sample : M4312-04 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
5261

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 18:08:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 19 04:37:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

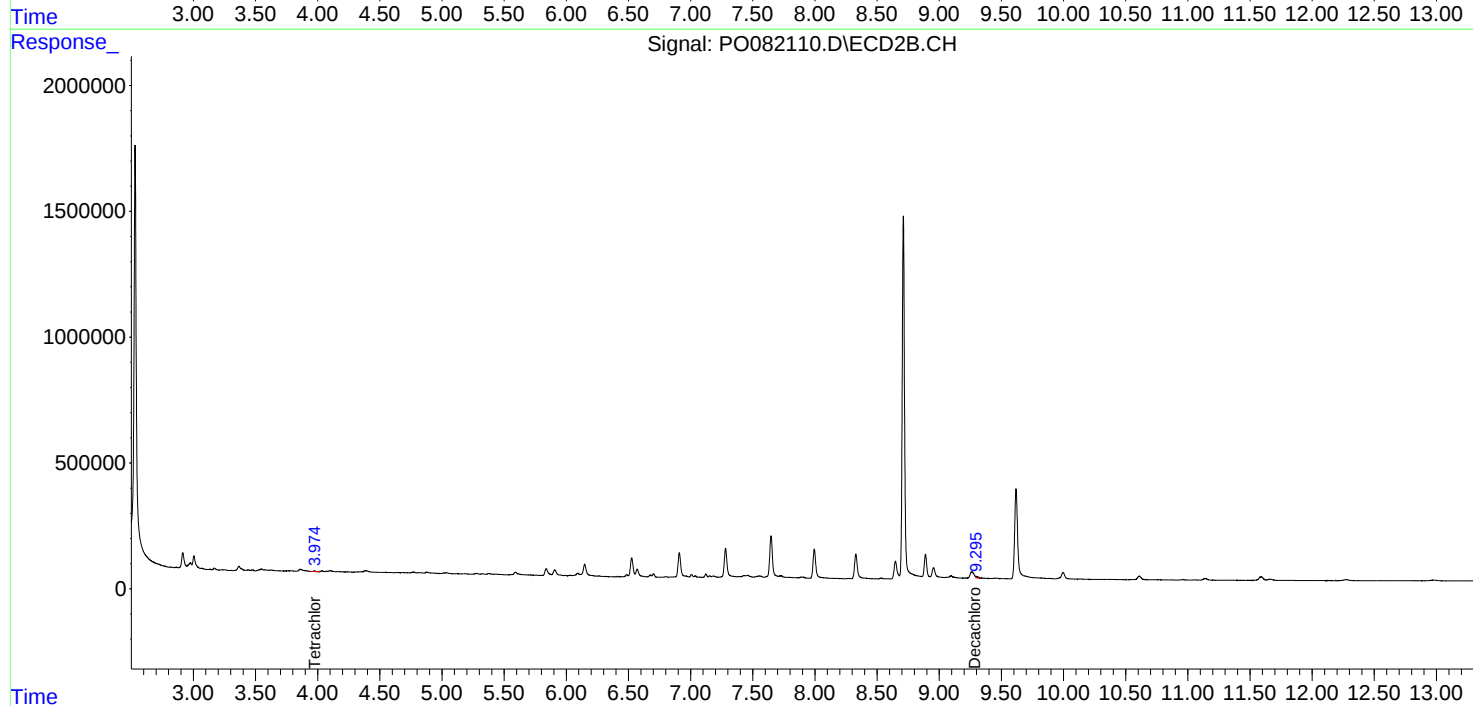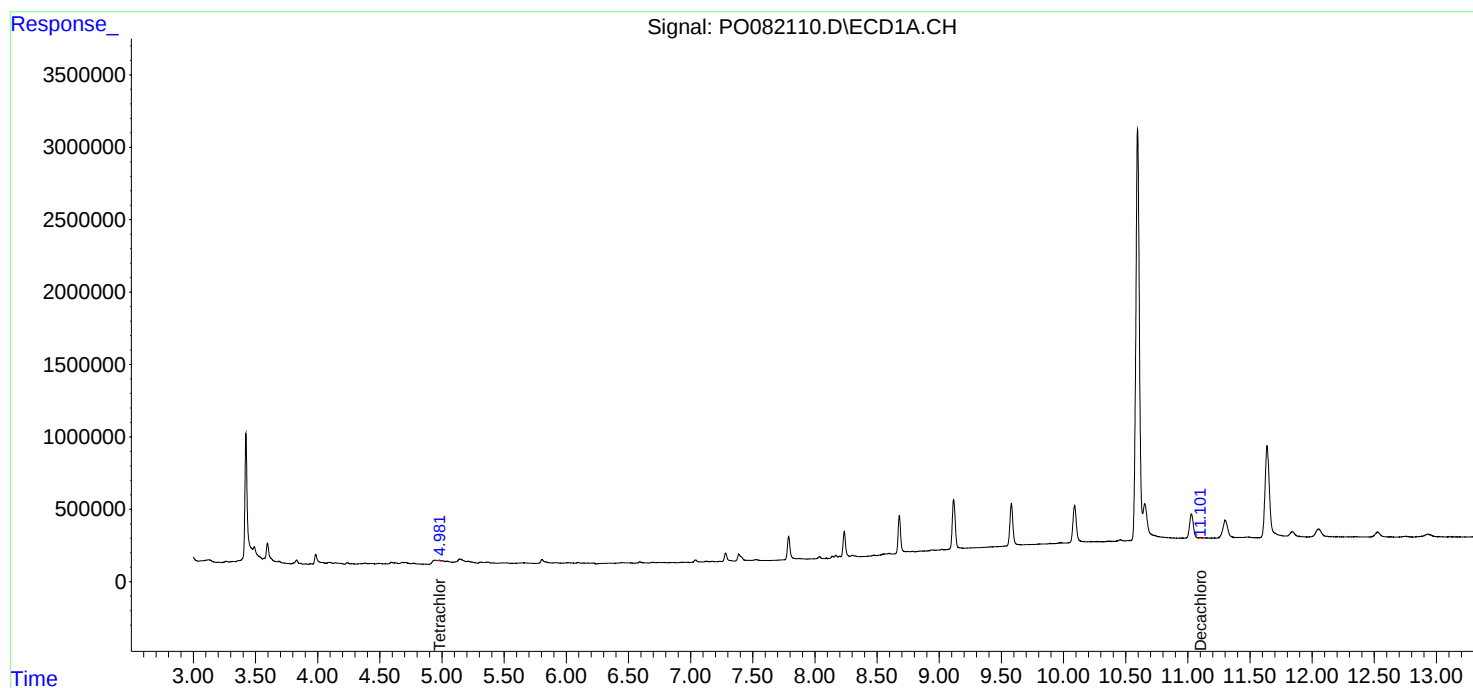


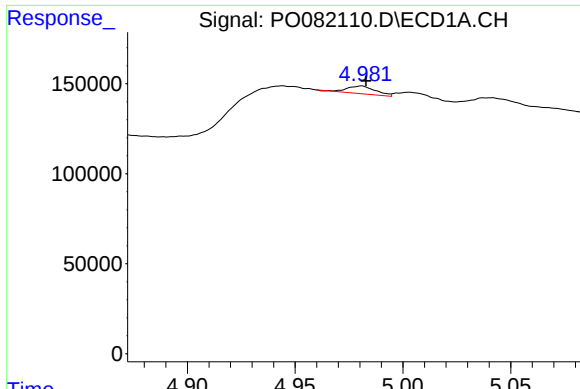

#1 Tetrachloro-m-xylene

R.T.: 4.981 min
Delta R.T.: -0.002 min
Response: 40655
Conc: 0.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
5261

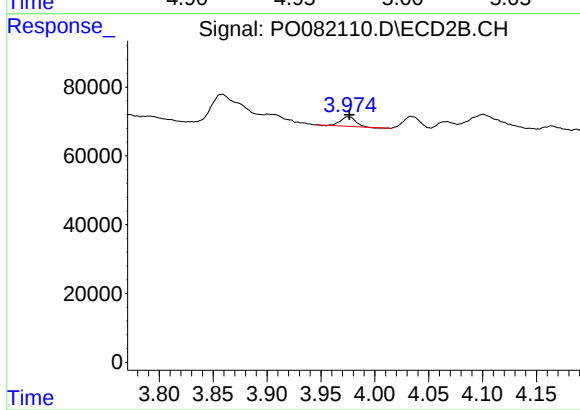

#1 Tetrachloro-m-xylene

R.T.: 3.975 min
Delta R.T.: -0.002 min
Response: 26192
Conc: 0.89 ng/ml

#2 Decachlorobiphenyl

R.T.: 11.101 min
Delta R.T.: 0.000 min
Response: 83883
Conc: 1.51 ng/ml m

#2 Decachlorobiphenyl

R.T.: 9.295 min
Delta R.T.: -0.011 min
Response: 57174
Conc: 2.24 ng/ml m