

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102221\
 Data File : PO082111.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Oct 2021 15:56
 Operator : AJ\MA
 Sample : M4312-05 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 comp

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 18:09:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 19 04:37:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.983	3.975	32569	18908	0.403m	0.641m#
2) SA Decachlor...	11.099	9.314	33010	17881	0.594	0.702m

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102221\
Data File : P0082111.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Oct 2021 15:56
Operator : AJ\MA
Sample : M4312-05 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
comp

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 18:09:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 19 04:37:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

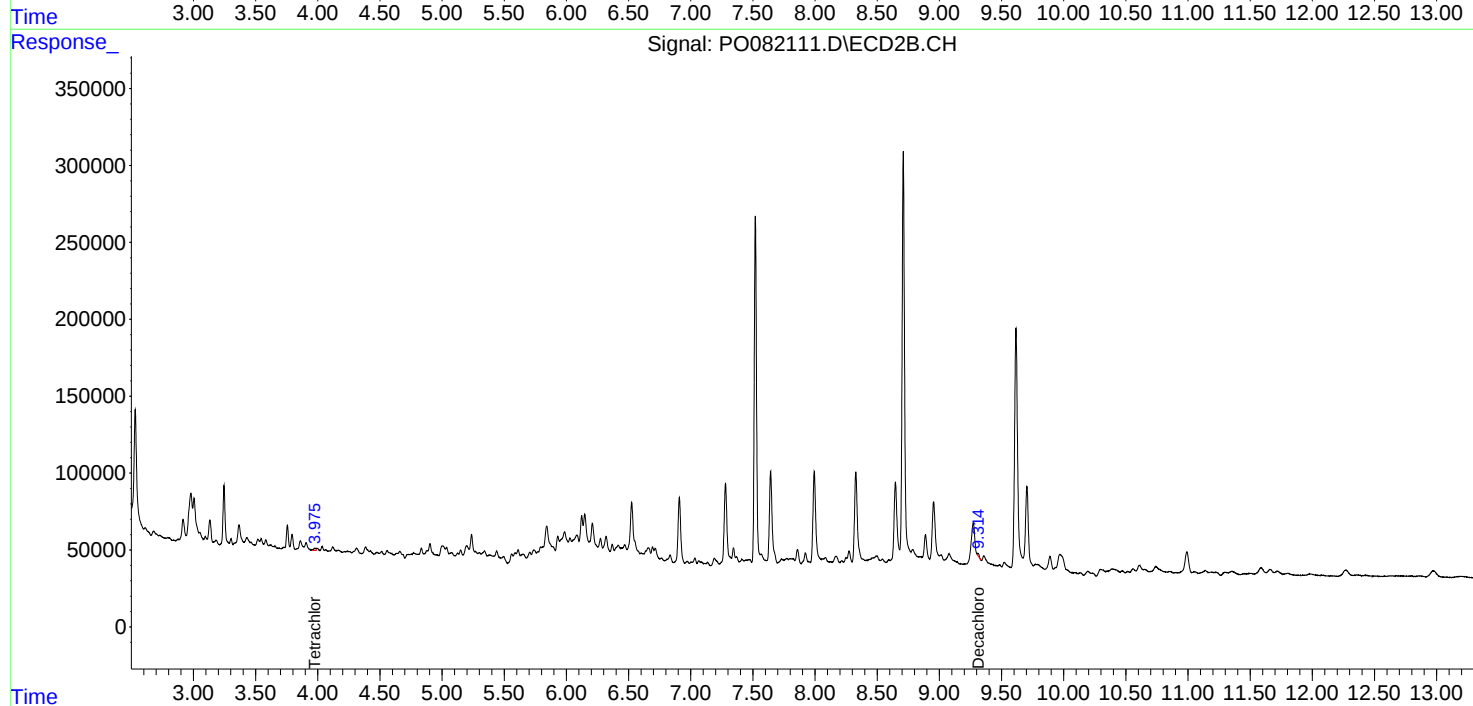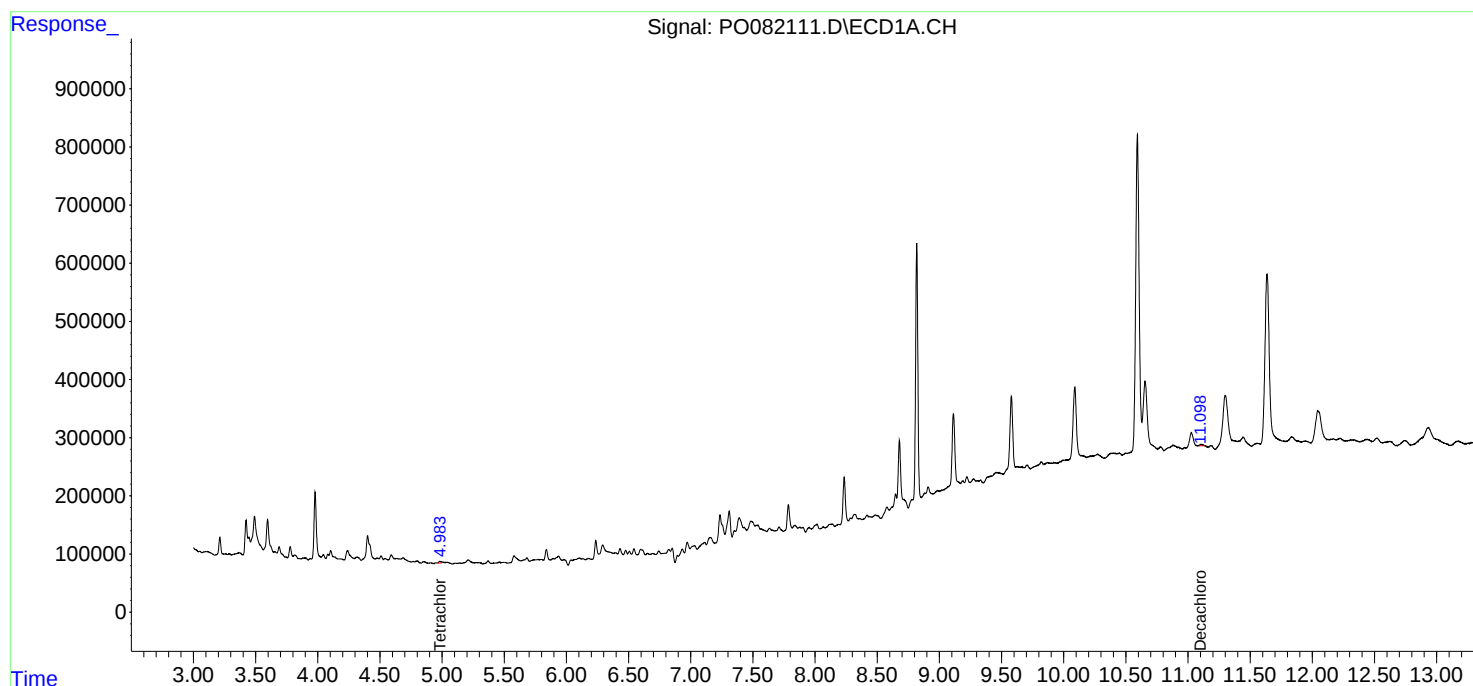


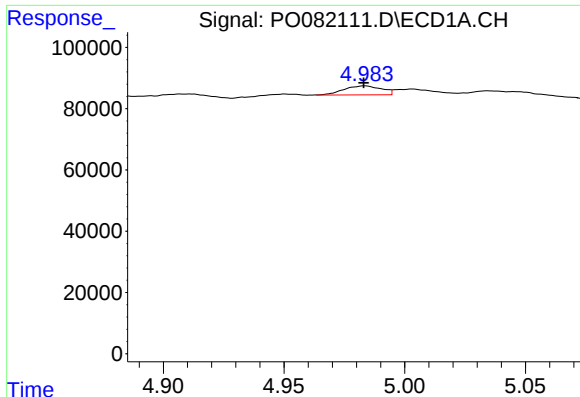

#1 Tetrachloro-m-xylene


R.T.: 4.983 min
Delta R.T.: 0.000 min
Response: 32569
Conc: 0.40 ng/ml m

Instrument :
ECD_O
ClientSampleId :
comp

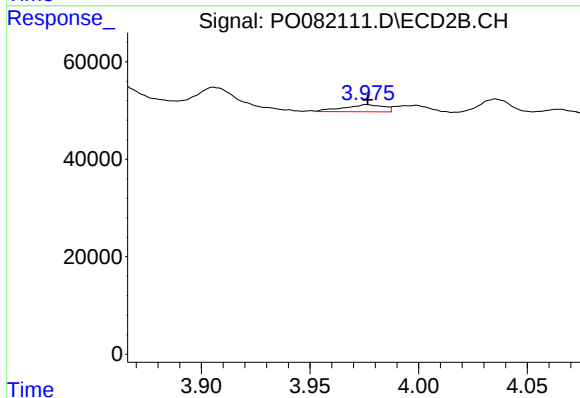


#1 Tetrachloro-m-xylene

R.T.: 3.975 min
Delta R.T.: -0.001 min
Response: 18908
Conc: 0.64 ng/ml m

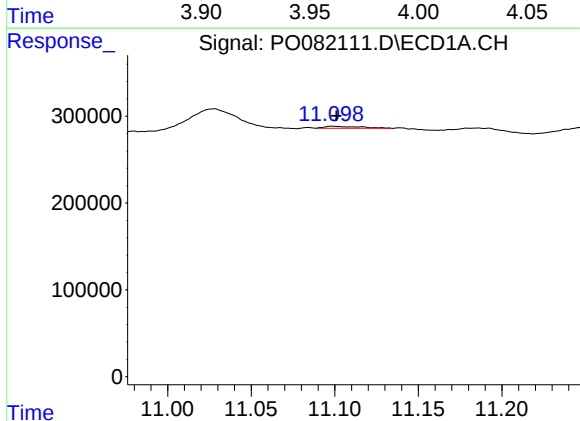

#2 Decachlorobiphenyl

R.T.: 11.099 min
Delta R.T.: -0.002 min
Response: 33010
Conc: 0.59 ng/ml

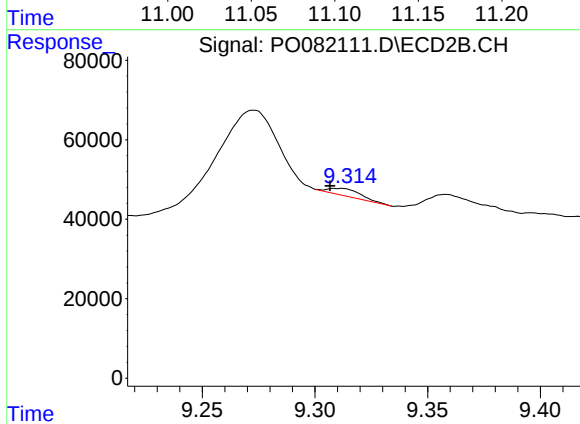

#2 Decachlorobiphenyl

R.T.: 9.314 min
Delta R.T.: 0.008 min
Response: 17881
Conc: 0.70 ng/ml m