

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102320\
 Data File : P0072715.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Oct 2020 13:15
 Operator : DD\AJ
 Sample : PB132575BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB132575BL

Manual Integrations
 APPROVED

mohammad
 10/26/2020 5:06:18 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 04:05:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 14 17:47:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.332	3.507	1975659	998107	23.293m	23.696
2) SA Decachlor...	9.930	8.669	2207456	1110943	20.012	21.490

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102320\
Data File : PO072715.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Oct 2020 13:15
Operator : DD\AJ
Sample : PB132575BL
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB132575BL


Manual Integrations
APPROVED

mohammad
10/26/2020 5:06:18 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 04:05:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 14 17:47:24 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

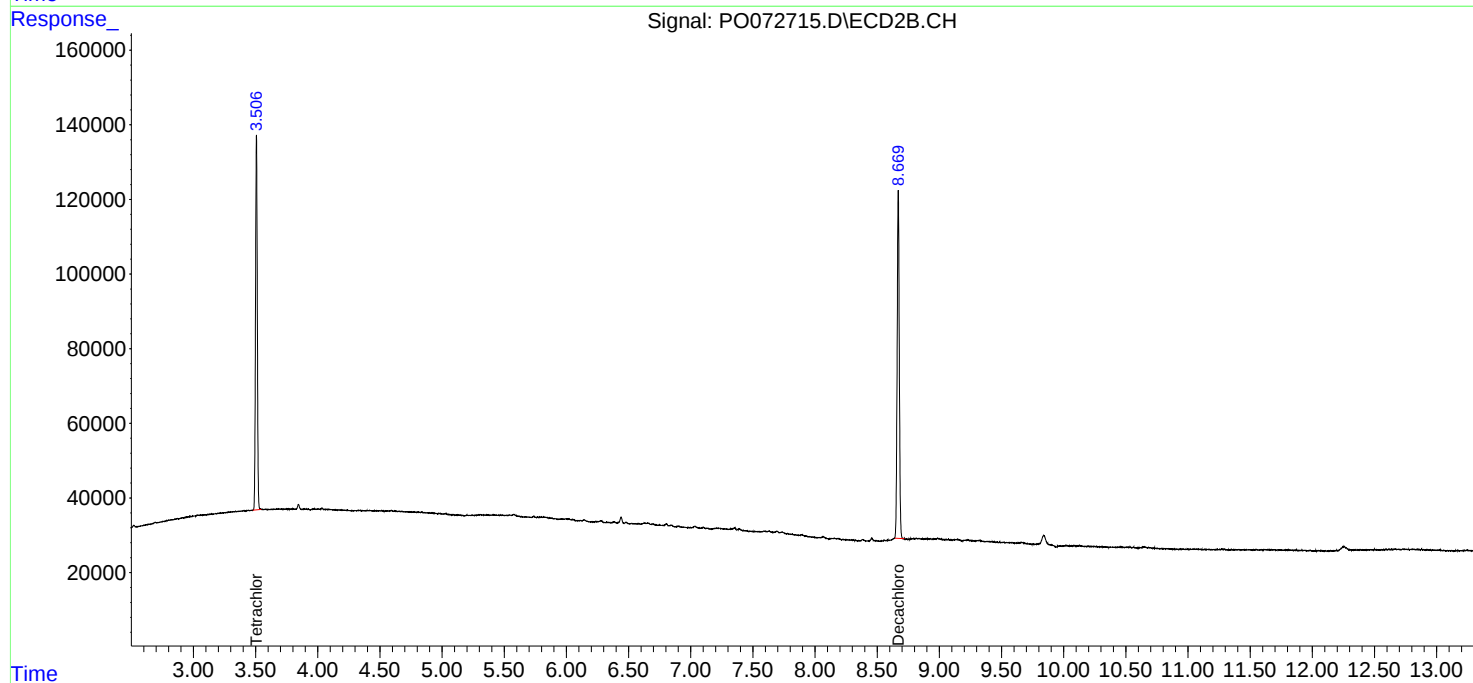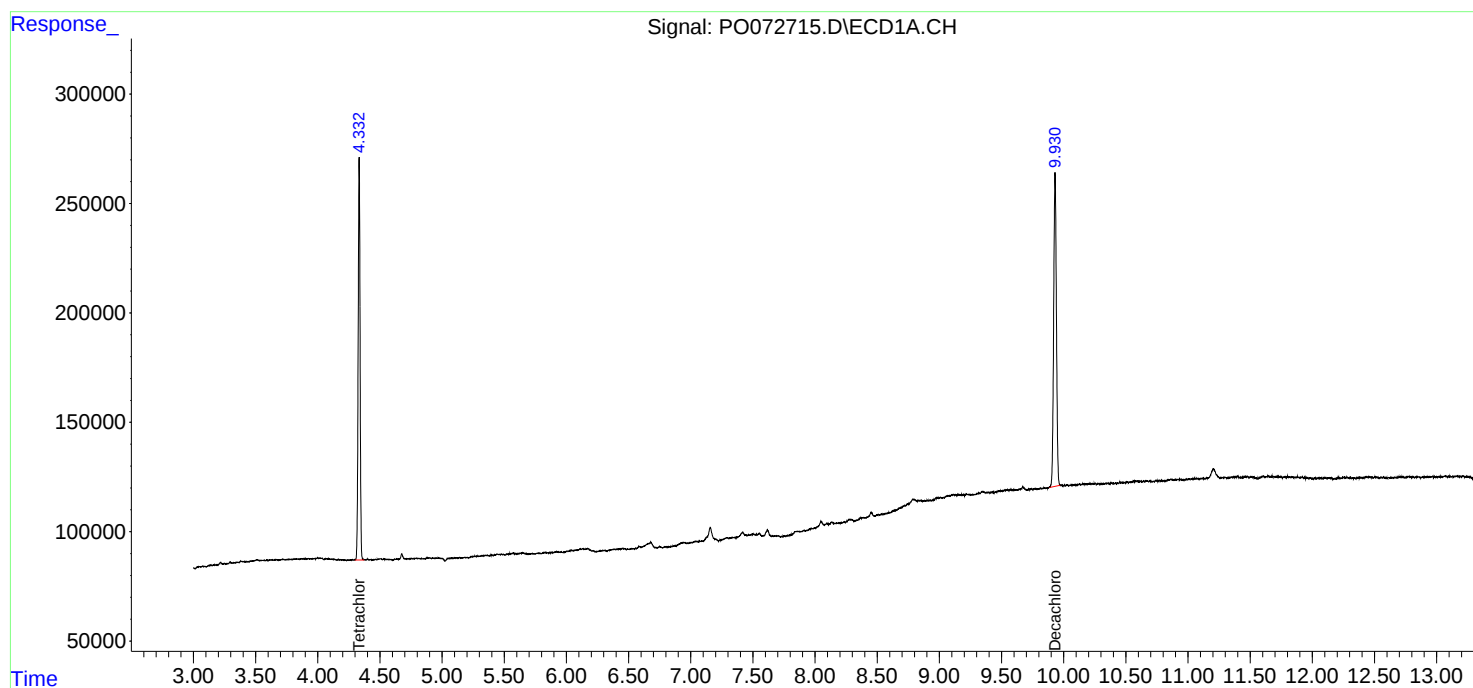

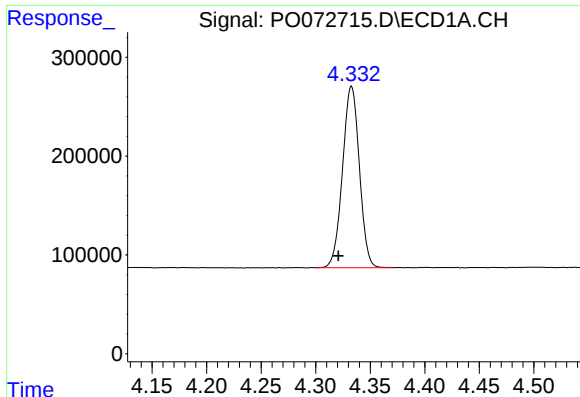


#1 Tetrachloro-m-xylene

R.T.: 4.332 min
Delta R.T.: 0.011 min
Response: 1975659
Conc: 23.29 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PB132575BL


Manual Integrations
APPROVED

mohammad
10/26/2020 5:06:18 PM

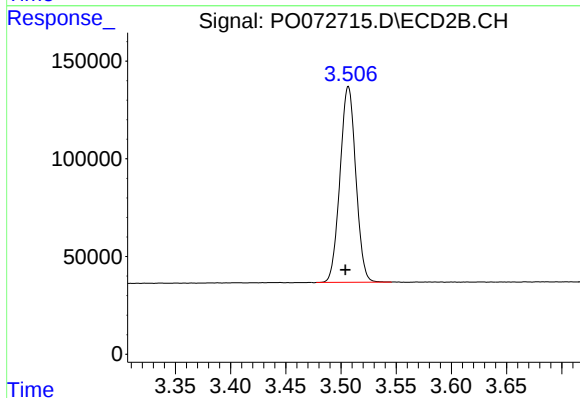


#1 Tetrachloro-m-xylene

R.T.: 3.507 min
Delta R.T.: 0.002 min
Response: 998107
Conc: 23.70 ng/ml

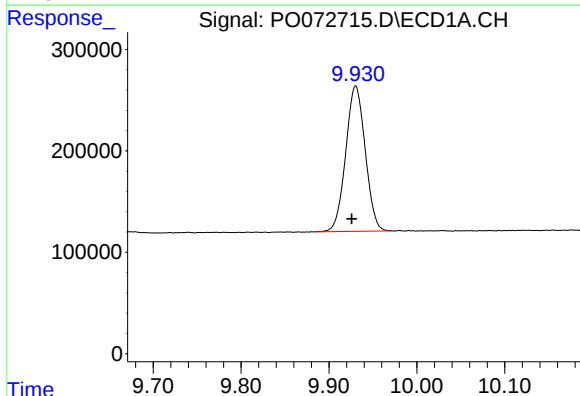

#2 Decachlorobiphenyl

R.T.: 9.930 min
Delta R.T.: 0.004 min
Response: 2207456
Conc: 20.01 ng/ml

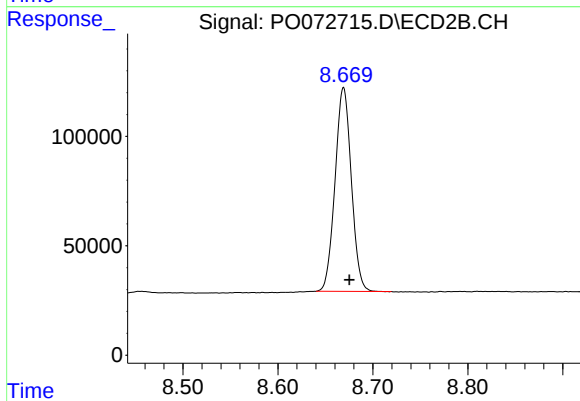

#2 Decachlorobiphenyl

R.T.: 8.669 min
Delta R.T.: -0.006 min
Response: 1110943
Conc: 21.49 ng/ml